

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072118\
 Data File : VV006688.D
 Acq On : 21 Jul 2018 15:58
 Operator : SY/MD
 Sample : J4078-04
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6

Quant Time: Jul 22 23:37:03 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jul 22 23:06:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	225080	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	208639	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	88795	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	68263	4.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.40%
7) Chloroethane-d5	1.58	69	55491	5.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.20%
11) 1,1-Dichloroethene-d2	2.13	63	100997	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	3.95	46	143188	41.74	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.48%
24) Chloroform-d	4.41	84	130812	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.09	65	63218	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
32) Benzene-d6	5.10	84	275981	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.12	67	88384	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.36	98	234490	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
43) trans-1,3-Dichloropropene-	7.67	79	25377	4.26	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.20%
46) 2-Hexanone-d5	8.14	63	137533	46.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.52%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	61236	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	82265	5.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	9823	3.73 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072118\
Data File : VV006688.D
Acq On : 21 Jul 2018 15:58
Operator : SY/MD
Sample : J4078-04
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA6

Quant Time: Jul 22 23:37:03 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jul 22 23:06:02 2018
Response via : Initial Calibration

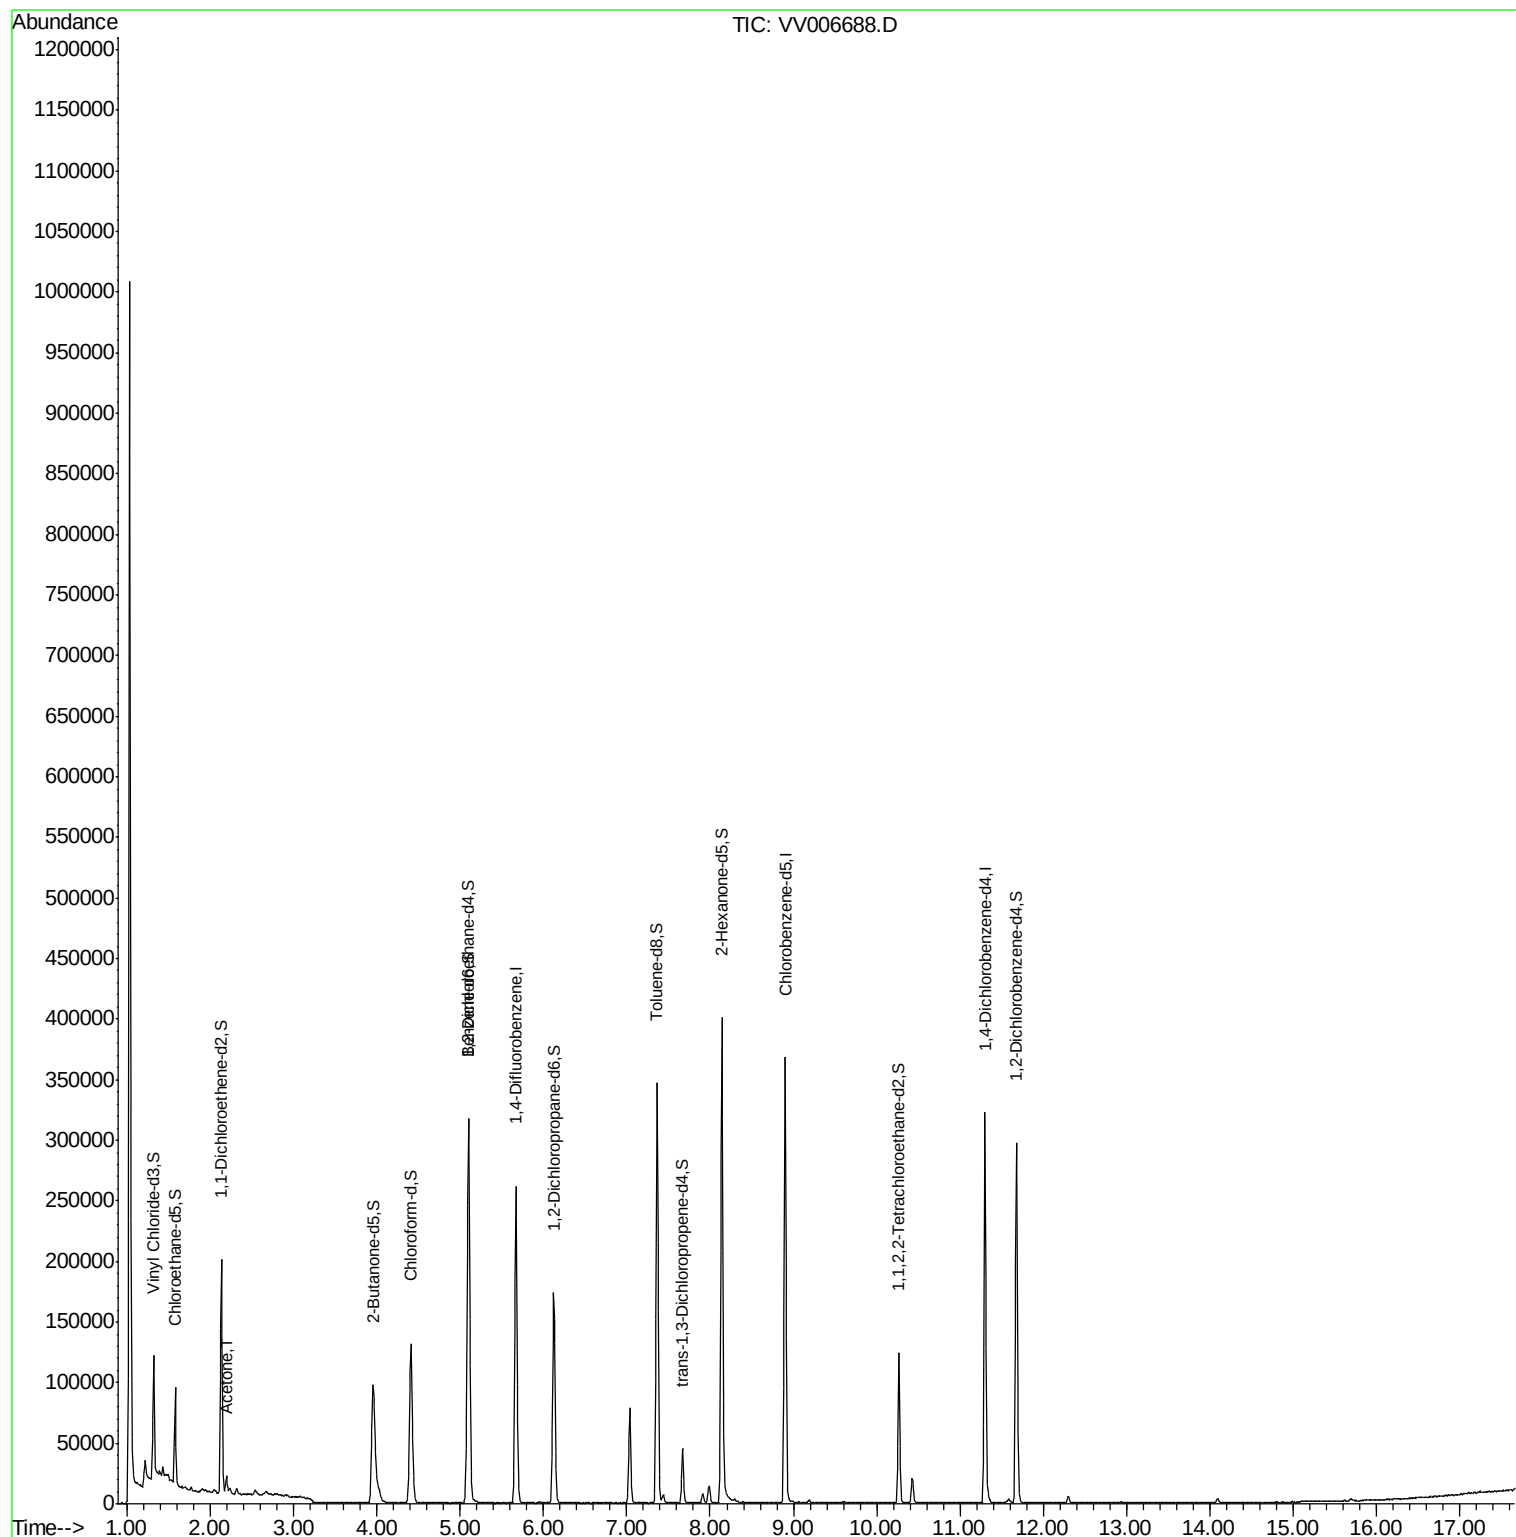

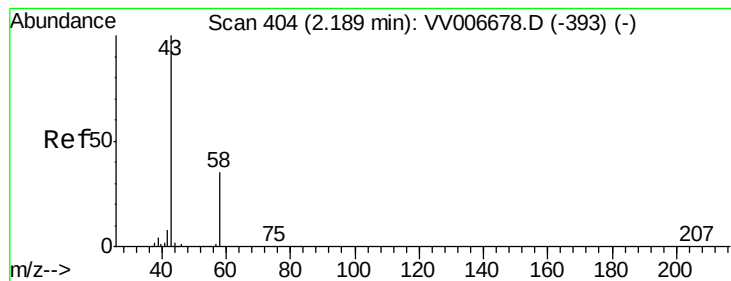

#13

Acetone

Concen: 3.73 ug/L

RT: 2.19 min Scan# 405

Delta R.T. 0.00 min

Lab File: VV006688.D

Acq: 21 Jul 2018 15:58

Instrument :
MSVOA_V
ClientSampleId :
C0AA6

Tot Ion: 43 Resp: 9823

Ion Ratio Lower Upper

43 100

58 37.0 0.0 72.8

