

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072118\
 Data File : VV006689.D
 Acq On : 21 Jul 2018 16:25
 Operator : SY/MD
 Sample : J4078-05
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7

Quant Time: Jul 22 23:38:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jul 22 23:06:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	212409	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	198402	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	83537	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	67426	4.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.40%
7) Chloroethane-d5	1.58	69	53489	5.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.40%
11) 1,1-Dichloroethene-d2	2.13	63	99104	3.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.20%
20) 2-Butanone-d5	3.96	46	64679	19.98	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	39.96%#
24) Chloroform-d	4.41	84	125620	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
26) 1,2-Dichloroethane-d4	5.09	65	61026	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	5.10	84	262786	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.12	67	84514	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.36	98	225044	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.67	79	23908	4.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.40%
46) 2-Hexanone-d5	8.14	63	127591	45.13	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.26%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	58695	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	80004	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	6655	2.68 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072118\
Data File : VV006689.D
Acq On : 21 Jul 2018 16:25
Operator : SY/MD
Sample : J4078-05
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Quant Time: Jul 22 23:38:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jul 22 23:06:02 2018
Response via : Initial Calibration

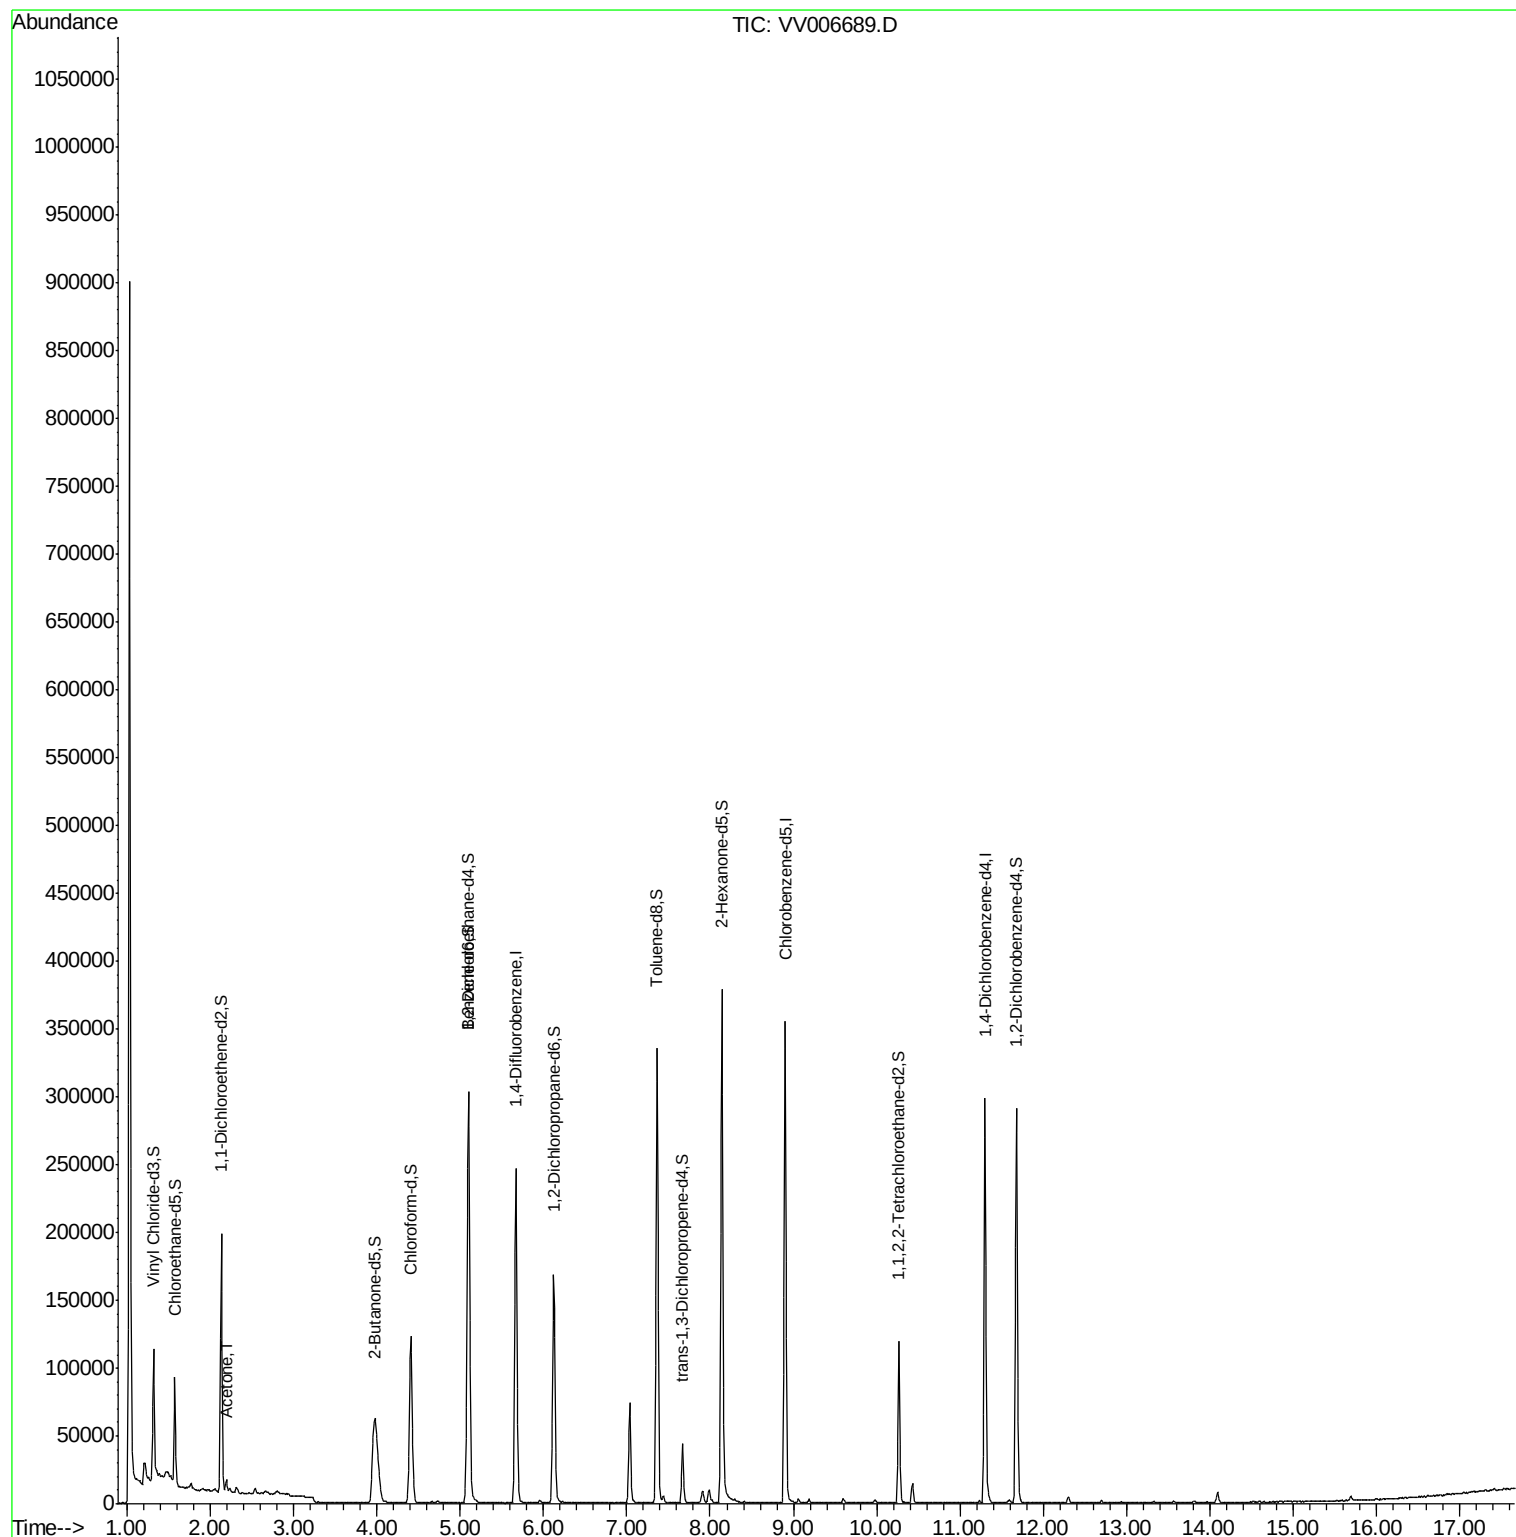

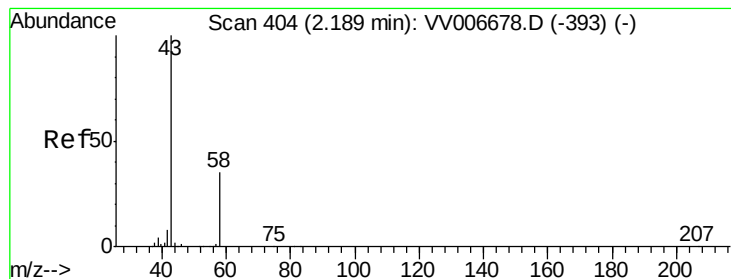

#13

Acetone

Concen: 2.68 ug/L

RT: 2.19 min Scan# 405

Delta R.T. 0.00 min

Lab File: VV006689.D

Acq: 21 Jul 2018 16:25

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Tot Ion: 43 Resp: 6655

Ion Ratio Lower Upper

43 100

58 32.0 0.0 72.8

