
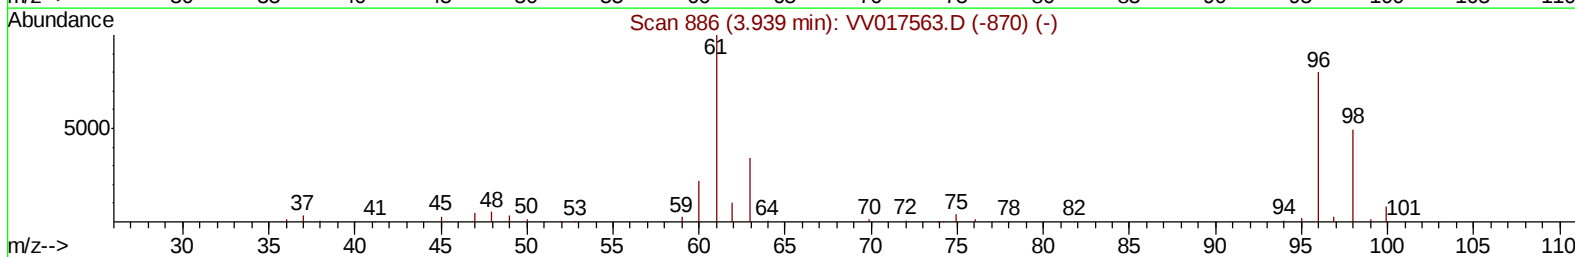
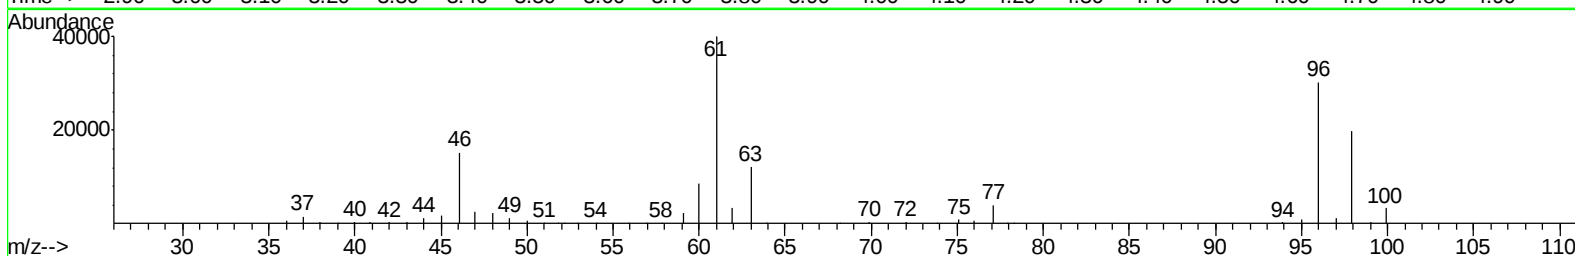


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\  
Data File : VV017576.D  
Acq On : 21 Jul 2020 20:05  
Operator : SY/MD  
Sample : L3336-13  
Misc : 5.0mL/MSVOA V/WATER  
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Jul 22 03:29:31 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM072120WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed Jul 22 03:23:09 2020  
Response via : Initial Calibration

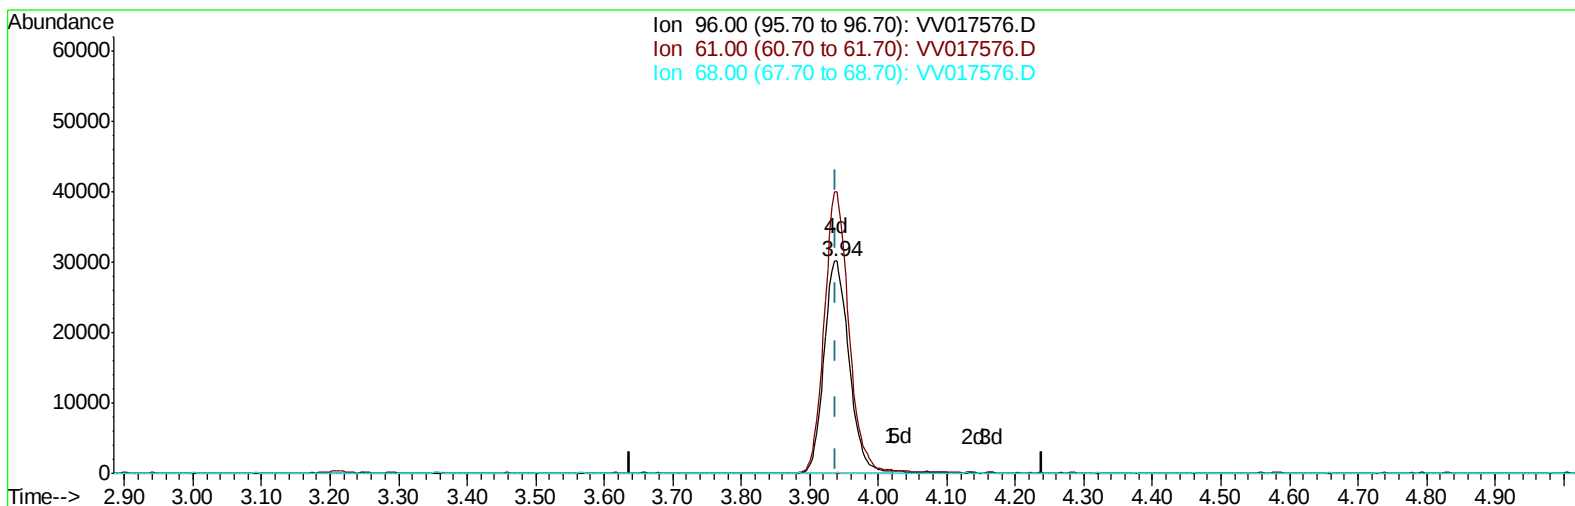

TIC: VV017576.D

(20) cis-1,2-Dichloroethene (T)

3.939min (+0.000) 32.11ug/L m

response 76229

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 96.00 | 100    | 100    |
| 61.00 | 125.50 | 132.51 |
| 68.00 | 0.00   | 0.39#  |
| 0.00  | 0.00   | 0.00   |