


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
Data File : VV017575.D
Acq On : 21 Jul 2020 19:42
Operator : SY/MD
Sample : L3336-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9D

Manual Integrations
APPROVED

MMDadoda
7/22/2020 2:17:44 PM

Quant Time: Jul 22 05:17:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 22 03:23:09 2020
Response via : Initial Calibration

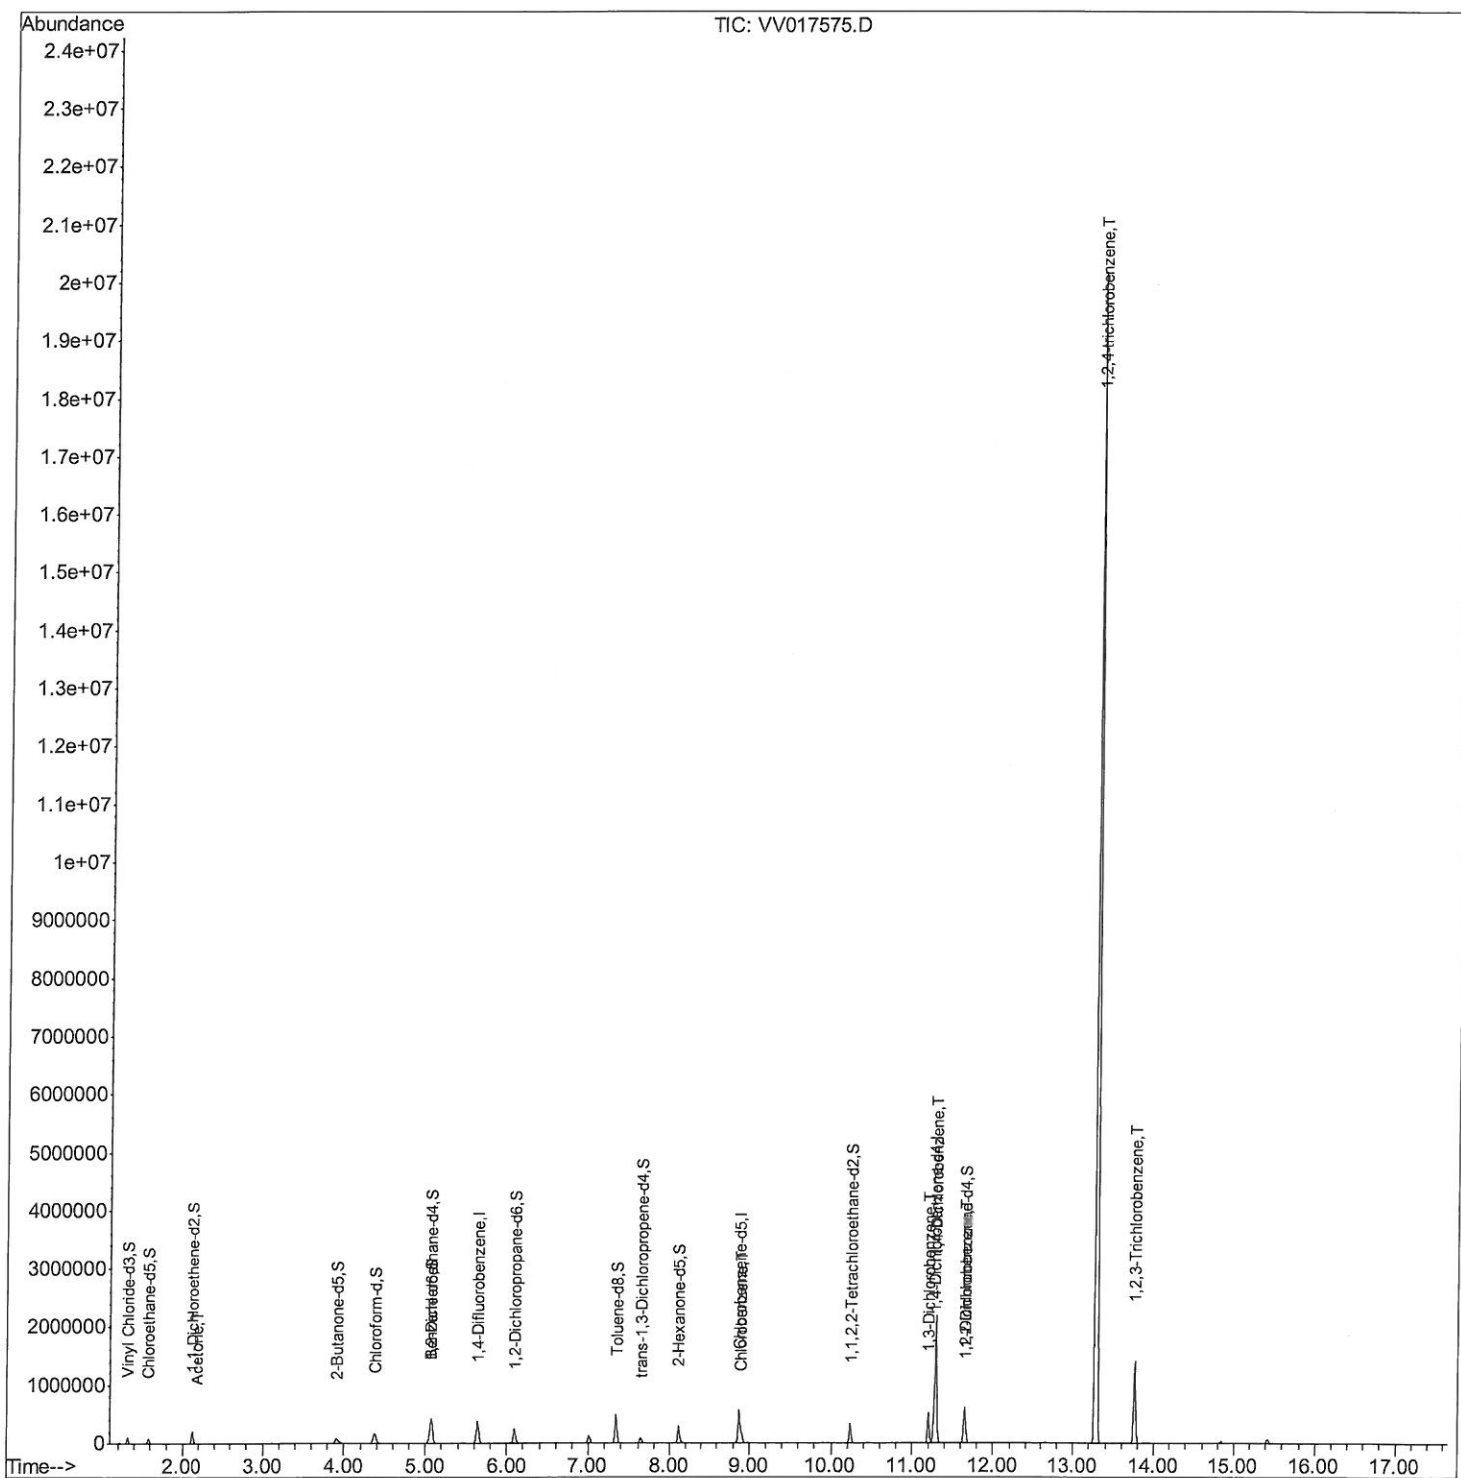

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017575.D
 Acq On : 21 Jul 2020 19:42
 Operator : SY/MD
 Sample : L3336-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9D

Manual Integrations
 APPROVED

MMDadoda
 7/22/2020 2:17:44 PM

Quant Time: Jul 22 03:29:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 22 03:23:09 2020
 Response via : Initial Calibration

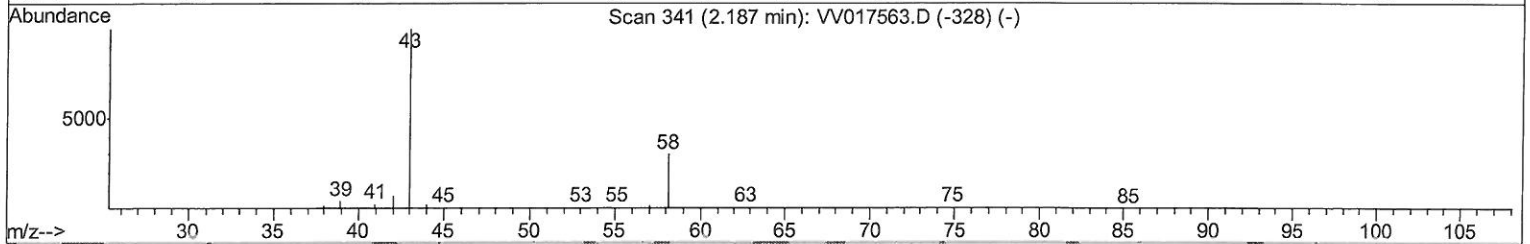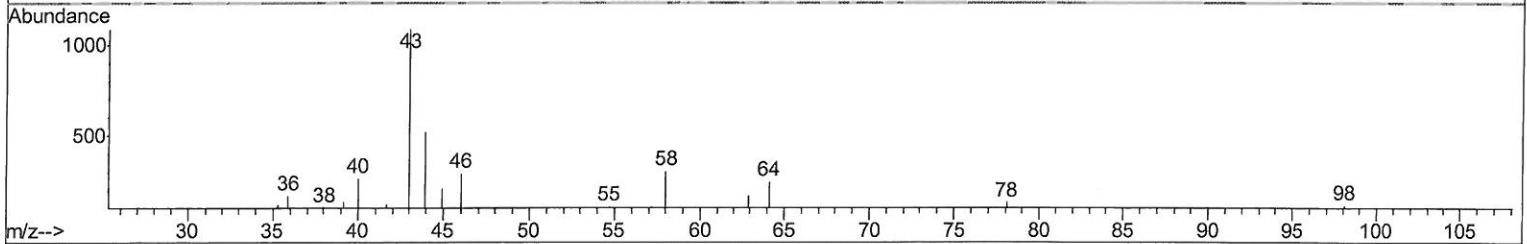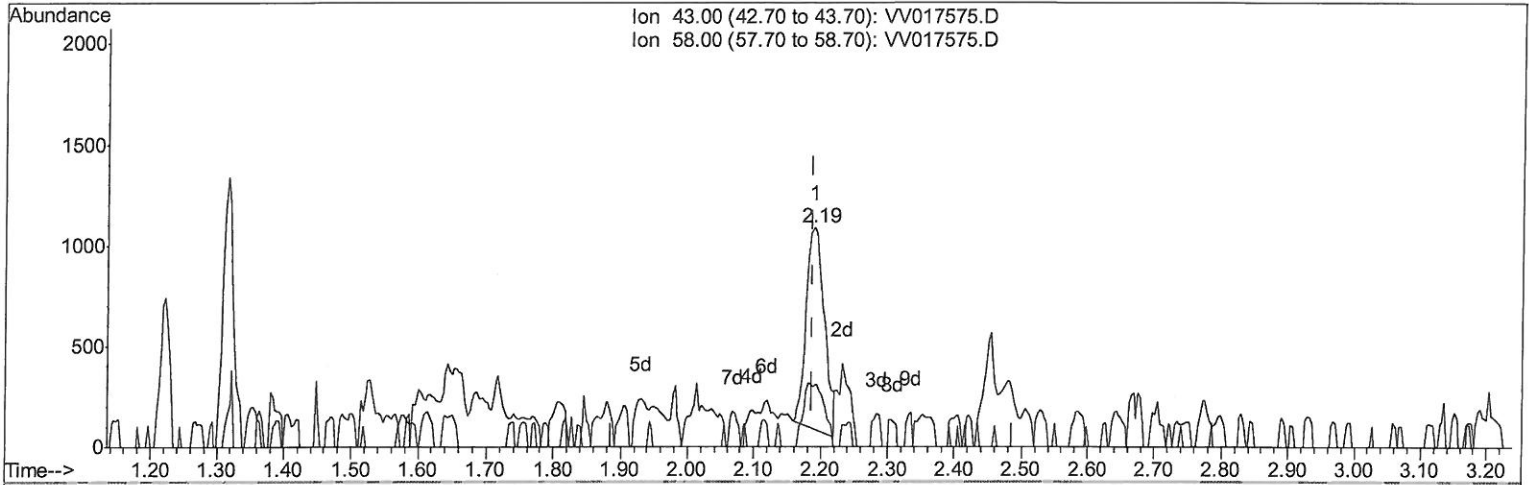

TIC: VV017575.D

(13) Acetone (T)

2.190min (+0.003) 1.48ug/L

response 1925

Ion	Exp%	Act%
43.00	100	100
58.00	29.00	16.31
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017575.D
 Acq On : 21 Jul 2020 19:42
 Operator : SY/MD
 Sample : L3336-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9D

Manual Integrations
 APPROVED

MMDadoda
 7/22/2020 2:17:44 PM

Quant Time: Jul 22 03:29:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 22 03:23:09 2020
 Response via : Initial Calibration

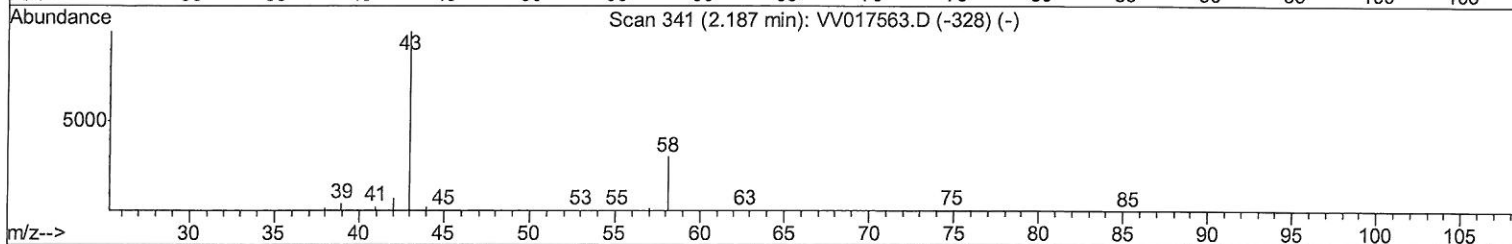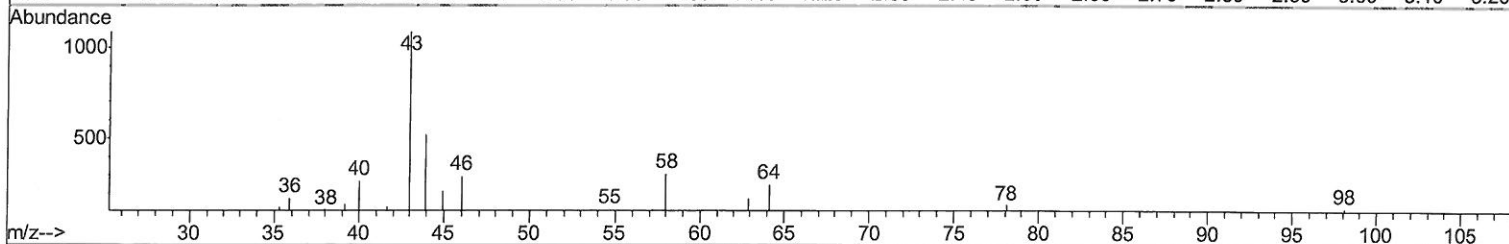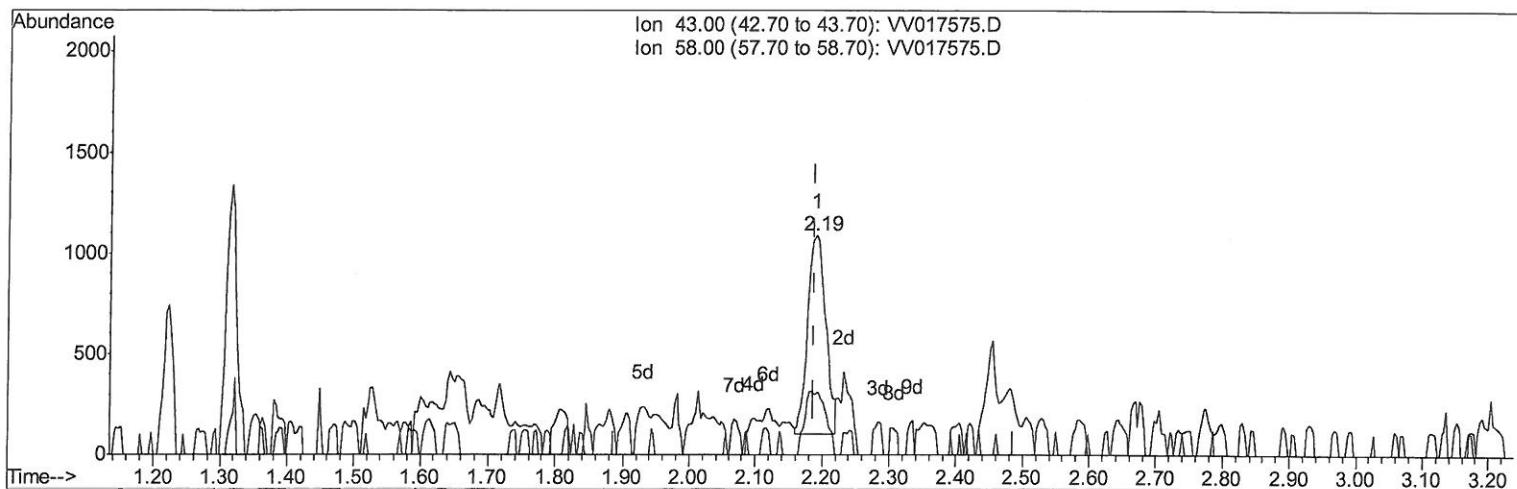

TIC: VV017575.D

(13) Acetone (T)

2.190min (+0.003) 1.44ug/L m

response 1862

Ion	Exp%	Act%
43.00	100	100
58.00	29.00	16.86
0.00	0.00	0.00
0.00	0.00	0.00

MD
 7/24/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017575.D
 Acq On : 21 Jul 2020 19:42
 Operator : SY/MD
 Sample : L3336-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9D

Manual Integrations
 APPROVED

MMDadoda
 7/22/2020 2:17:44 PM

Quant Time: Jul 22 05:17:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 22 03:23:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	307846	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	300121	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	159573	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65820	35.04	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.08%
7) Chloroethane-d5	1.58	69	50229	38.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	77.80%
11) 1,1-Dichloroethene-d2	2.12	63	108801	28.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.56%#
21) 2-Butanone-d5	3.91	46	131736	91.67	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.67%
24) Chloroform-d	4.38	84	184330	42.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.44%
26) 1,2-Dichloroethane-d4	5.06	65	131658	44.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.08%
32) Benzene-d6	5.07	84	337401	42.10	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.20%
36) 1,2-Dichloropropane-d6	6.09	67	105438	43.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.66%
41) Toluene-d8	7.34	98	304332	40.23	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.46%
43) trans-1,3-Dichloropropene-	7.64	79	50889	36.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.08%
47) 2-Hexanone-d5	8.11	63	100318	90.96	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.96%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	153072	44.73	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.46%
64) 1,2-Dichlorobenzene-d4	11.65	152	146889	44.39	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.78%

Target Compounds

					Ovalue
13) Acetone	2.19	43	1862m	1.436	ug/L
51) Chlorobenzene	8.90	112	91063	14.154	ug/L
62) 1,3-Dichlorobenzene	11.20	146	208542	38.922	ug/L
63) 1,4-Dichlorobenzene	11.29	146	830203	151.808	ug/L
65) 1,2-Dichlorobenzene	11.67	146	40079	7.378	ug/L
68) 1,2,4-trichlorobenzene	13.29	180	5806944	1547.847	ug/L
70) 1,2,3-Trichlorobenzene	13.77	180	412877	110.022	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed