

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017567.D
 Acq On : 21 Jul 2020 16:33
 Operator : SY/MD
 Sample : VV0721WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	164517	170350	12.53%	1.643%
2	1.576	144	151	160	rBV	120001	135432	9.96%	1.306%
3	2.119	310	320	348	rVB	287231	444911	32.73%	4.292%
4	2.843	543	545	548	rBV2	1062	547	0.04%	0.005%
5	3.081	617	619	621	rBV3	679	440	0.03%	0.004%
6	3.296	682	686	689	rBV4	747	659	0.05%	0.006%
7	3.341	698	700	705	rVB4	1049	865	0.06%	0.008%
8	3.370	705	709	712	rBV3	939	668	0.05%	0.006%
9	3.438	727	730	732	rBV3	929	601	0.04%	0.006%
10	3.502	746	750	753	rBV4	977	708	0.05%	0.007%
11	3.653	793	797	799	rVV3	642	450	0.03%	0.004%
12	3.846	851	857	860	rBV4	813	748	0.06%	0.007%
13	3.907	865	876	906	rBV	98216	288057	21.19%	2.779%
14	4.315	1000	1003	1005	rBV2	1044	515	0.04%	0.005%
15	4.376	1005	1022	1046	rVV	223906	555372	40.85%	5.357%
16	4.511	1062	1064	1068	rVB2	968	540	0.04%	0.005%
17	4.598	1088	1091	1094	rVB6	1016	550	0.04%	0.005%
18	4.624	1097	1099	1102	rBV3	752	447	0.03%	0.004%
19	4.846	1160	1168	1169	rBV4	1696	1608	0.12%	0.016%
20	4.991	1209	1213	1215	rBV	782	545	0.04%	0.005%
21	5.071	1220	1238	1262	rBV2	527302	1359431	100.00%	13.114%
22	5.421	1344	1347	1349	rBV3	920	543	0.04%	0.005%
23	5.495	1366	1370	1373	rBV3	1252	919	0.07%	0.009%
24	5.640	1402	1415	1439	rBV	394808	788833	58.03%	7.609%
25	5.823	1470	1472	1476	rVB4	1790	1144	0.08%	0.011%
26	5.933	1496	1506	1507	rBV10	5808	7597	0.56%	0.073%
27	6.045	1536	1541	1542	rBV3	1051	845	0.06%	0.008%
28	6.093	1543	1556	1580	rVV	301351	610214	44.89%	5.886%
29	6.299	1618	1620	1623	rBV2	881	582	0.04%	0.006%
30	6.380	1637	1645	1648	rBV7	964	1344	0.10%	0.013%
31	6.502	1679	1683	1686	rBV4	1030	897	0.07%	0.009%
32	6.621	1718	1720	1726	rVB7	1191	834	0.06%	0.008%
33	6.653	1726	1730	1733	rBV5	1292	1148	0.08%	0.011%
34	6.804	1775	1777	1779	rBV3	969	527	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017567.D
 Acq On : 21 Jul 2020 16:33
 Operator : SY/MD
 Sample : VV0721WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

35	6.939	1816	1819	1823	rVB3	1174	900	0.07%	0.009%
36	7.007	1828	1840	1865	rVV	183137	334642	24.62%	3.228%
37	7.338	1931	1943	1963	rBV	647147	1091685	80.30%	10.531%
38	7.556	2008	2011	2015	rBV4	1440	1362	0.10%	0.013%
39	7.640	2027	2037	2057	rBV	130511	229497	16.88%	2.214%
40	7.804	2086	2088	2091	rBV2	833	622	0.05%	0.006%
41	7.849	2100	2102	2105	rBV3	782	682	0.05%	0.007%
42	8.039	2159	2161	2165	rVB4	1290	848	0.06%	0.008%
43	8.068	2167	2170	2172	rBV3	1017	641	0.05%	0.006%
44	8.106	2172	2182	2210	rBV	340370	613717	45.15%	5.920%
45	8.740	2377	2379	2382	rVV2	782	450	0.03%	0.004%
46	8.871	2408	2420	2448	rBV	597366	960872	70.68%	9.269%
47	9.039	2467	2472	2473	rBV4	2591	2058	0.15%	0.020%
48	9.090	2485	2488	2490	rBV2	1204	677	0.05%	0.007%
49	9.119	2494	2497	2502	rBV3	801	536	0.04%	0.005%
50	9.158	2506	2509	2510	rBV	1962	1107	0.08%	0.011%
51	9.209	2523	2525	2528	rVB3	1029	570	0.04%	0.005%
52	9.289	2546	2550	2553	rBV3	1073	677	0.05%	0.007%
53	9.309	2553	2556	2558	rBV2	666	498	0.04%	0.005%
54	9.334	2562	2564	2569	rBV4	752	740	0.05%	0.007%
55	9.395	2578	2583	2588	rVB5	1111	1001	0.07%	0.010%
56	9.428	2588	2593	2595	rBV4	609	555	0.04%	0.005%
57	9.588	2632	2643	2647	rBV9	3285	5478	0.40%	0.053%
58	9.749	2691	2693	2699	rVB3	878	843	0.06%	0.008%
59	9.894	2735	2738	2740	rBV3	604	515	0.04%	0.005%
60	9.955	2750	2757	2761	rBV6	2969	3727	0.27%	0.036%
61	10.032	2778	2781	2783	rBV2	627	467	0.03%	0.005%
62	10.074	2791	2794	2799	rBV3	625	598	0.04%	0.006%
63	10.109	2802	2805	2810	rBV6	726	739	0.05%	0.007%
64	10.167	2821	2823	2827	rVB2	1112	727	0.05%	0.007%
65	10.193	2829	2831	2833	rBV2	1313	719	0.05%	0.007%
66	10.238	2833	2845	2867	rVV	428066	662555	48.74%	6.391%
67	10.347	2876	2879	2883	rBV4	992	691	0.05%	0.007%
68	10.804	3019	3021	3023	rBV2	914	442	0.03%	0.004%
69	10.865	3037	3040	3042	rVV3	1064	661	0.05%	0.006%
70	10.881	3042	3045	3048	rVB4	1035	758	0.06%	0.007%
71	10.939	3056	3063	3070	rBV6	2821	4215	0.31%	0.041%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017567.D
 Acq On : 21 Jul 2020 16:33
 Operator : SY/MD
 Sample : VV0721WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

72	11.064	3100	3102	3104	rVB3	1194	534	0.04%	0.005%
73	11.122	3117	3120	3123	rVB3	1040	744	0.05%	0.007%
74	11.209	3140	3147	3154	rBV8	4401	6325	0.47%	0.061%
75	11.270	3154	3166	3187	rVV	613856	938100	69.01%	9.049%
76	11.386	3200	3202	3207	rBV4	1022	789	0.06%	0.008%
77	11.437	3216	3218	3221	rVB2	933	516	0.04%	0.005%
78	11.521	3239	3244	3248	rBV2	1223	970	0.07%	0.009%
79	11.592	3264	3266	3270	rBV	1042	770	0.06%	0.007%
80	11.646	3270	3283	3302	rBV	689470	1069705	78.69%	10.319%
81	11.778	3320	3324	3326	rBV2	1415	1075	0.08%	0.010%
82	11.878	3351	3355	3361	rBV5	983	1113	0.08%	0.011%
83	11.958	3377	3380	3383	rBV4	930	691	0.05%	0.007%
84	12.347	3497	3501	3504	rBV3	587	500	0.04%	0.005%
85	12.669	3596	3601	3613	rVB9	4476	6749	0.50%	0.065%
86	12.984	3693	3699	3702	rBV7	1134	940	0.07%	0.009%
87	13.225	3771	3774	3778	rVB3	659	540	0.04%	0.005%
88	13.254	3778	3783	3786	rBV4	1189	1072	0.08%	0.010%
89	13.289	3786	3794	3803	rVV9	5447	9130	0.67%	0.088%
90	13.434	3837	3839	3842	rVB2	1117	488	0.04%	0.005%
91	13.460	3844	3847	3850	rBV2	912	820	0.06%	0.008%
92	13.537	3864	3871	3883	rVB7	3529	6007	0.44%	0.058%
93	13.591	3886	3888	3889	rBV2	1075	477	0.04%	0.005%
94	13.624	3894	3898	3902	rBV4	1062	772	0.06%	0.007%
95	13.669	3908	3912	3915	rBV4	677	760	0.06%	0.007%
96	13.775	3938	3945	3955	rVB10	4768	8045	0.59%	0.078%
97	14.051	4028	4031	4033	rBV	871	474	0.03%	0.005%
98	14.257	4093	4095	4098	rBV2	958	467	0.03%	0.005%
99	14.881	4287	4289	4290	rBV	854	478	0.04%	0.005%
100	14.958	4310	4313	4319	rBV7	1099	1136	0.08%	0.011%


Sum of corrected areas: 10366530

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072120\
Data File : VV017567.D
Acq On : 21 Jul 2020 16:33
Operator : SY/MD
Sample : VV0721WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

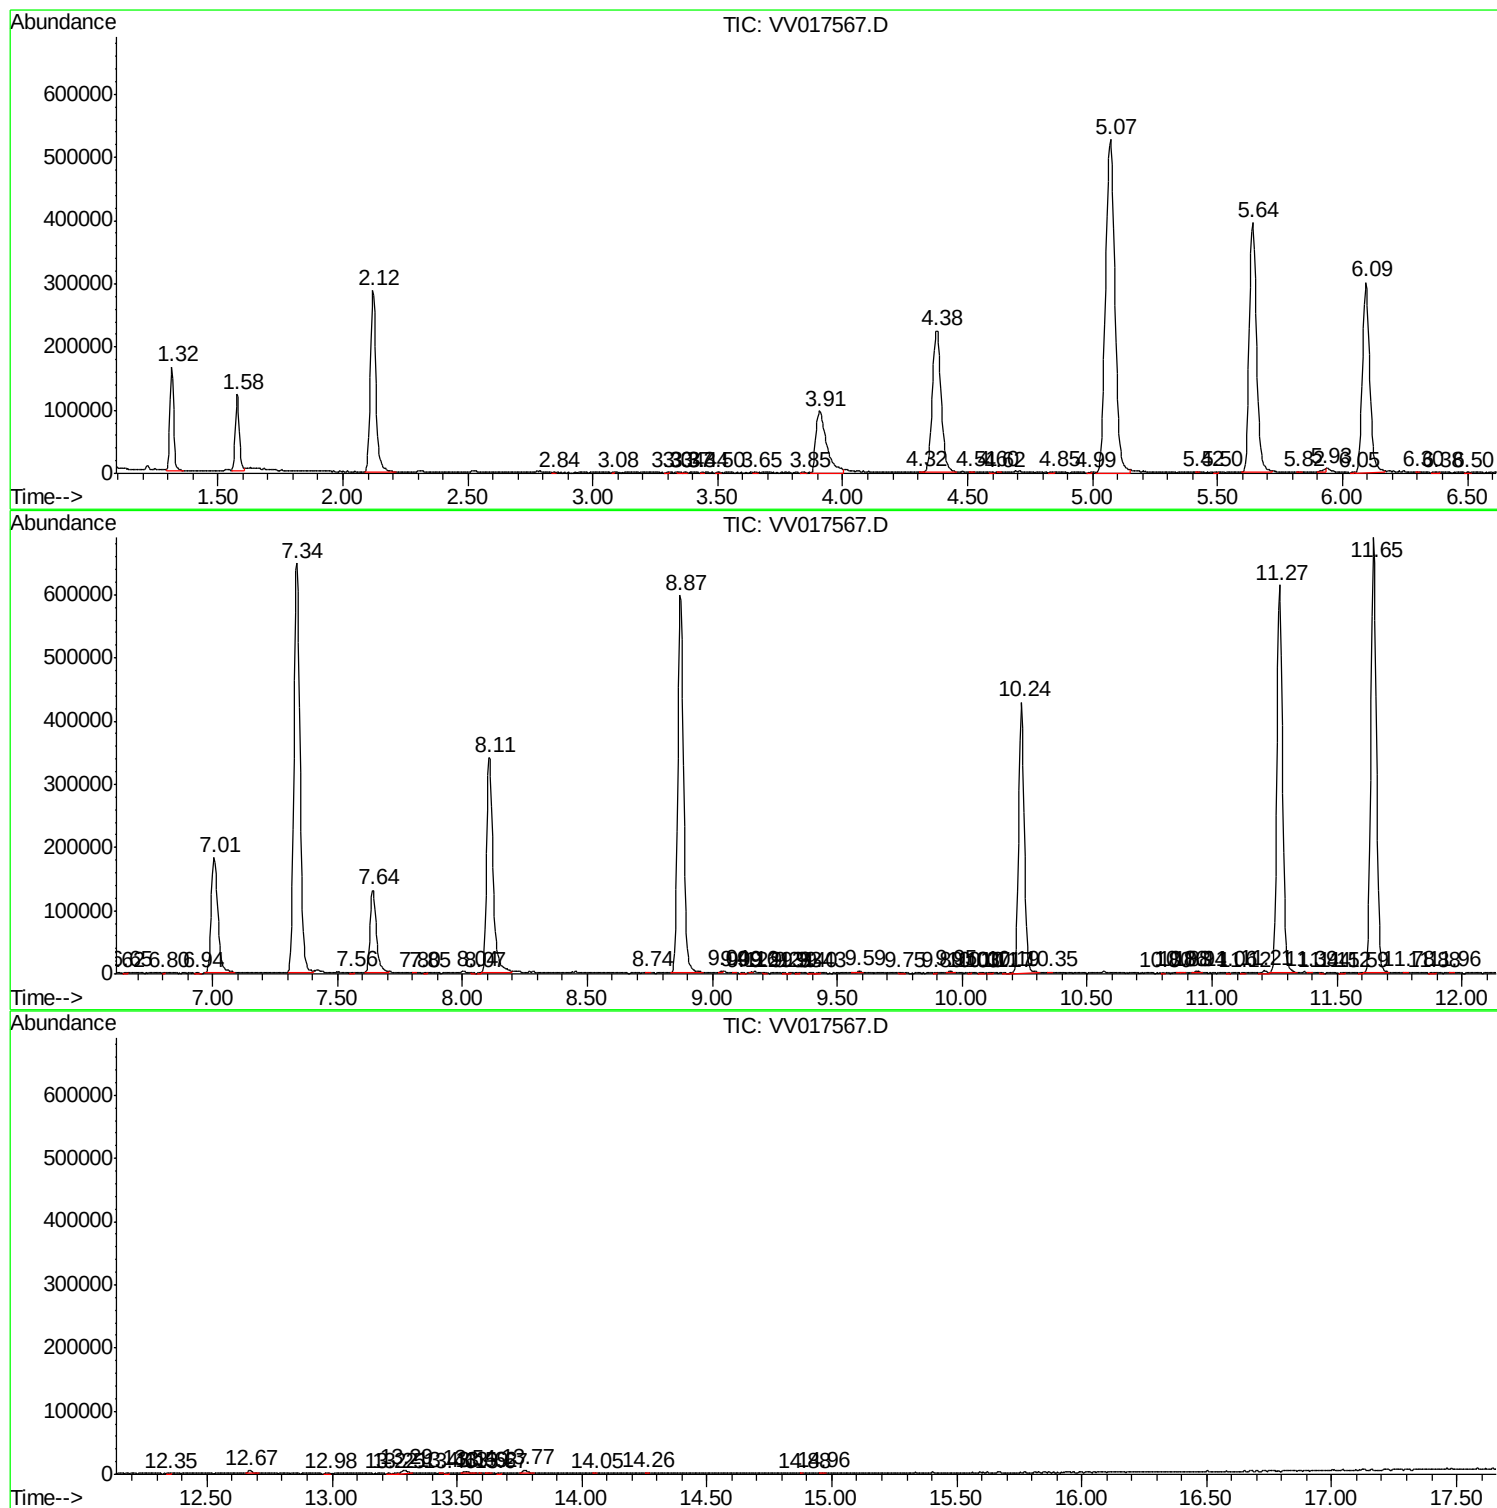

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017567.D
Acq On : 21 Jul 2020 16:33
Operator : SY/MD
Sample : VV0721WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV072120\
Data File : VV017567.D
Acq On : 21 Jul 2020 16:33
Operator : SY/MD
Sample : VV0721WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc