

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017568.D
 Acq On : 21 Jul 2020 16:59
 Operator : SY/MD
 Sample : L3336-04DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	117696	119787	11.05%	1.262%
2	1.576	145	151	162	rBV	92614	103740	9.57%	1.093%
3	2.122	310	321	341	rBV3	248527	413406	38.15%	4.356%
4	2.392	402	405	407	rVB2	626	387	0.04%	0.004%
5	2.566	458	459	461	rBV	762	388	0.04%	0.004%
6	3.019	597	600	604	rVB3	971	592	0.05%	0.006%
7	3.077	614	618	621	rBV5	1124	939	0.09%	0.010%
8	3.142	636	638	641	rVB2	823	373	0.03%	0.004%
9	3.158	641	643	644	rBV	1025	442	0.04%	0.005%
10	3.209	644	659	680	rVV	277785	590333	54.47%	6.220%
11	3.460	732	737	738	rBV3	696	565	0.05%	0.006%
12	3.624	785	788	790	rVB3	787	457	0.04%	0.005%
13	3.698	809	811	812	rBV	836	395	0.04%	0.004%
14	3.814	844	847	851	rVB4	936	749	0.07%	0.008%
15	3.839	851	855	857	rBV2	1038	782	0.07%	0.008%
16	3.913	865	878	880	rBV	94262	165178	15.24%	1.740%
17	4.293	994	996	997	rBV2	758	387	0.04%	0.004%
18	4.376	1006	1022	1042	rVV2	186161	453325	41.83%	4.776%
19	4.608	1089	1094	1095	rBV3	971	765	0.07%	0.008%
20	4.701	1117	1123	1124	rBV4	1135	809	0.07%	0.009%
21	4.749	1136	1138	1141	rBV3	888	452	0.04%	0.005%
22	4.830	1158	1163	1166	rBV5	837	787	0.07%	0.008%
23	4.907	1184	1187	1188	rBV2	1019	488	0.05%	0.005%
24	5.071	1216	1238	1262	rBV2	414079	1083734	100.00%	11.418%
25	5.305	1307	1311	1312	rBV4	824	539	0.05%	0.006%
26	5.370	1329	1331	1334	rVB2	1273	568	0.05%	0.006%
27	5.392	1334	1338	1343	rBV6	1058	1087	0.10%	0.011%
28	5.511	1372	1375	1378	rBV4	1073	747	0.07%	0.008%
29	5.592	1398	1400	1401	rBV2	753	326	0.03%	0.003%
30	5.640	1403	1415	1440	rVV	391913	782034	72.16%	8.239%
31	5.936	1494	1507	1529	rBV	102954	211019	19.47%	2.223%
32	6.093	1543	1556	1575	rBV	239182	486533	44.89%	5.126%
33	6.405	1651	1653	1657	rVB3	1428	1016	0.09%	0.011%
34	6.431	1657	1661	1662	rBV2	919	669	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017568.D
 Acq On : 21 Jul 2020 16:59
 Operator : SY/MD
 Sample : L3336-04DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

35	6.476	1673	1675	1678	rBV3	1054	667	0.06%	0.007%
36	6.592	1710	1711	1714	rBV2	457	333	0.03%	0.004%
37	6.752	1757	1761	1763	rBV3	803	577	0.05%	0.006%
38	6.894	1803	1805	1808	rVB3	523	311	0.03%	0.003%
39	6.939	1817	1819	1820	rBV	665	299	0.03%	0.003%
40	7.006	1830	1840	1860	rBV	130979	240919	22.23%	2.538%
41	7.164	1886	1889	1891	rBV3	979	776	0.07%	0.008%
42	7.276	1922	1924	1926	rVB2	1260	519	0.05%	0.005%
43	7.334	1930	1942	1968	rBV	488038	851144	78.54%	8.967%
44	7.640	2026	2037	2060	rBV	95679	173467	16.01%	1.828%
45	7.775	2076	2079	2080	rBV3	879	373	0.03%	0.004%
46	7.903	2115	2119	2121	rBV4	997	703	0.06%	0.007%
47	7.955	2132	2135	2139	rVB2	1077	698	0.06%	0.007%
48	7.993	2142	2147	2151	rBV5	1010	1190	0.11%	0.013%
49	8.071	2169	2171	2172	rBV2	699	323	0.03%	0.003%
50	8.106	2172	2182	2209	rVV	278338	500085	46.14%	5.269%
51	8.318	2246	2248	2250	rBV2	776	447	0.04%	0.005%
52	8.498	2301	2304	2306	rBV2	888	402	0.04%	0.004%
53	8.553	2318	2321	2324	rVB5	711	469	0.04%	0.005%
54	8.685	2358	2362	2363	rBV3	908	662	0.06%	0.007%
55	8.791	2392	2395	2396	rBV3	753	315	0.03%	0.003%
56	8.871	2408	2420	2443	rBV	592470	967713	89.29%	10.196%
57	9.161	2506	2510	2514	rBV5	1391	1423	0.13%	0.015%
58	9.238	2533	2534	2537	rBV2	829	434	0.04%	0.005%
59	9.273	2542	2545	2547	rVB3	1120	634	0.06%	0.007%
60	9.424	2587	2592	2594	rBV3	732	506	0.05%	0.005%
61	9.444	2594	2598	2600	rVB3	934	494	0.05%	0.005%
62	9.469	2604	2606	2608	rBV2	595	368	0.03%	0.004%
63	9.563	2632	2635	2636	rBV3	1001	588	0.05%	0.006%
64	9.710	2678	2681	2682	rBV	632	399	0.04%	0.004%
65	9.871	2729	2731	2734	rVB2	942	445	0.04%	0.005%
66	9.955	2754	2757	2760	rBV4	841	563	0.05%	0.006%
67	10.013	2771	2775	2777	rVB3	898	706	0.07%	0.007%
68	10.096	2797	2801	2803	rBV5	788	736	0.07%	0.008%
69	10.141	2813	2815	2817	rBV2	751	406	0.04%	0.004%
70	10.238	2832	2845	2860	rBV	337848	527513	48.68%	5.558%
71	10.370	2885	2886	2889	rBV3	523	301	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017568.D
 Acq On : 21 Jul 2020 16:59
 Operator : SY/MD
 Sample : L3336-04DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

72	10.469	2912	2917	2920	rBV5	1361	1234	0.11%	0.013%
73	10.498	2923	2926	2928	rBV	672	362	0.03%	0.004%
74	10.881	3035	3045	3046	rBV7	2487	2886	0.27%	0.030%
75	11.003	3078	3083	3090	rVB8	764	782	0.07%	0.008%
76	11.270	3155	3166	3189	rVB	601006	924858	85.34%	9.744%
77	11.460	3223	3225	3227	rBV3	1135	477	0.04%	0.005%
78	11.501	3236	3238	3240	rBV3	671	305	0.03%	0.003%
79	11.646	3269	3283	3299	rBV	540726	846155	78.08%	8.915%
80	12.077	3415	3417	3423	rBV4	388	409	0.04%	0.004%
81	12.116	3423	3429	3431	rBV6	724	836	0.08%	0.009%
82	12.183	3447	3450	3454	rBV3	484	312	0.03%	0.003%
83	12.263	3473	3475	3478	rVB2	883	388	0.04%	0.004%
84	12.292	3481	3484	3486	rBV2	609	411	0.04%	0.004%
85	12.357	3501	3504	3507	rBV3	1071	748	0.07%	0.008%
86	12.443	3529	3531	3534	rVB	1151	653	0.06%	0.007%
87	12.460	3534	3536	3539	rBV3	679	462	0.04%	0.005%
88	12.527	3554	3557	3559	rBV2	825	460	0.04%	0.005%
89	12.797	3637	3641	3646	rBV3	652	678	0.06%	0.007%
90	13.231	3774	3776	3779	rVB2	844	396	0.04%	0.004%
91	13.369	3816	3819	3821	rBV3	1066	811	0.07%	0.009%
92	13.447	3839	3843	3846	rBV3	1118	812	0.07%	0.009%
93	13.530	3866	3869	3872	rBV3	2000	1722	0.16%	0.018%
94	13.611	3889	3894	3896	rBV2	1001	780	0.07%	0.008%
95	13.662	3907	3910	3911	rBV	905	445	0.04%	0.005%
96	13.942	3995	3997	3999	rBV3	679	318	0.03%	0.003%
97	14.373	4129	4131	4132	rBV2	1066	449	0.04%	0.005%
98	14.575	4191	4194	4195	rBV2	839	421	0.04%	0.004%
99	15.029	4332	4335	4336	rBV2	907	531	0.05%	0.006%
100	15.119	4359	4363	4364	rBV3	1175	729	0.07%	0.008%


Sum of corrected areas: 9491536

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072120\
Data File : VV017568.D
Acq On : 21 Jul 2020 16:59
Operator : SY/MD
Sample : L3336-04DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
PMW-2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

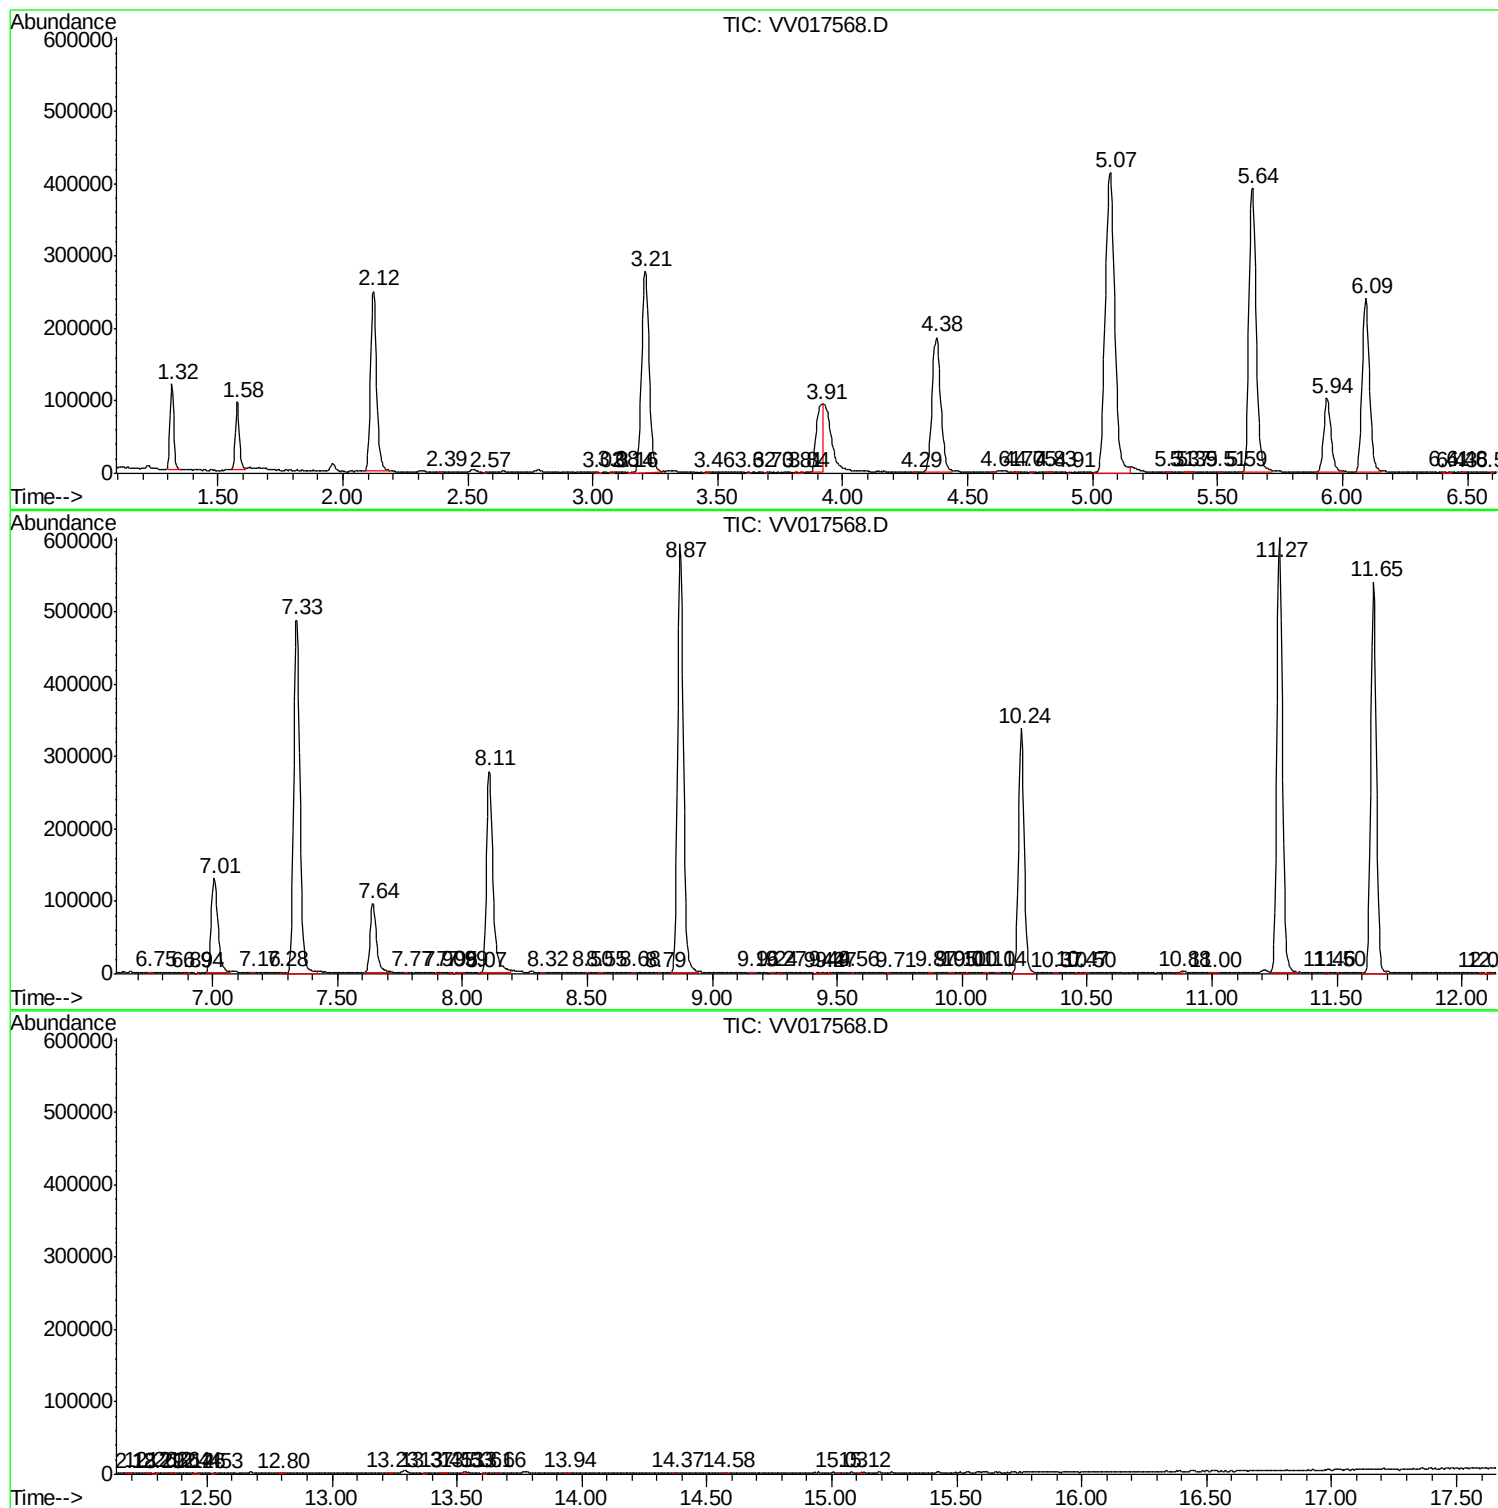

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV072120\
Data File : VV017568.D
Acq On : 21 Jul 2020 16:59
Operator : SY/MD
Sample : L3336-04DL 20X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
PMW-2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV072120\
Data File : VV017568.D
Acq On : 21 Jul 2020 16:59
Operator : SY/MD
Sample : L3336-04DL 20X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
PMW-2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc