

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017570.D
 Acq On : 21 Jul 2020 17:46
 Operator : SY/MD
 Sample : L3336-22DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DUP(071520)DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	116677	117787	4.69%	0.995%
2	1.576	145	151	161	rBV	91871	101693	4.05%	0.859%
3	2.119	310	320	349	rBV	213232	330772	13.18%	2.793%
4	2.405	407	409	414	rBV4	852	618	0.02%	0.005%
5	2.585	459	465	467	rBV6	840	774	0.03%	0.007%
6	2.778	522	525	529	rBV4	1308	1049	0.04%	0.009%
7	3.058	609	612	615	rVB4	1160	567	0.02%	0.005%
8	3.177	646	649	653	rBV4	656	543	0.02%	0.005%
9	3.228	663	665	670	rVB3	799	651	0.03%	0.005%
10	3.302	686	688	692	rBV3	952	551	0.02%	0.005%
11	3.412	718	722	725	rVB5	729	521	0.02%	0.004%
12	3.450	730	734	736	rBV3	1015	503	0.02%	0.004%
13	3.650	794	796	801	rVV3	700	473	0.02%	0.004%
14	3.907	864	876	906	rBV	83991	257894	10.27%	2.178%
15	4.296	995	997	1000	rBV4	912	448	0.02%	0.004%
16	4.376	1007	1022	1045	rVB2	175189	430031	17.13%	3.632%
17	4.569	1075	1082	1085	rBV7	1672	1768	0.07%	0.015%
18	4.592	1085	1089	1092	rVB4	733	449	0.02%	0.004%
19	4.611	1092	1095	1098	rBV4	1113	834	0.03%	0.007%
20	4.653	1105	1108	1112	rVB3	861	715	0.03%	0.006%
21	4.675	1113	1115	1118	rVB2	941	523	0.02%	0.004%
22	4.746	1134	1137	1140	rBV3	1192	699	0.03%	0.006%
23	4.804	1152	1155	1158	rBV2	961	634	0.03%	0.005%
24	4.933	1192	1195	1197	rVB3	1171	579	0.02%	0.005%
25	4.945	1197	1199	1205	rBV4	611	623	0.02%	0.005%
26	5.071	1220	1238	1269	rBV2	416157	1112997	44.34%	9.400%
27	5.270	1298	1300	1305	rBV5	771	458	0.02%	0.004%
28	5.296	1305	1308	1311	rBV3	795	575	0.02%	0.005%
29	5.331	1317	1319	1324	rVB4	829	590	0.02%	0.005%
30	5.405	1340	1342	1347	rVB3	777	522	0.02%	0.004%
31	5.479	1362	1365	1367	rBV3	1277	816	0.03%	0.007%
32	5.640	1402	1415	1445	rBV	396208	787620	31.38%	6.652%
33	5.871	1481	1487	1489	rBV4	1272	1023	0.04%	0.009%
34	5.939	1497	1508	1515	rBV4	4124	8434	0.34%	0.071%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017570.D
 Acq On : 21 Jul 2020 17:46
 Operator : SY/MD
 Sample : L3336-22DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DUP(071520)DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

35	6.093	1542	1556	1581	rBV	242584	495117	19.72%	4.181%
36	6.360	1634	1639	1647	rBV3	811	1195	0.05%	0.010%
37	6.482	1675	1677	1680	rVB2	1193	639	0.03%	0.005%
38	6.646	1724	1728	1729	rBV2	1436	986	0.04%	0.008%
39	6.781	1768	1770	1775	rVB5	781	561	0.02%	0.005%
40	6.820	1778	1782	1784	rBV4	792	697	0.03%	0.006%
41	7.006	1829	1840	1865	rBV	134461	245533	9.78%	2.074%
42	7.129	1876	1878	1882	rVB2	1607	920	0.04%	0.008%
43	7.264	1918	1920	1923	rVB3	1299	676	0.03%	0.006%
44	7.289	1923	1928	1931	rBV5	1273	1113	0.04%	0.009%
45	7.338	1931	1943	1962	rBV	497796	859677	34.25%	7.260%
46	7.643	2028	2038	2059	rBV2	95136	169123	6.74%	1.428%
47	7.916	2117	2123	2125	rBV5	792	798	0.03%	0.007%
48	8.106	2173	2182	2205	rBV	292419	518691	20.66%	4.381%
49	8.322	2247	2249	2251	rBV2	948	521	0.02%	0.004%
50	8.505	2302	2306	2308	rBV3	1381	1033	0.04%	0.009%
51	8.556	2318	2322	2325	rBV3	786	801	0.03%	0.007%
52	8.727	2371	2375	2377	rBV3	737	578	0.02%	0.005%
53	8.781	2390	2392	2397	rVB2	730	553	0.02%	0.005%
54	8.823	2402	2405	2407	rBV3	998	633	0.03%	0.005%
55	8.875	2408	2421	2424	rBV	635152	936590	37.31%	7.910%
56	9.164	2508	2511	2514	rBV5	1356	997	0.04%	0.008%
57	9.344	2565	2567	2570	rVB3	1058	487	0.02%	0.004%
58	9.392	2580	2582	2584	rBV	789	485	0.02%	0.004%
59	9.444	2594	2598	2601	rBV3	804	650	0.03%	0.005%
60	9.476	2605	2608	2611	rVB4	748	537	0.02%	0.005%
61	9.550	2627	2631	2632	rBV2	1020	728	0.03%	0.006%
62	9.672	2667	2669	2674	rBV3	801	570	0.02%	0.005%
63	9.891	2735	2737	2741	rBV4	783	567	0.02%	0.005%
64	9.945	2751	2754	2757	rBV4	1097	709	0.03%	0.006%
65	10.016	2772	2776	2778	rBV3	775	541	0.02%	0.005%
66	10.029	2778	2780	2782	rVV2	689	464	0.02%	0.004%
67	10.074	2790	2794	2797	rVV4	753	747	0.03%	0.006%
68	10.087	2797	2798	2802	rVB2	1063	601	0.02%	0.005%
69	10.183	2826	2828	2830	rBV3	815	454	0.02%	0.004%
70	10.238	2833	2845	2859	rBV	345058	540267	21.52%	4.563%
71	10.784	3012	3015	3017	rBV4	886	645	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017570.D
 Acq On : 21 Jul 2020 17:46
 Operator : SY/MD
 Sample : L3336-22DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DUP(071520)DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

72	10.820	3022	3026	3029	rBV4	727	657	0.03%	0.006%
73	10.871	3039	3042	3044	rBV3	1018	497	0.02%	0.004%
74	10.939	3060	3063	3065	rBV3	1186	707	0.03%	0.006%
75	11.077	3100	3106	3109	rVV5	791	882	0.04%	0.007%
76	11.202	3133	3145	3156	rBV	418289	650796	25.93%	5.496%
77	11.292	3156	3173	3195	rVB2	1070843	2510254	100.00%	21.200%
78	11.563	3254	3257	3261	rBV3	1092	631	0.03%	0.005%
79	11.646	3271	3283	3304	rBV2	591451	1053402	41.96%	8.896%
80	11.845	3340	3345	3346	rBV4	804	615	0.02%	0.005%
81	11.865	3349	3351	3353	rBV3	1381	751	0.03%	0.006%
82	11.939	3367	3374	3380	rVB6	1315	1325	0.05%	0.011%
83	12.157	3439	3442	3446	rBV3	588	617	0.02%	0.005%
84	12.411	3517	3521	3523	rBV3	1199	909	0.04%	0.008%
85	12.559	3562	3567	3571	rBV4	1012	1000	0.04%	0.008%
86	12.665	3594	3600	3602	rBV5	2458	2063	0.08%	0.017%
87	12.772	3627	3633	3634	rBV4	931	1005	0.04%	0.008%
88	12.817	3643	3647	3650	rBV4	934	599	0.02%	0.005%
89	13.042	3714	3717	3721	rBV2	597	535	0.02%	0.005%
90	13.206	3762	3768	3771	rBV3	1224	1191	0.05%	0.010%
91	13.283	3780	3792	3809	rBV	434644	654645	26.08%	5.529%
92	13.389	3823	3825	3828	rBV4	881	570	0.02%	0.005%
93	13.466	3847	3849	3854	rVB4	1380	637	0.03%	0.005%
94	13.527	3863	3868	3869	rBV2	1835	1329	0.05%	0.011%
95	14.019	4018	4021	4023	rBV3	1369	833	0.03%	0.007%
96	14.090	4040	4043	4046	rBV2	1081	732	0.03%	0.006%
97	14.173	4067	4069	4073	rVB3	1006	494	0.02%	0.004%
98	14.341	4118	4121	4123	rBV2	1168	603	0.02%	0.005%
99	14.788	4256	4260	4262	rBV4	1229	835	0.03%	0.007%
100	15.080	4346	4351	4352	rBV3	1194	1063	0.04%	0.009%


Sum of corrected areas: 11840795

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072120\
Data File : VV017570.D
Acq On : 21 Jul 2020 17:46
Operator : SY/MD
Sample : L3336-22DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DUP(071520)DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

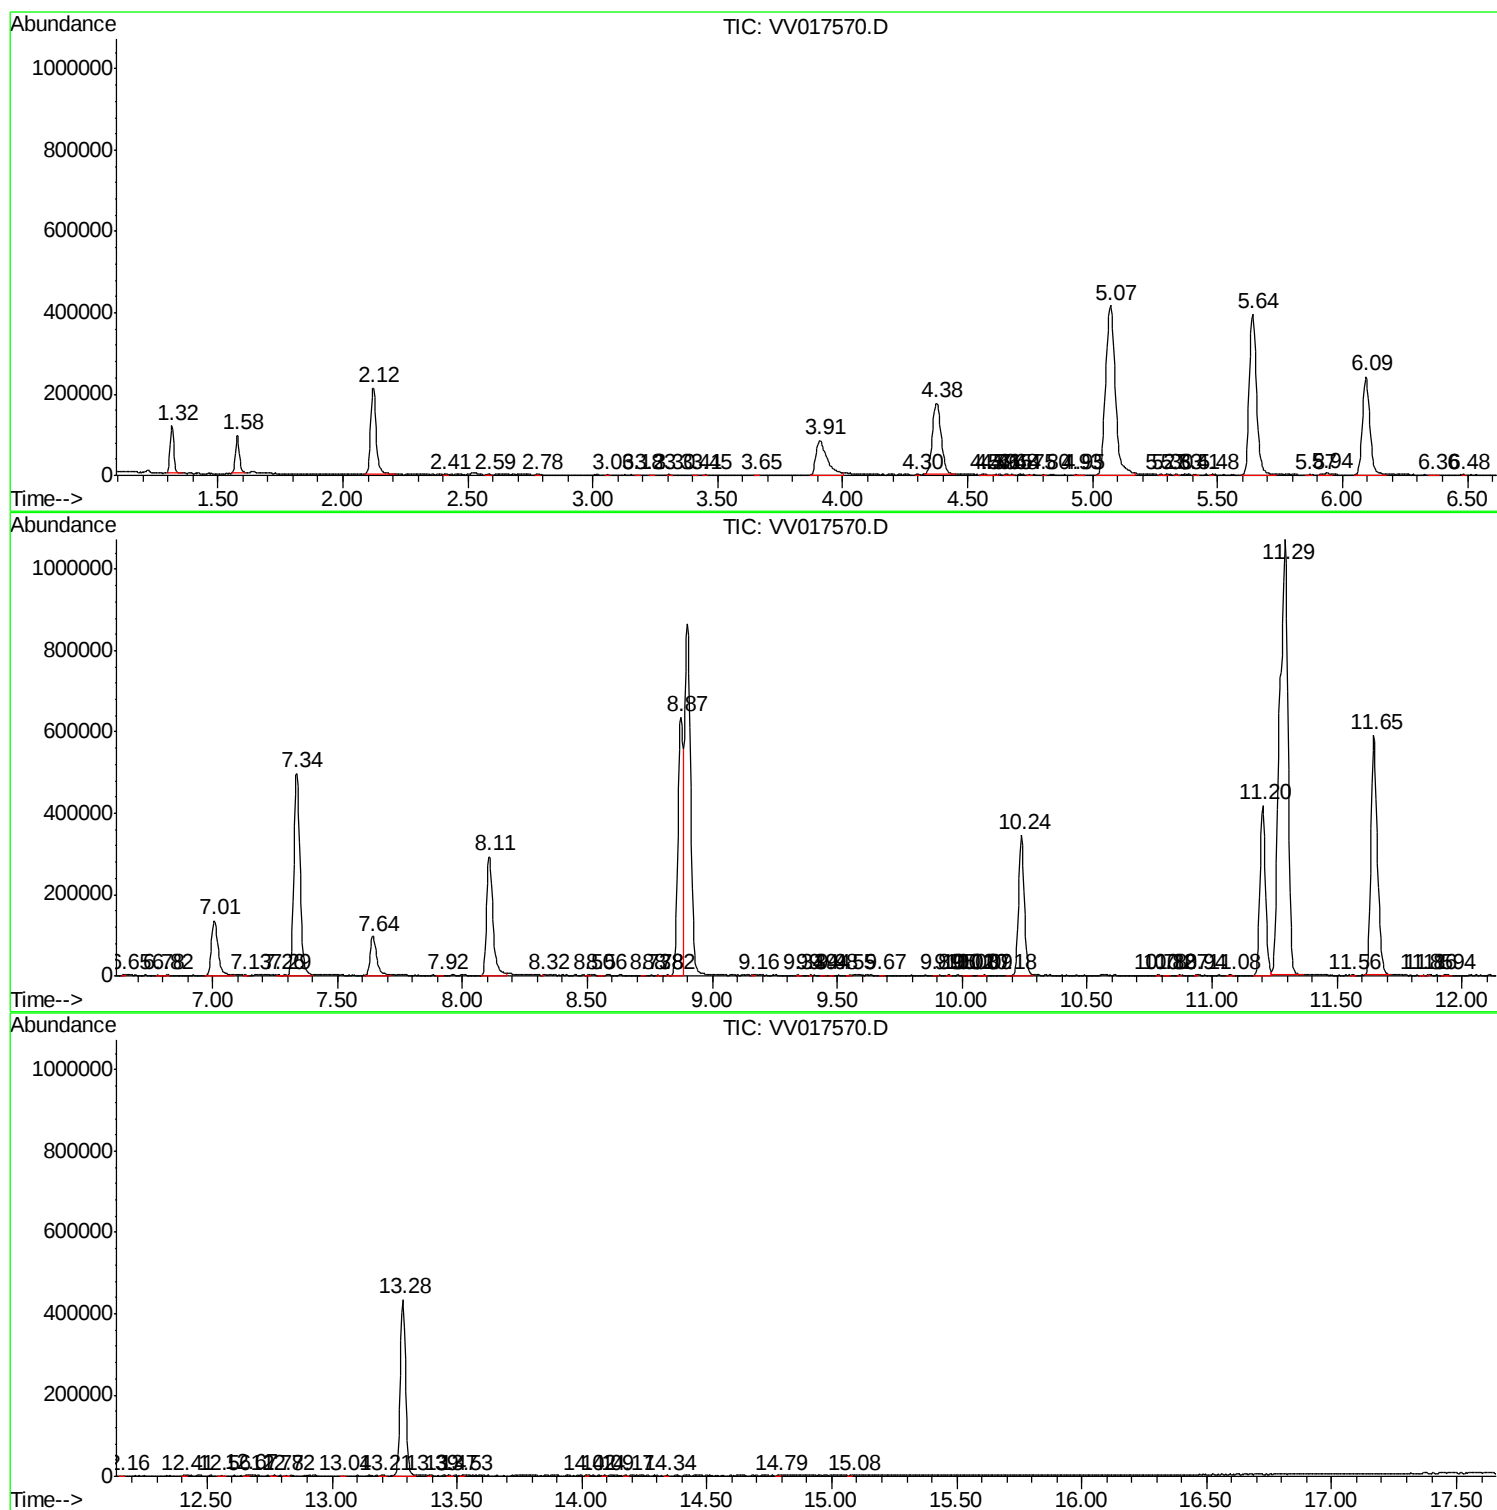

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017570.D
Acq On : 21 Jul 2020 17:46
Operator : SY/MD
Sample : L3336-22DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DUP(071520)DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017570.D
Acq On : 21 Jul 2020 17:46
Operator : SY/MD
Sample : L3336-22DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DUP(071520)DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc