

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017571.D
 Acq On : 21 Jul 2020 18:09
 Operator : SY/MD
 Sample : L3336-14DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9DDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	118773	118243	9.64%	1.155%
2	1.579	145	152	161	rBV	91517	103372	8.43%	1.009%
3	2.119	310	320	341	rBV	209426	324698	26.46%	3.171%
4	2.438	416	419	421	rBV3	907	608	0.05%	0.006%
5	2.582	462	464	470	rVB5	712	552	0.04%	0.005%
6	2.621	470	476	477	rBV4	1435	1234	0.10%	0.012%
7	2.724	506	508	512	rBV3	1074	652	0.05%	0.006%
8	2.833	538	542	545	rBV4	953	721	0.06%	0.007%
9	2.952	574	579	581	rBV4	856	620	0.05%	0.006%
10	3.081	614	619	622	rBV5	1053	733	0.06%	0.007%
11	3.097	622	624	627	rBV4	777	592	0.05%	0.006%
12	3.196	653	655	657	rVV3	929	499	0.04%	0.005%
13	3.209	657	659	662	rVV4	826	596	0.05%	0.006%
14	3.232	665	666	670	rVV2	995	422	0.03%	0.004%
15	3.508	751	752	761	rVB4	955	929	0.08%	0.009%
16	3.688	803	808	811	rBV5	642	477	0.04%	0.005%
17	3.910	866	877	911	rBV	79810	253145	20.63%	2.472%
18	4.232	974	977	979	rBV2	1143	648	0.05%	0.006%
19	4.376	1005	1022	1043	rBV	181661	444203	36.20%	4.338%
20	4.601	1089	1092	1093	rBV2	1087	656	0.05%	0.006%
21	4.634	1100	1102	1108	rVB6	863	633	0.05%	0.006%
22	4.692	1117	1120	1124	rBV2	1450	1263	0.10%	0.012%
23	4.788	1146	1150	1151	rBV	627	422	0.03%	0.004%
24	4.897	1181	1184	1188	rBV3	608	444	0.04%	0.004%
25	5.071	1222	1238	1263	rBV2	419105	1064179	86.73%	10.392%
26	5.286	1302	1305	1308	rBV4	1345	841	0.07%	0.008%
27	5.479	1362	1365	1370	rBV5	1493	1098	0.09%	0.011%
28	5.563	1389	1391	1394	rBV3	717	412	0.03%	0.004%
29	5.640	1399	1415	1440	rBV	397645	790098	64.40%	7.715%
30	6.007	1525	1529	1532	rBV3	751	682	0.06%	0.007%
31	6.093	1543	1556	1575	rBV	240594	488430	39.81%	4.770%
32	6.354	1634	1637	1639	rBV4	1192	543	0.04%	0.005%
33	6.457	1667	1669	1673	rBV3	870	560	0.05%	0.005%
34	6.521	1686	1689	1692	rBV2	915	493	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017571.D
 Acq On : 21 Jul 2020 18:09
 Operator : SY/MD
 Sample : L3336-14DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9DDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

35	6.621	1716	1720	1721	rBV3	584	412	0.03%	0.004%
36	6.650	1722	1729	1731	rBV6	1420	1368	0.11%	0.013%
37	6.708	1743	1747	1750	rBV3	648	641	0.05%	0.006%
38	6.801	1773	1776	1778	rBV2	807	504	0.04%	0.005%
39	6.923	1811	1814	1816	rBV5	984	791	0.06%	0.008%
40	7.007	1829	1840	1861	rVV	129969	240277	19.58%	2.346%
41	7.158	1883	1887	1889	rBV4	856	754	0.06%	0.007%
42	7.254	1915	1917	1921	rVB3	952	419	0.03%	0.004%
43	7.296	1928	1930	1931	rBV2	1027	458	0.04%	0.004%
44	7.338	1931	1943	1968	rVV	494747	849690	69.25%	8.297%
45	7.534	2001	2004	2006	rVB2	1207	705	0.06%	0.007%
46	7.601	2021	2025	2026	rBV3	1068	609	0.05%	0.006%
47	7.643	2027	2038	2060	rVV	96301	166746	13.59%	1.628%
48	7.807	2086	2089	2095	rVB4	1034	910	0.07%	0.009%
49	7.958	2132	2136	2138	rBV	732	448	0.04%	0.004%
50	7.971	2138	2140	2145	rVV3	825	668	0.05%	0.007%
51	8.003	2145	2150	2155	rVV6	1634	1426	0.12%	0.014%
52	8.106	2170	2182	2209	rBV	287636	518516	42.26%	5.063%
53	8.505	2304	2306	2309	rVV3	644	475	0.04%	0.005%
54	8.695	2361	2365	2367	rBV4	801	546	0.04%	0.005%
55	8.833	2403	2408	2409	rBV3	1321	1064	0.09%	0.010%
56	8.871	2409	2420	2444	rVV	594340	977298	79.65%	9.543%
57	9.125	2497	2499	2502	rBV3	807	438	0.04%	0.004%
58	9.174	2507	2514	2516	rBV7	1460	1574	0.13%	0.015%
59	9.228	2527	2531	2535	rBV4	1010	904	0.07%	0.009%
60	9.341	2562	2566	2569	rBV3	817	684	0.06%	0.007%
61	9.466	2603	2605	2609	rVB2	948	572	0.05%	0.006%
62	9.492	2612	2613	2619	rVB3	789	434	0.04%	0.004%
63	9.537	2624	2627	2631	rBV2	769	649	0.05%	0.006%
64	9.559	2631	2634	2636	rBV4	1787	1166	0.10%	0.011%
65	9.646	2659	2661	2664	rBV2	872	426	0.03%	0.004%
66	10.103	2799	2803	2806	rBV2	505	422	0.03%	0.004%
67	10.122	2806	2809	2812	rBV2	666	433	0.04%	0.004%
68	10.158	2817	2820	2825	rVB5	1195	833	0.07%	0.008%
69	10.238	2832	2845	2865	rBV	341452	540090	44.02%	5.274%
70	10.315	2865	2869	2873	rVB4	1446	1376	0.11%	0.013%
71	10.389	2889	2892	2894	rBV3	1152	482	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017571.D
 Acq On : 21 Jul 2020 18:09
 Operator : SY/MD
 Sample : L3336-14DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9DDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

72	10.559	2941	2945	2950	rVV5	1265	1132	0.09%	0.011%
73	10.669	2975	2979	2984	rBV5	631	476	0.04%	0.005%
74	10.707	2988	2991	2995	rVB2	766	564	0.05%	0.006%
75	10.810	3019	3023	3026	rVB4	595	460	0.04%	0.004%
76	10.939	3060	3063	3065	rBV3	1220	797	0.06%	0.008%
77	10.981	3073	3076	3081	rVB5	1287	956	0.08%	0.009%
78	11.058	3094	3100	3101	rBV3	816	658	0.05%	0.006%
79	11.138	3121	3125	3130	rVB6	1256	1085	0.09%	0.011%
80	11.170	3130	3135	3136	rBV3	739	591	0.05%	0.006%
81	11.206	3136	3146	3155	rVV	25622	40653	3.31%	0.397%
82	11.270	3155	3166	3189	rVB2	614898	1074712	87.59%	10.495%
83	11.421	3211	3213	3217	rBV3	894	744	0.06%	0.007%
84	11.450	3220	3222	3227	rBV2	574	417	0.03%	0.004%
85	11.646	3269	3283	3302	rBV	554787	872166	71.08%	8.517%
86	12.032	3399	3403	3407	rBV3	720	714	0.06%	0.007%
87	12.090	3418	3421	3423	rVB2	685	416	0.03%	0.004%
88	12.370	3504	3508	3510	rBV2	781	550	0.04%	0.005%
89	12.485	3539	3544	3546	rBV5	910	932	0.08%	0.009%
90	12.620	3582	3586	3589	rBV4	978	1010	0.08%	0.010%
91	12.662	3596	3599	3601	rBV3	1476	914	0.07%	0.009%
92	12.891	3667	3670	3673	rBV3	900	579	0.05%	0.006%
93	13.122	3736	3742	3743	rVV4	797	611	0.05%	0.006%
94	13.283	3780	3792	3809	rBV	792365	1226944	100.00%	11.981%
95	13.530	3865	3869	3873	rBV6	1650	1489	0.12%	0.015%
96	13.727	3928	3930	3933	rBV2	903	671	0.05%	0.007%
97	13.768	3933	3943	3956	rVV	56780	89406	7.29%	0.873%
98	14.026	4019	4023	4025	rBV2	685	532	0.04%	0.005%
99	14.135	4055	4057	4061	rVB4	778	466	0.04%	0.005%
100	14.370	4128	4130	4136	rBV4	1264	1065	0.09%	0.010%


Sum of corrected areas: 10240616

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072120\
Data File : VV017571.D
Acq On : 21 Jul 2020 18:09
Operator : SY/MD
Sample : L3336-14DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9DDL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

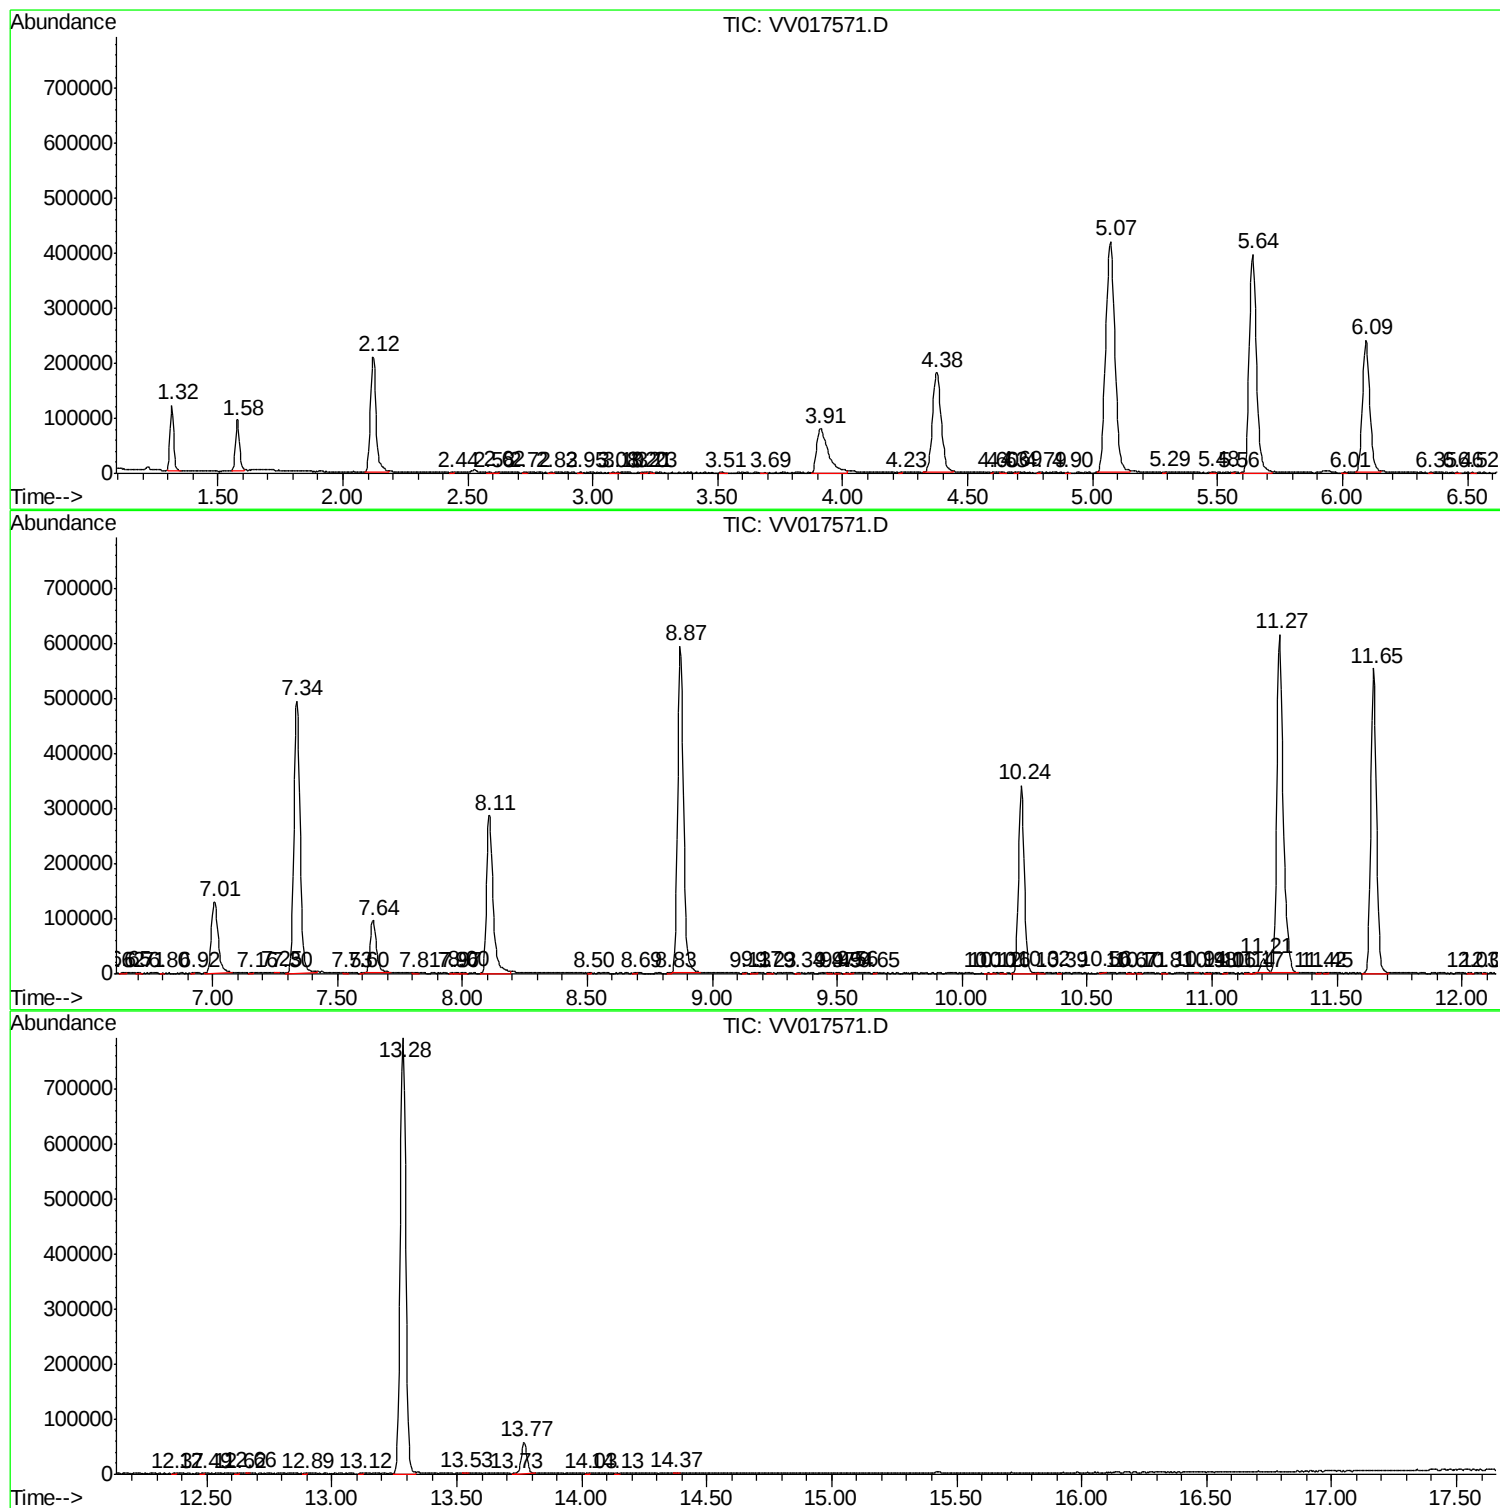

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017571.D
Acq On : 21 Jul 2020 18:09
Operator : SY/MD
Sample : L3336-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9DDL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017571.D
Acq On : 21 Jul 2020 18:09
Operator : SY/MD
Sample : L3336-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9DDL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc