

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017572.D
 Acq On : 21 Jul 2020 18:32
 Operator : SY/MD
 Sample : L3336-13DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9SDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	113095	117615	5.02%	1.070%
2	1.576	145	151	162	rBV	83365	92350	3.94%	0.840%
3	2.119	310	320	342	rVB	204454	307777	13.14%	2.800%
4	2.389	402	404	409	rBV3	624	562	0.02%	0.005%
5	2.624	475	477	479	rBV2	1089	756	0.03%	0.007%
6	2.817	534	537	538	rBV	705	380	0.02%	0.003%
7	2.939	573	575	577	rBV2	850	380	0.02%	0.003%
8	3.058	606	612	616	rBV7	994	1174	0.05%	0.011%
9	3.261	669	675	677	rBV5	937	938	0.04%	0.009%
10	3.293	683	685	689	rVB3	1232	673	0.03%	0.006%
11	3.325	691	695	696	rBV2	843	418	0.02%	0.004%
12	3.357	703	705	712	rVB6	1073	794	0.03%	0.007%
13	3.592	775	778	783	rVB4	814	619	0.03%	0.006%
14	3.640	789	793	796	rVV4	1554	1236	0.05%	0.011%
15	3.672	800	803	808	rBV4	871	1014	0.04%	0.009%
16	3.717	814	817	821	rBV3	768	616	0.03%	0.006%
17	3.756	825	829	835	rVB5	1189	1091	0.05%	0.010%
18	3.907	866	876	919	rBV	77861	265396	11.33%	2.414%
19	4.286	990	994	999	rVB6	1048	1002	0.04%	0.009%
20	4.376	1004	1022	1048	rVV	172770	431994	18.44%	3.930%
21	4.669	1111	1113	1117	rVB3	833	651	0.03%	0.006%
22	4.698	1118	1122	1129	rBV6	1241	1238	0.05%	0.011%
23	4.730	1129	1132	1136	rBV4	949	587	0.03%	0.005%
24	4.769	1142	1144	1145	rBV	973	538	0.02%	0.005%
25	4.952	1197	1201	1204	rBV3	1024	742	0.03%	0.007%
26	4.968	1204	1206	1210	rVB3	830	459	0.02%	0.004%
27	5.010	1216	1219	1221	rBV3	908	511	0.02%	0.005%
28	5.071	1221	1238	1267	rBV2	407406	1045888	44.65%	9.514%
29	5.450	1354	1356	1358	rBV3	769	384	0.02%	0.003%
30	5.550	1385	1387	1390	rBV3	864	586	0.03%	0.005%
31	5.566	1390	1392	1395	rVB	744	372	0.02%	0.003%
32	5.582	1395	1397	1401	rBV3	594	553	0.02%	0.005%
33	5.640	1402	1415	1436	rBV	381634	758512	32.39%	6.900%
34	5.839	1474	1477	1480	rBV2	839	523	0.02%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017572.D
 Acq On : 21 Jul 2020 18:32
 Operator : SY/MD
 Sample : L3336-13DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9SDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

35	5.891	1489	1493	1496	rVB3	1132	789	0.03%	0.007%
36	5.933	1498	1506	1517	rVV3	4338	9365	0.40%	0.085%
37	5.987	1520	1523	1526	rBV2	1058	803	0.03%	0.007%
38	6.093	1543	1556	1583	rVB	235279	476462	20.34%	4.334%
39	6.360	1635	1639	1642	rBV3	928	684	0.03%	0.006%
40	6.444	1663	1665	1669	rVB3	763	485	0.02%	0.004%
41	6.556	1696	1700	1703	rBV3	1344	1202	0.05%	0.011%
42	6.630	1718	1723	1724	rBV2	794	628	0.03%	0.006%
43	6.804	1774	1777	1779	rBV4	688	383	0.02%	0.003%
44	6.849	1787	1791	1793	rBV2	586	410	0.02%	0.004%
45	6.913	1806	1811	1812	rBV3	674	558	0.02%	0.005%
46	7.006	1829	1840	1861	rBV	129661	234331	10.00%	2.132%
47	7.338	1931	1943	1962	rBV	483034	828389	35.37%	7.535%
48	7.643	2027	2038	2056	rBV	95236	164979	7.04%	1.501%
49	7.810	2087	2090	2091	rBV3	826	419	0.02%	0.004%
50	7.865	2105	2107	2108	rBV	828	395	0.02%	0.004%
51	8.109	2172	2183	2215	rBV	261573	505300	21.57%	4.596%
52	8.611	2335	2339	2343	rBV5	578	764	0.03%	0.007%
53	8.685	2360	2362	2366	rVV2	638	412	0.02%	0.004%
54	8.746	2377	2381	2382	rBV3	891	646	0.03%	0.006%
55	8.785	2390	2393	2395	rBV2	733	502	0.02%	0.005%
56	8.871	2409	2420	2444	rVV	591905	1063052	45.39%	9.670%
57	9.029	2463	2469	2472	rBV8	1164	1394	0.06%	0.013%
58	9.093	2485	2489	2490	rBV3	785	472	0.02%	0.004%
59	9.132	2498	2501	2503	rBV3	1186	951	0.04%	0.009%
60	9.151	2505	2507	2508	rVV	888	379	0.02%	0.003%
61	9.161	2508	2510	2515	rVV4	1442	1198	0.05%	0.011%
62	9.222	2527	2529	2533	rBV3	608	449	0.02%	0.004%
63	9.309	2554	2556	2559	rVB3	1220	583	0.02%	0.005%
64	9.534	2624	2626	2630	rBV3	940	625	0.03%	0.006%
65	9.762	2694	2697	2705	rVB7	975	827	0.04%	0.008%
66	9.833	2714	2719	2720	rBV4	1123	725	0.03%	0.007%
67	9.878	2730	2733	2734	rBV2	784	397	0.02%	0.004%
68	9.932	2747	2750	2751	rBV2	721	382	0.02%	0.003%
69	10.029	2777	2780	2783	rVB4	1204	700	0.03%	0.006%
70	10.238	2831	2845	2859	rBV	331652	529457	22.61%	4.816%
71	10.350	2875	2880	2882	rBV3	871	732	0.03%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017572.D
 Acq On : 21 Jul 2020 18:32
 Operator : SY/MD
 Sample : L3336-13DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9SDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

72	10.363	2882	2884	2889	rVV2	675	465	0.02%	0.004%
73	10.469	2915	2917	2921	rVB3	749	458	0.02%	0.004%
74	10.489	2921	2923	2926	rBV2	996	709	0.03%	0.006%
75	10.604	2952	2959	2960	rBV6	908	802	0.03%	0.007%
76	10.675	2978	2981	2983	rVB3	989	502	0.02%	0.005%
77	10.791	3015	3017	3020	rBV2	973	616	0.03%	0.006%
78	10.846	3032	3034	3038	rBV3	804	686	0.03%	0.006%
79	10.913	3053	3055	3058	rBV3	611	414	0.02%	0.004%
80	11.202	3133	3145	3156	rBV	494773	751333	32.08%	6.834%
81	11.292	3156	3173	3194	rVB2	961013	2342157	100.00%	21.305%
82	11.646	3271	3283	3307	rBV2	568505	986153	42.10%	8.971%
83	11.900	3355	3362	3363	rBV5	983	747	0.03%	0.007%
84	12.090	3419	3421	3424	rVB3	1031	620	0.03%	0.006%
85	12.145	3436	3438	3442	rBV5	915	687	0.03%	0.006%
86	12.479	3539	3542	3544	rBV3	821	492	0.02%	0.004%
87	12.566	3564	3569	3570	rBV	954	667	0.03%	0.006%
88	12.624	3583	3587	3589	rBV3	677	495	0.02%	0.005%
89	12.730	3615	3620	3622	rBV3	996	873	0.04%	0.008%
90	12.807	3641	3644	3646	rBV4	822	586	0.03%	0.005%
91	12.865	3659	3662	3665	rBV2	1054	746	0.03%	0.007%
92	12.935	3682	3684	3689	rVB4	1297	797	0.03%	0.007%
93	12.964	3689	3693	3694	rBV2	742	533	0.02%	0.005%
94	13.286	3785	3793	3804	rVB3	18519	29554	1.26%	0.269%
95	13.624	3894	3898	3899	rBV	976	570	0.02%	0.005%
96	13.897	3980	3983	3985	rBV3	886	471	0.02%	0.004%
97	14.070	4035	4037	4041	rBV3	909	773	0.03%	0.007%
98	14.112	4048	4050	4053	rBV2	942	464	0.02%	0.004%
99	14.132	4053	4056	4060	rVV3	859	735	0.03%	0.007%
100	14.189	4072	4074	4077	rBV3	1043	598	0.03%	0.005%


Sum of corrected areas: 10993261

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072120\
Data File : VV017572.D
Acq On : 21 Jul 2020 18:32
Operator : SY/MD
Sample : L3336-13DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9SDL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

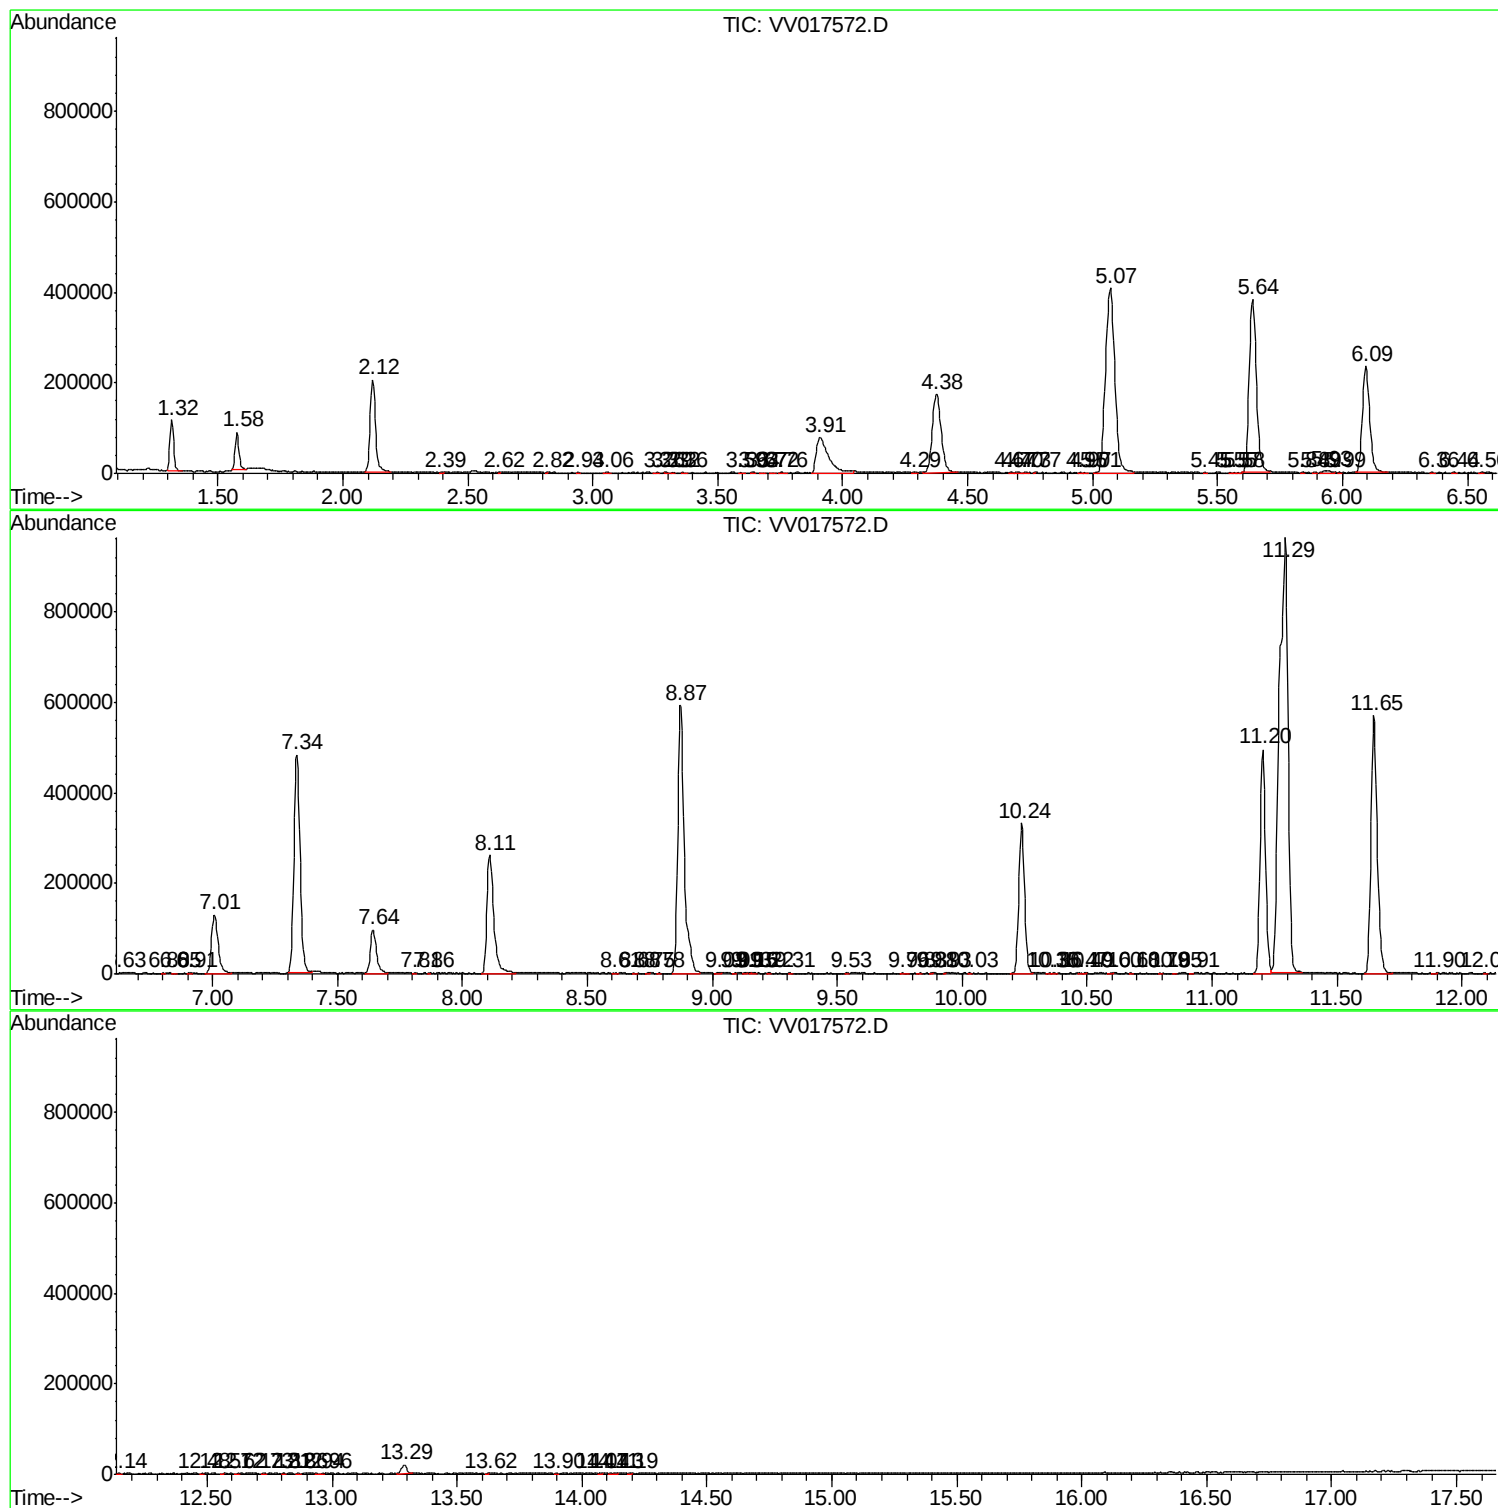

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017572.D
Acq On : 21 Jul 2020 18:32
Operator : SY/MD
Sample : L3336-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9SDL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017572.D
Acq On : 21 Jul 2020 18:32
Operator : SY/MD
Sample : L3336-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9SDL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc