

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017575.D
 Acq On : 21 Jul 2020 19:42
 Operator : SY/MD
 Sample : L3336-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9D

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	111056	113452	0.36%	0.243%
2	1.576	145	151	164	rBV	89647	100245	0.32%	0.215%
3	2.016	285	288	289	rBV2	945	549	0.00%	0.001%
4	2.119	310	320	338	rBV	202976	310509	0.99%	0.665%
5	2.306	375	378	379	rBV2	1541	773	0.00%	0.002%
6	2.569	456	460	464	rVB3	972	715	0.00%	0.002%
7	2.630	473	479	480	rBV4	825	802	0.00%	0.002%
8	2.669	487	491	495	rBV5	1413	1533	0.00%	0.003%
9	2.765	519	521	523	rBV2	894	509	0.00%	0.001%
10	2.891	557	560	562	rBV3	1153	798	0.00%	0.002%
11	2.997	589	593	595	rVB3	986	669	0.00%	0.001%
12	3.020	598	600	604	rVV3	833	550	0.00%	0.001%
13	3.116	624	630	634	rBV4	697	818	0.00%	0.002%
14	3.245	667	670	674	rVB3	858	610	0.00%	0.001%
15	3.659	797	799	804	rVB3	719	491	0.00%	0.001%
16	3.762	827	831	834	rBV2	561	416	0.00%	0.001%
17	3.907	866	876	912	rBV2	78301	246797	0.79%	0.528%
18	4.312	1000	1002	1005	rBV2	896	517	0.00%	0.001%
19	4.380	1006	1023	1045	rVV	179852	448156	1.44%	0.959%
20	4.563	1078	1080	1083	rVB2	824	431	0.00%	0.001%
21	4.923	1188	1192	1194	rBV4	1074	823	0.00%	0.002%
22	4.962	1202	1204	1206	rBV3	940	424	0.00%	0.001%
23	5.071	1220	1238	1264	rBV2	413894	1075628	3.45%	2.303%
24	5.354	1324	1326	1328	rBV3	719	417	0.00%	0.001%
25	5.380	1332	1334	1339	rVV4	719	559	0.00%	0.001%
26	5.431	1347	1350	1355	rBV5	656	590	0.00%	0.001%
27	5.505	1368	1373	1376	rBV3	1238	1115	0.00%	0.002%
28	5.537	1381	1383	1387	rVB2	1113	442	0.00%	0.001%
29	5.563	1387	1391	1394	rVB3	869	647	0.00%	0.001%
30	5.640	1403	1415	1440	rBV	369945	734550	2.35%	1.572%
31	5.936	1495	1507	1509	rBV10	5395	7879	0.03%	0.017%
32	6.093	1542	1556	1574	rBV	243988	485647	1.56%	1.040%
33	6.331	1626	1630	1634	rBV4	998	732	0.00%	0.002%
34	6.354	1635	1637	1642	rBV4	672	620	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017575.D
 Acq On : 21 Jul 2020 19:42
 Operator : SY/MD
 Sample : L3336-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9D

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

35	6.421	1653	1658	1660	rBV6	950	949	0.00%	0.002%
36	6.450	1664	1667	1670	rBV3	956	602	0.00%	0.001%
37	6.515	1684	1687	1690	rBV2	696	655	0.00%	0.001%
38	6.637	1721	1725	1726	rBV4	2038	1326	0.00%	0.003%
39	6.775	1763	1768	1769	rBV3	588	432	0.00%	0.001%
40	6.910	1805	1810	1814	rVB4	705	732	0.00%	0.002%
41	7.006	1829	1840	1860	rBV	132116	236117	0.76%	0.505%
42	7.180	1890	1894	1897	rBV4	1344	1262	0.00%	0.003%
43	7.338	1931	1943	1961	rBV	477520	833265	2.67%	1.784%
44	7.643	2027	2038	2055	rBV	94302	164596	0.53%	0.352%
45	8.045	2160	2163	2166	rBV2	690	495	0.00%	0.001%
46	8.106	2172	2182	2204	rBV	290736	516799	1.66%	1.106%
47	8.457	2286	2291	2297	rVB4	1092	983	0.00%	0.002%
48	8.489	2297	2301	2305	rVB5	1402	1259	0.00%	0.003%
49	8.508	2305	2307	2309	rBV3	1213	669	0.00%	0.001%
50	8.614	2337	2340	2341	rBV2	1021	526	0.00%	0.001%
51	8.717	2370	2372	2375	rVB2	1182	490	0.00%	0.001%
52	8.778	2388	2391	2392	rBV	791	557	0.00%	0.001%
53	8.871	2408	2420	2445	rBV2	579784	1212606	3.88%	2.596%
54	9.026	2464	2468	2470	rBV4	1092	743	0.00%	0.002%
55	9.113	2493	2495	2500	rBV2	802	606	0.00%	0.001%
56	9.141	2500	2504	2505	rBV3	1080	700	0.00%	0.001%
57	9.228	2528	2531	2532	rBV	879	520	0.00%	0.001%
58	9.402	2583	2585	2588	rBV3	950	683	0.00%	0.001%
59	9.485	2603	2611	2612	rBV7	673	739	0.00%	0.002%
60	9.495	2612	2614	2620	rVB4	637	488	0.00%	0.001%
61	9.711	2678	2681	2683	rBV2	1132	725	0.00%	0.002%
62	9.952	2752	2756	2762	rBV5	825	986	0.00%	0.002%
63	10.042	2780	2784	2789	rVB5	994	1100	0.00%	0.002%
64	10.067	2789	2792	2795	rBV2	737	627	0.00%	0.001%
65	10.157	2818	2820	2825	rBV	596	425	0.00%	0.001%
66	10.238	2833	2845	2860	rBV	347322	544436	1.74%	1.165%
67	10.395	2885	2894	2895	rBV7	2674	2825	0.01%	0.006%
68	10.682	2978	2983	2985	rBV4	555	503	0.00%	0.001%
69	10.698	2985	2988	2991	rVV3	603	495	0.00%	0.001%
70	10.762	3002	3008	3009	rBV3	827	705	0.00%	0.002%
71	10.936	3056	3062	3064	rBV6	1655	1462	0.00%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
 Data File : VV017575.D
 Acq On : 21 Jul 2020 19:42
 Operator : SY/MD
 Sample : L3336-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9D

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

72	10.987	3074	3078	3080	rBV2	641	446	0.00%	0.001%
73	11.067	3098	3103	3104	rBV4	1061	854	0.00%	0.002%
74	11.157	3127	3131	3133	rBV3	992	587	0.00%	0.001%
75	11.202	3133	3145	3156	rBV	534605	814819	2.61%	1.744%
76	11.293	3156	3173	3197	rVB2	2191895	4216795	13.51%	9.027%
77	11.508	3238	3240	3243	rBV3	637	407	0.00%	0.001%
78	11.553	3248	3254	3257	rBV5	1602	1726	0.01%	0.004%
79	11.604	3265	3270	3271	rBV3	1411	1207	0.00%	0.003%
80	11.646	3271	3283	3302	rVV2	613035	1063194	3.41%	2.276%
81	11.736	3309	3311	3320	rVB7	1398	1268	0.00%	0.003%
82	11.807	3329	3333	3337	rBV6	1150	1033	0.00%	0.002%
83	11.916	3364	3367	3370	rBV4	744	633	0.00%	0.001%
84	11.997	3388	3392	3395	rBV3	888	665	0.00%	0.001%
85	12.177	3445	3448	3450	rBV2	938	610	0.00%	0.001%
86	12.264	3472	3475	3479	rBV5	720	644	0.00%	0.001%
87	12.280	3479	3480	3483	rBV3	700	423	0.00%	0.001%
88	12.428	3521	3526	3527	rBV3	1506	1211	0.00%	0.003%
89	12.466	3535	3538	3543	rVB3	1127	957	0.00%	0.002%
90	12.495	3544	3547	3549	rBV3	932	598	0.00%	0.001%
91	12.669	3594	3601	3612	rVB3	13913	21104	0.07%	0.045%
92	12.858	3657	3660	3664	rBV4	1111	1039	0.00%	0.002%
93	12.981	3694	3698	3704	rVB5	779	891	0.00%	0.002%
94	13.096	3727	3734	3735	rBV2	900	858	0.00%	0.002%
95	13.289	3778	3794	3813	rBV	20186902	31221978	100.00%	66.836%
96	13.765	3930	3942	3958	rBV	1419519	2173010	6.96%	4.652%
97	14.106	4043	4048	4049	rBV4	3836	3082	0.01%	0.007%
98	14.620	4205	4208	4209	rBV	743	408	0.00%	0.001%
99	15.260	4404	4407	4413	rVB7	1645	1770	0.01%	0.004%
100	15.421	4448	4457	4469	rBV2	68441	109419	0.35%	0.234%


Sum of corrected areas: 46714137

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072120\
Data File : VV017575.D
Acq On : 21 Jul 2020 19:42
Operator : SY/MD
Sample : L3336-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9D

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

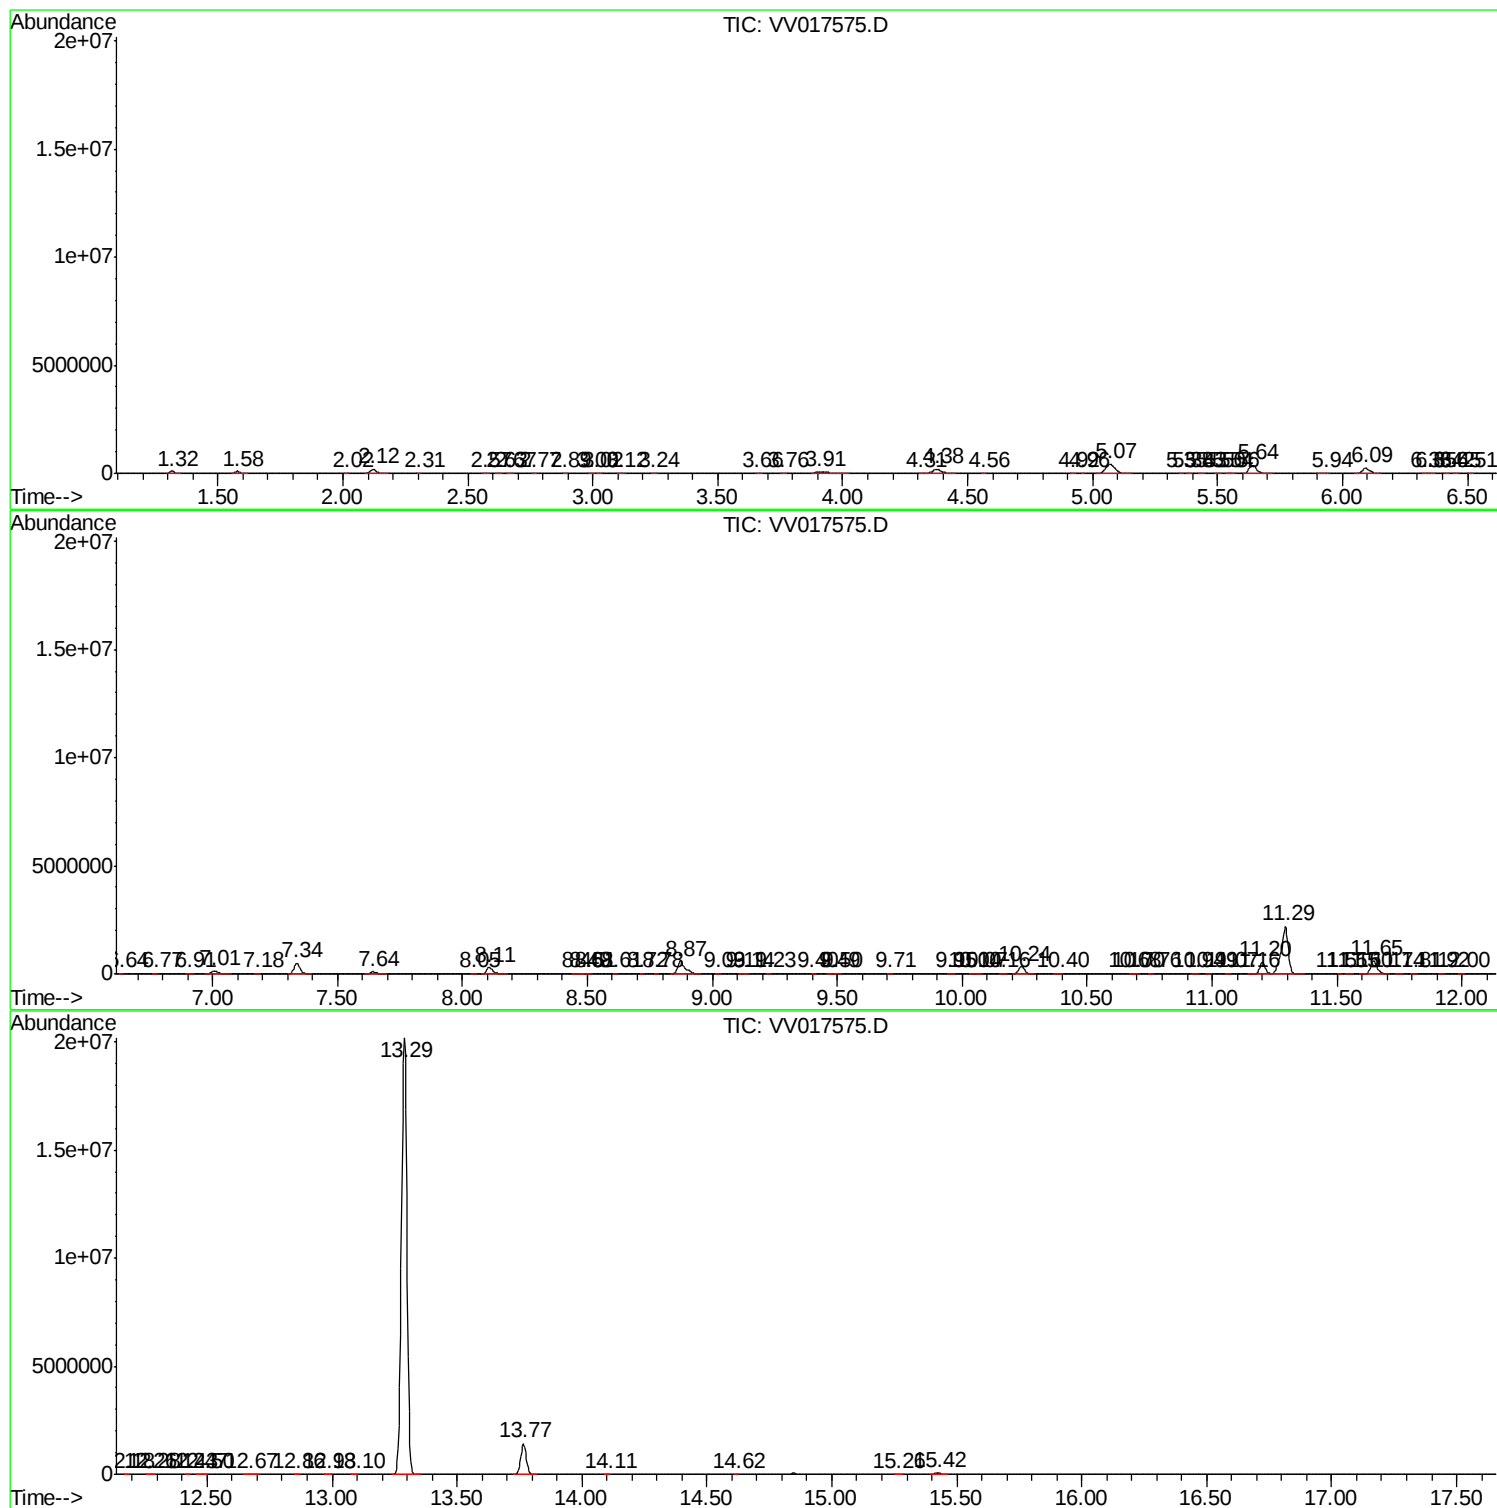

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017575.D
Acq On : 21 Jul 2020 19:42
Operator : SY/MD
Sample : L3336-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9D

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072120\
Data File : VV017575.D
Acq On : 21 Jul 2020 19:42
Operator : SY/MD
Sample : L3336-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9D

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc