


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072120\
 Data File : VV017559.D
 Acq On : 21 Jul 2020 10:56
 Operator : SY/MD
 Sample : BFB64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis
 Last Update : Wed Jul 22 03:23:09 2020

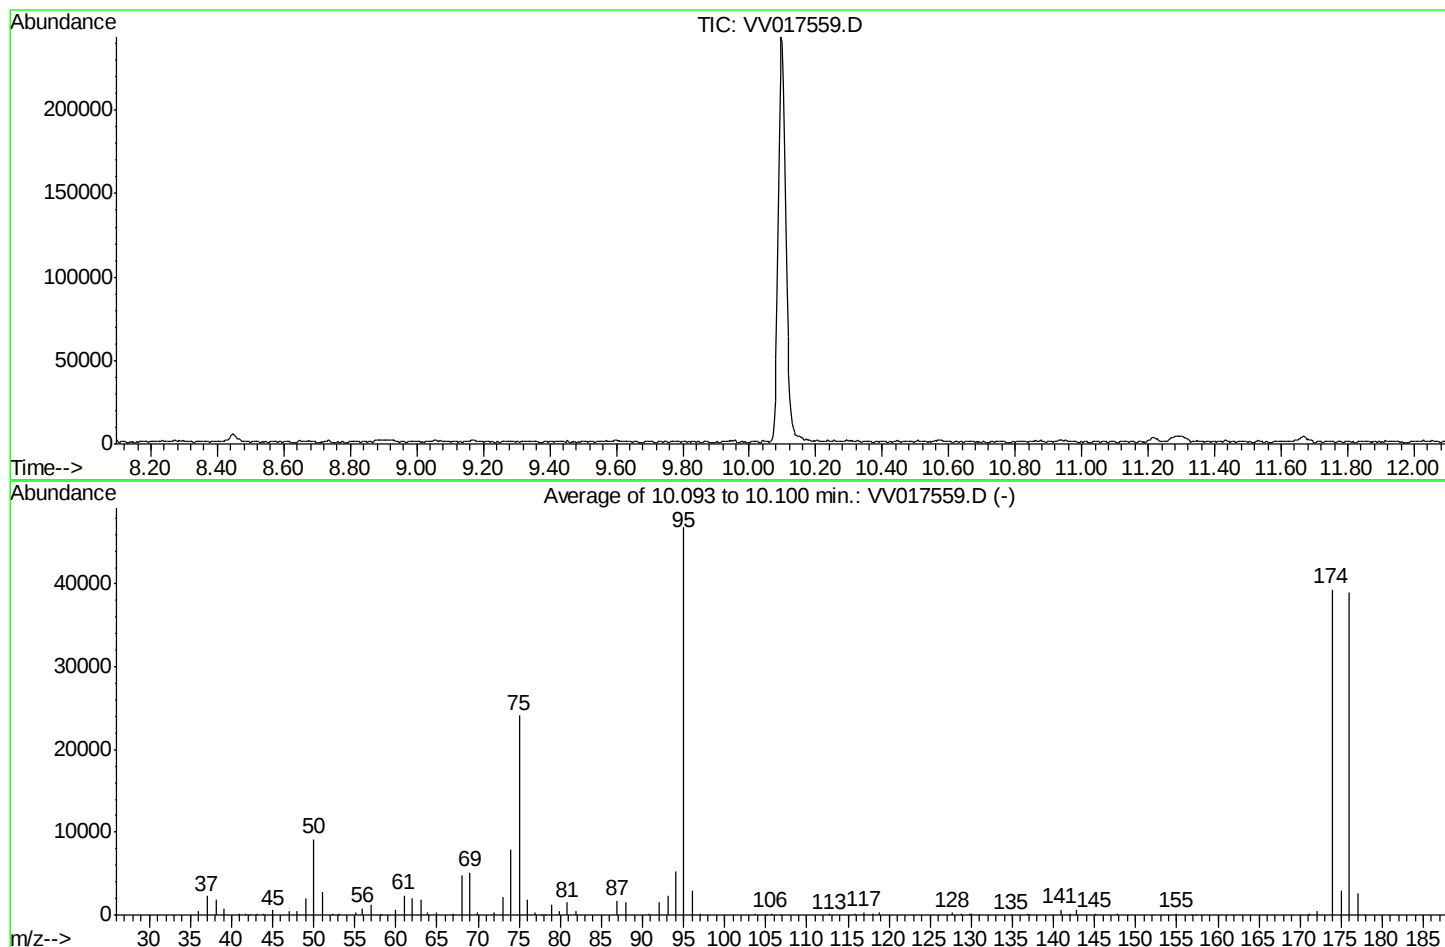

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	9162	PASS
75	95	30	80	51.5	24120	PASS
95	95	100	100	100.0	46856	PASS
96	95	5	9	6.4	3020	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	39376	PASS
175	174	5	9	7.6	2987	PASS
176	174	95	101	99.0	38986	PASS
177	176	5	9	6.7	2619	PASS

m/z	Abundance
36.00	490.0
37.00	2198.0
38.10	1945.0
39.00	895.0
39.80	380.0
41.10	109.0
41.60	114.0
42.20	103.0
43.00	162.0
43.90	455.0
45.00	458.0
47.00	451.0
48.00	448.0
49.00	2009.0
50.00	8897.0
51.00	2723.0
52.20	198.0
53.10	119.0
55.00	264.0
55.90	768.0
57.00	1202.0
58.30	121.0
59.90	508.0
61.00	2339.0
62.00	1990.0
63.00	1586.0
63.90	254.0
65.00	324.0
66.90	191.0
68.00	4628.0
69.00	4610.0
70.00	333.0
72.00	223.0
73.00	2125.0
74.00	7760.0
75.00	22840.0
76.00	1885.0
76.90	299.0
78.10	223.0
78.90	1131.0
79.80	418.0
80.80	1358.0
81.90	369.0
86.90	1685.0
87.90	1386.0
90.80	160.0
91.90	1429.0
93.00	2151.0
94.00	4932.0
95.00	44536.0
96.00	2984.0
97.10	166.0
103.70	207.0
105.10	110.0
105.70	191.0
106.80	108.0
112.80	141.0
115.80	144.0
117.00	339.0
118.00	215.0
118.70	337.0
127.70	271.0
128.70	114.0
129.80	169.0
134.90	128.0
136.80	113.0
137.00	115.0
140.90	663.0
142.00	188.0
142.80	562.0
145.00	196.0
147.90	181.0
155.10	144.0
172.00	459.0
173.90	36768.0
174.90	2705.0
175.90	36136.0
177.00	2314.0
177.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	553.0
37.00	2415.0
38.10	1967.0
39.00	814.0
39.80	360.0
41.00	121.0
41.60	108.0
43.00	155.0
43.90	496.0
45.00	586.0
46.90	450.0
48.00	528.0
49.00	2135.0
50.00	9533.0
51.00	2826.0
52.30	203.0
53.10	119.0
55.10	249.0
55.90	828.0
57.00	1275.0
58.20	109.0
59.90	661.0
61.00	2414.0
62.00	2120.0
63.00	1819.0
63.90	272.0
65.00	342.0
67.00	205.0
68.00	5030.0
69.00	5399.0
69.90	362.0
71.90	255.0
73.00	2271.0
74.00	8266.0
75.00	25088.0
76.00	2024.0
76.90	321.0
78.90	1372.0
79.80	428.0
80.90	1558.0
81.80	399.0
86.90	1840.0
87.90	1527.0
90.80	220.0
91.90	1611.0
93.10	2457.0
94.00	5491.0
95.00	48320.0
96.00	3101.0
97.00	151.0
103.70	234.0
105.70	240.0
106.80	115.0
112.80	126.0
115.80	164.0
116.90	396.0
118.00	237.0
118.70	355.0
127.70	301.0
128.80	135.0
129.80	164.0
130.00	160.0
130.90	117.0
136.80	182.0
140.90	709.0
142.10	195.0
142.80	601.0
145.10	215.0
147.90	133.0
155.00	170.0
156.80	111.0
171.20	179.0
172.00	530.0
173.90	40664.0
174.90	3051.0
175.90	40464.0
177.00	2750.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	554.0
37.00	2240.0
38.10	1828.0
39.00	746.0
39.90	314.0
40.90	166.0
41.70	107.0
43.10	138.0
43.90	467.0
45.00	672.0
47.00	469.0
48.00	535.0
49.00	2000.0
50.00	9058.0
51.00	2708.0
52.30	185.0
53.10	102.0
55.10	207.0
56.00	762.0
57.00	1225.0
58.00	145.0
59.90	706.0
61.00	2242.0
61.90	2166.0
63.10	1964.0
63.90	246.0
65.00	339.0
67.00	226.0
68.00	4914.0
69.00	5404.0
69.90	359.0
71.90	294.0
73.00	2195.0
74.00	7876.0
75.00	24432.0
76.00	1852.0
77.00	303.0
77.70	186.0
78.90	1437.0
79.90	378.0
80.90	1558.0
81.80	413.0
86.90	1804.0
87.90	1604.0
90.80	235.0
92.00	1605.0
93.00	2529.0
94.00	5459.0
95.00	47712.0
96.00	2977.0
96.90	161.0
103.80	245.0
105.70	269.0
115.90	178.0
116.90	389.0
118.00	214.0
118.80	304.0
127.70	256.0
128.90	114.0
130.10	191.0
131.00	123.0
136.80	221.0
140.90	703.0
142.10	185.0
142.90	615.0
145.10	234.0
147.70	151.0
154.90	172.0
156.80	125.0
157.20	103.0
171.20	169.0
172.00	578.0
173.90	40696.0
175.00	3205.0
175.90	40360.0
177.00	2795.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

Scan 2789 (10.058 min): VV017559.D
BFB64

m/z	Abundance
39.90	405.0
40.60	120.0
42.80	123.0
44.00	325.0
47.50	133.0
99.60	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64