

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
 Data File : VV026865.D
 Acq On : 21 Jul 2022 11:04
 Operator : SY/MD
 Sample : VV0721WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK399

Quant Time: Jul 22 05:54:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 22 05:53:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	221952	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	225362	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	95413	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	92737	4.580	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.600%
7) Chloroethane-d5	1.565	69	86135	4.923	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.400%
11) 1,1-Dichloroethene-d2	2.105	63	134425	3.458	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.200%
20) 2-Butanone-d5	3.889	46	147225	46.587	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.180%
24) Chloroform-d	4.346	84	179873	5.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
26) 1,2-Dichloroethane-d4	5.031	65	79756	5.156	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	5.047	84	336965	4.921	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
36) 1,2-Dichloropropane-d6	6.069	67	107284	5.225	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.600%
41) Toluene-d8	7.313	98	257456	4.235	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.800%
43) trans-1,3-Dichloroprop...	7.625	79	29002	4.317	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.400%
46) 2-Hexanone-d5	8.088	63	118956	40.900	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.800%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	75851	4.742	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	88206	5.306	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.200%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	13498	0.582	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
Data File : VV026865.D
Acq On : 21 Jul 2022 11:04
Operator : SY/MD
Sample : VV0721WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK399


Quant Time: Jul 22 05:54:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 22 05:53:14 2022
Response via : Initial Calibration

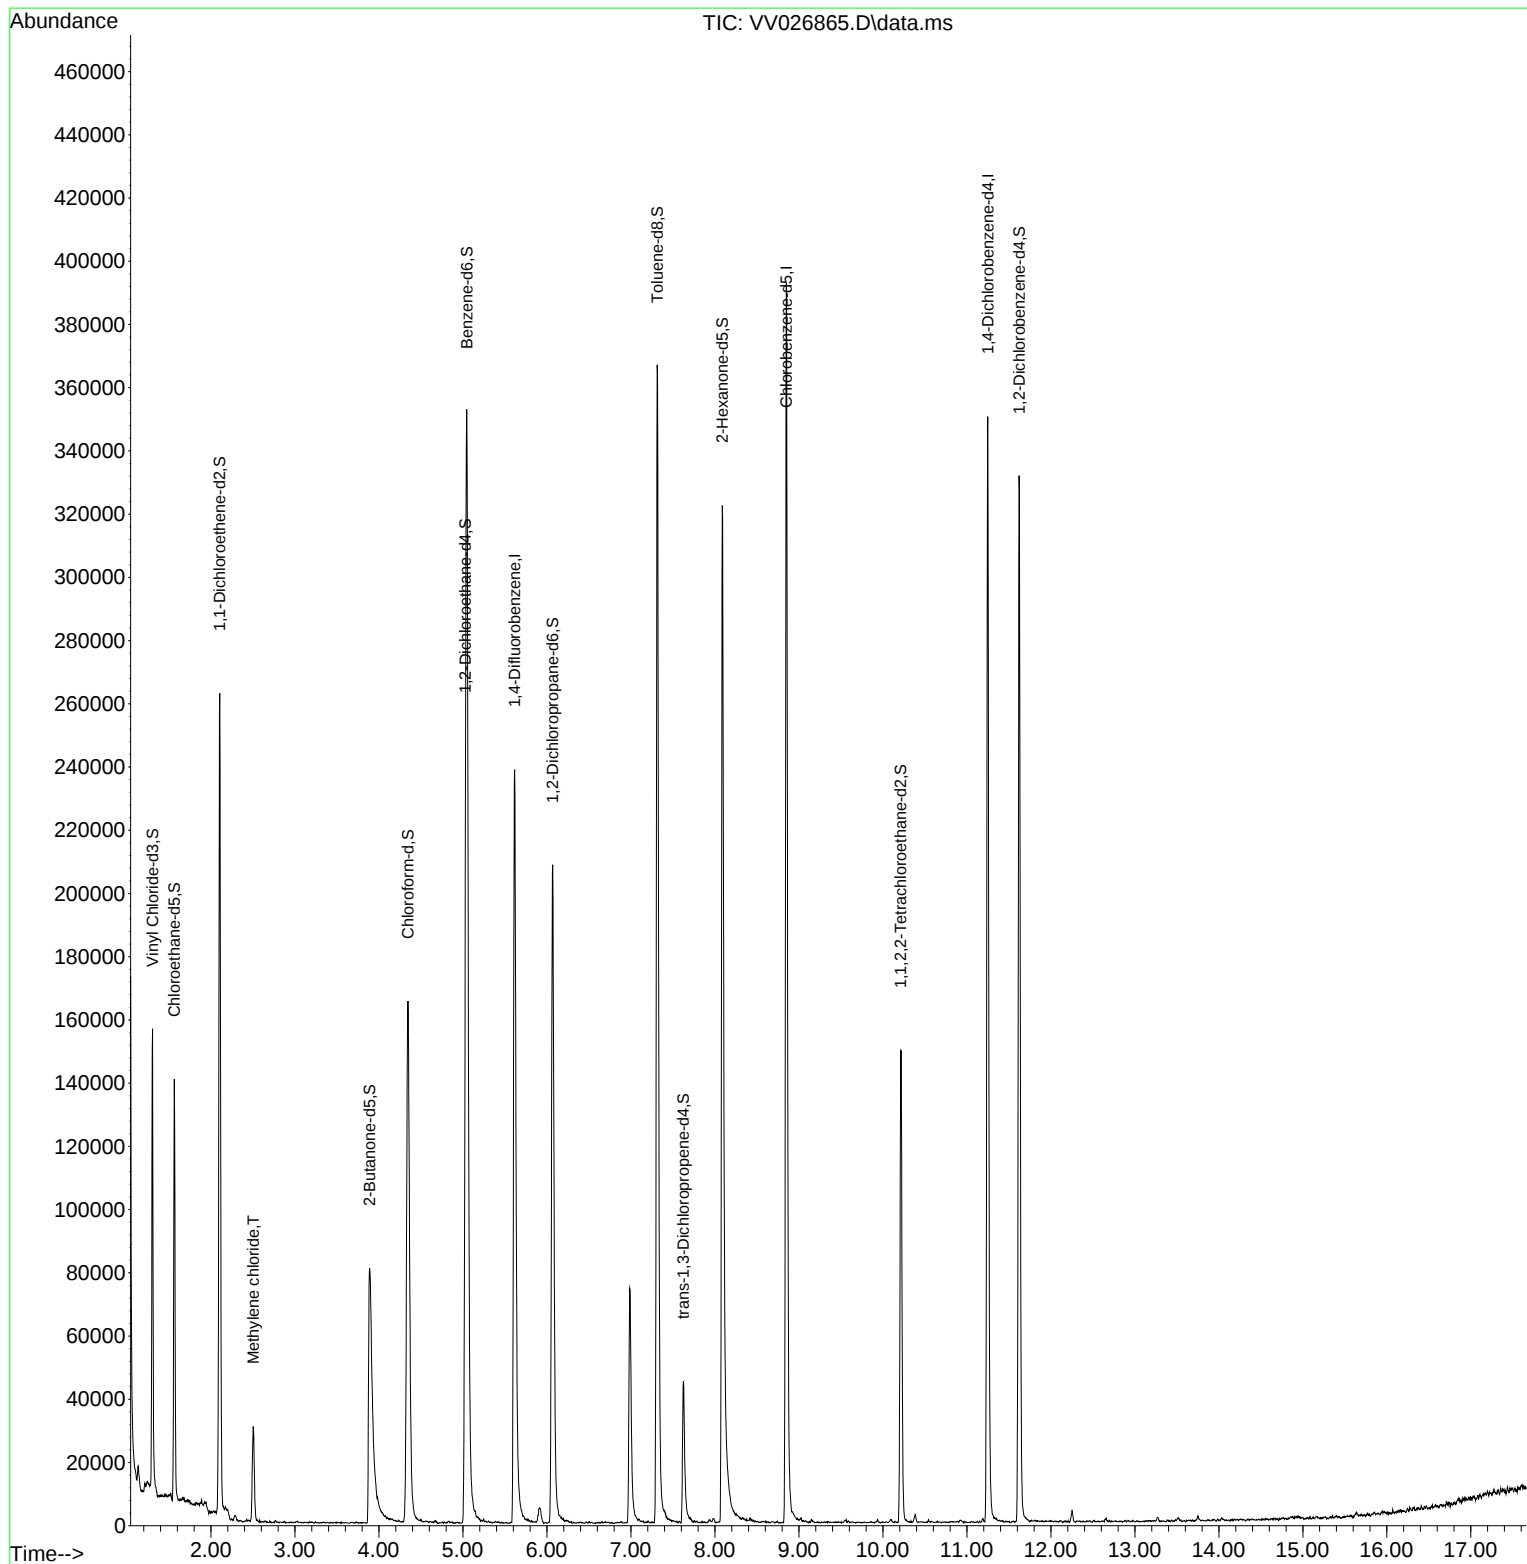

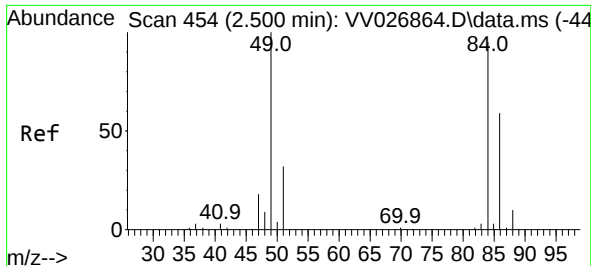

#16
Methylene chloride
Concen: 0.582 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026865.D
Acq: 21 Jul 2022 11:04

Instrument :
MSVOA_V
ClientSampleId :
VBLK399

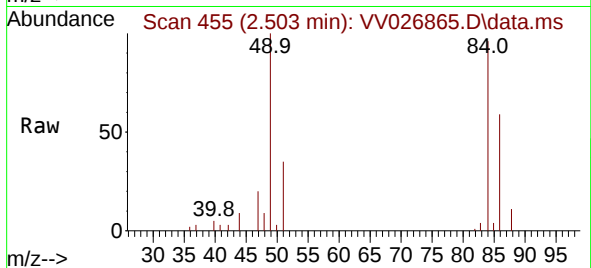

Tgt Ion: 84 Resp: 13498
Ion Ratio Lower Upper
84 100
86 61.1 44.8 83.2
49 104.2 78.7 146.1

