

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW072122\  
 Data File : VW026871.D  
 Acq On : 21 Jul 2022 13:41  
 Operator : SY/MD  
 Sample : N3809-05  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 YBE70

Quant Time: Jul 22 05:55:54 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR071122WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Jul 22 05:53:14 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon           | Response | Conc   | Units    | Dev(Min)  |
|-------------------------------|--------|----------------|----------|--------|----------|-----------|
| -----                         |        |                |          |        |          |           |
| Internal Standards            |        |                |          |        |          |           |
| 1) 1,4-Difluorobenzene        | 5.616  | 114            | 217985   | 5.000  | ug/L     | 0.00      |
| 28) Chlorobenzene-d5          | 8.854  | 117            | 227426   | 5.000  | ug/L     | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152            | 96328    | 5.000  | ug/L     | 0.00      |
| System Monitoring Compounds   |        |                |          |        |          |           |
| 4) Vinyl Chloride-d3          | 1.301  | 65             | 58963    | 2.965  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 59.200%  |           |
| 7) Chloroethane-d5            | 1.565  | 69             | 62767    | 3.653  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 73.000%  |           |
| 11) 1,1-Dichloroethene-d2     | 2.101  | 63             | 82046    | 2.149  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 43.000%# |           |
| 20) 2-Butanone-d5             | 3.889  | 46             | 184015   | 59.288 | ug/L     | 0.00      |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 118.580% |           |
| 24) Chloroform-d              | 4.346  | 84             | 158662   | 4.563  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 91.200%  |           |
| 26) 1,2-Dichloroethane-d4     | 5.031  | 65             | 72096    | 4.746  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 95.000%  |           |
| 32) Benzene-d6                | 5.047  | 84             | 254590   | 3.684  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 73.600%  |           |
| 36) 1,2-Dichloropropane-d6    | 6.069  | 67             | 95820    | 4.624  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 92.400%  |           |
| 41) Toluene-d8                | 7.313  | 98             | 175102   | 2.854  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 57.000%# |           |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79             | 23879    | 3.522  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 70.400%  |           |
| 46) 2-Hexanone-d5             | 8.088  | 63             | 129364   | 44.075 | ug/L     | 0.00      |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 88.160%  |           |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84             | 73376    | 4.546  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 91.000%  |           |
| 66) 1,2-Dichlorobenzene-d4    | 11.625 | 152            | 79976    | 4.765  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 95.400%  |           |
| Target Compounds              |        |                |          |        |          |           |
| 16) Methylene chloride        | 2.503  | 84             | 14760    | 0.648  | ug/L     | Qvalue 97 |
| -----                         |        |                |          |        |          |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072122\  
Data File : VV026871.D  
Acq On : 21 Jul 2022 13:41  
Operator : SY/MD  
Sample : N3809-05  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
YBE70

Quant Time: Jul 22 05:55:54 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR071122WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Jul 22 05:53:14 2022  
Response via : Initial Calibration

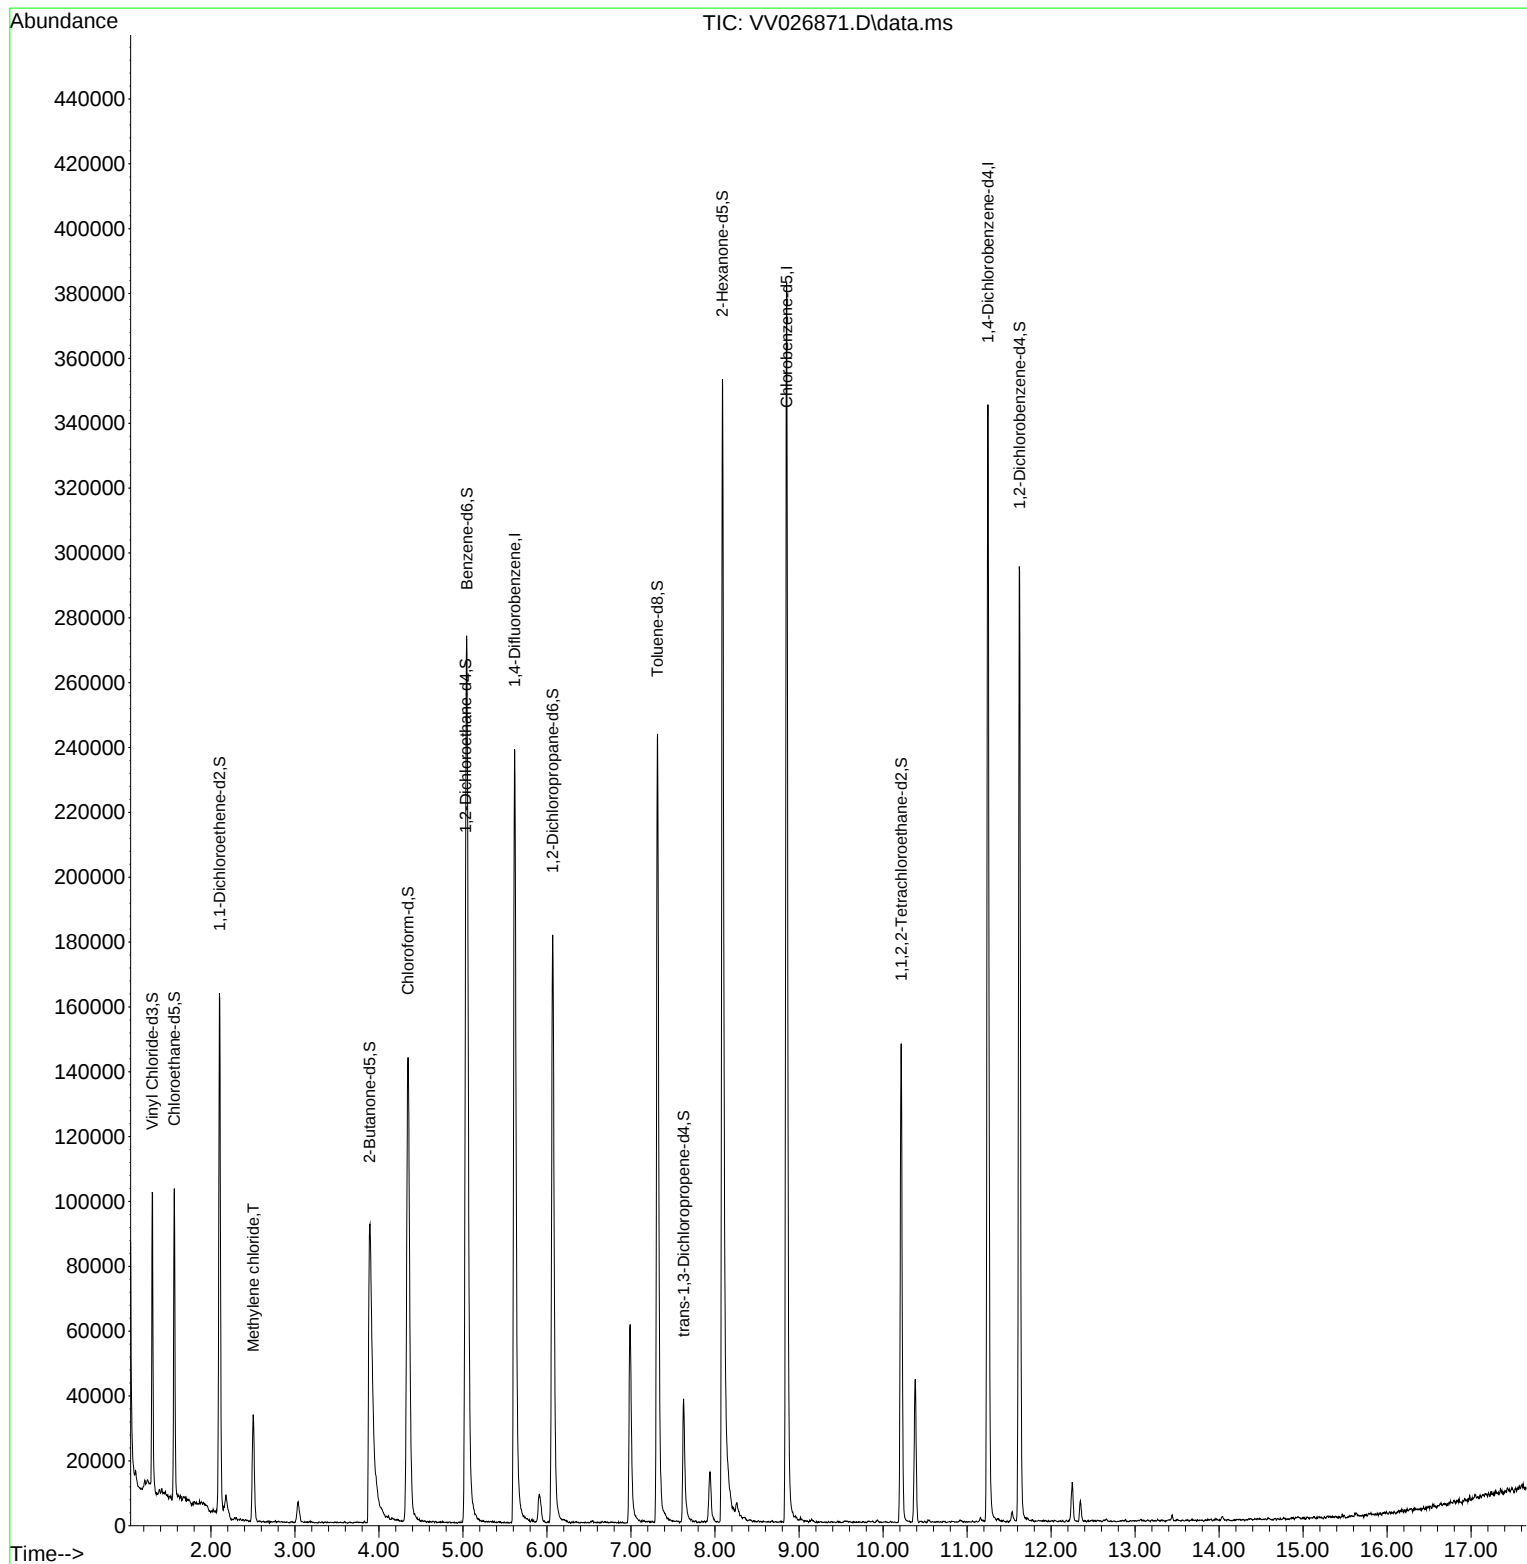

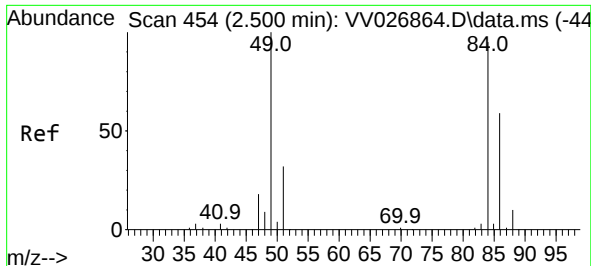

#16  
Methylene chloride  
Concen: 0.648 ug/L  
RT: 2.503 min Scan# 4  
Delta R.T. 0.003 min  
Lab File: VV026871.D  
Acq: 21 Jul 2022 13:41

Instrument :  
MSVOA\_V  
ClientSampleId :  
YBE70

Tgt Ion: 84 Resp: 14760  
Ion Ratio Lower Upper  
84 100  
86 70.0 44.8 83.2  
49 111.2 78.7 146.1

