

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072122\
 Data File : VW026876.D
 Acq On : 21 Jul 2022 15:56
 Operator : SY/MD
 Sample : N3809-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 22 05:57:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 22 05:53:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	221057	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	230133	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	98195	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	95806	4.751	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.561	69	86760	4.979	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.600%
11) 1,1-Dichloroethene-d2	2.101	63	135460	3.499	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.000%
20) 2-Butanone-d5	3.892	46	171048	54.344	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.680%
24) Chloroform-d	4.343	84	185196	5.252	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.000%
26) 1,2-Dichloroethane-d4	5.027	65	79504	5.161	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	5.043	84	352437	5.040	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.800%
36) 1,2-Dichloropropane-d6	6.066	67	111248	5.306	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.200%
41) Toluene-d8	7.313	98	275589	4.440	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	7.622	79	30710	4.477	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.088	63	128735	43.345	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.700%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	75220	4.605	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	93741	5.479	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.600%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	19564	0.847	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
Data File : VV026876.D
Acq On : 21 Jul 2022 15:56
Operator : SY/MD
Sample : N3809-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jul 22 05:57:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 22 05:53:14 2022
Response via : Initial Calibration

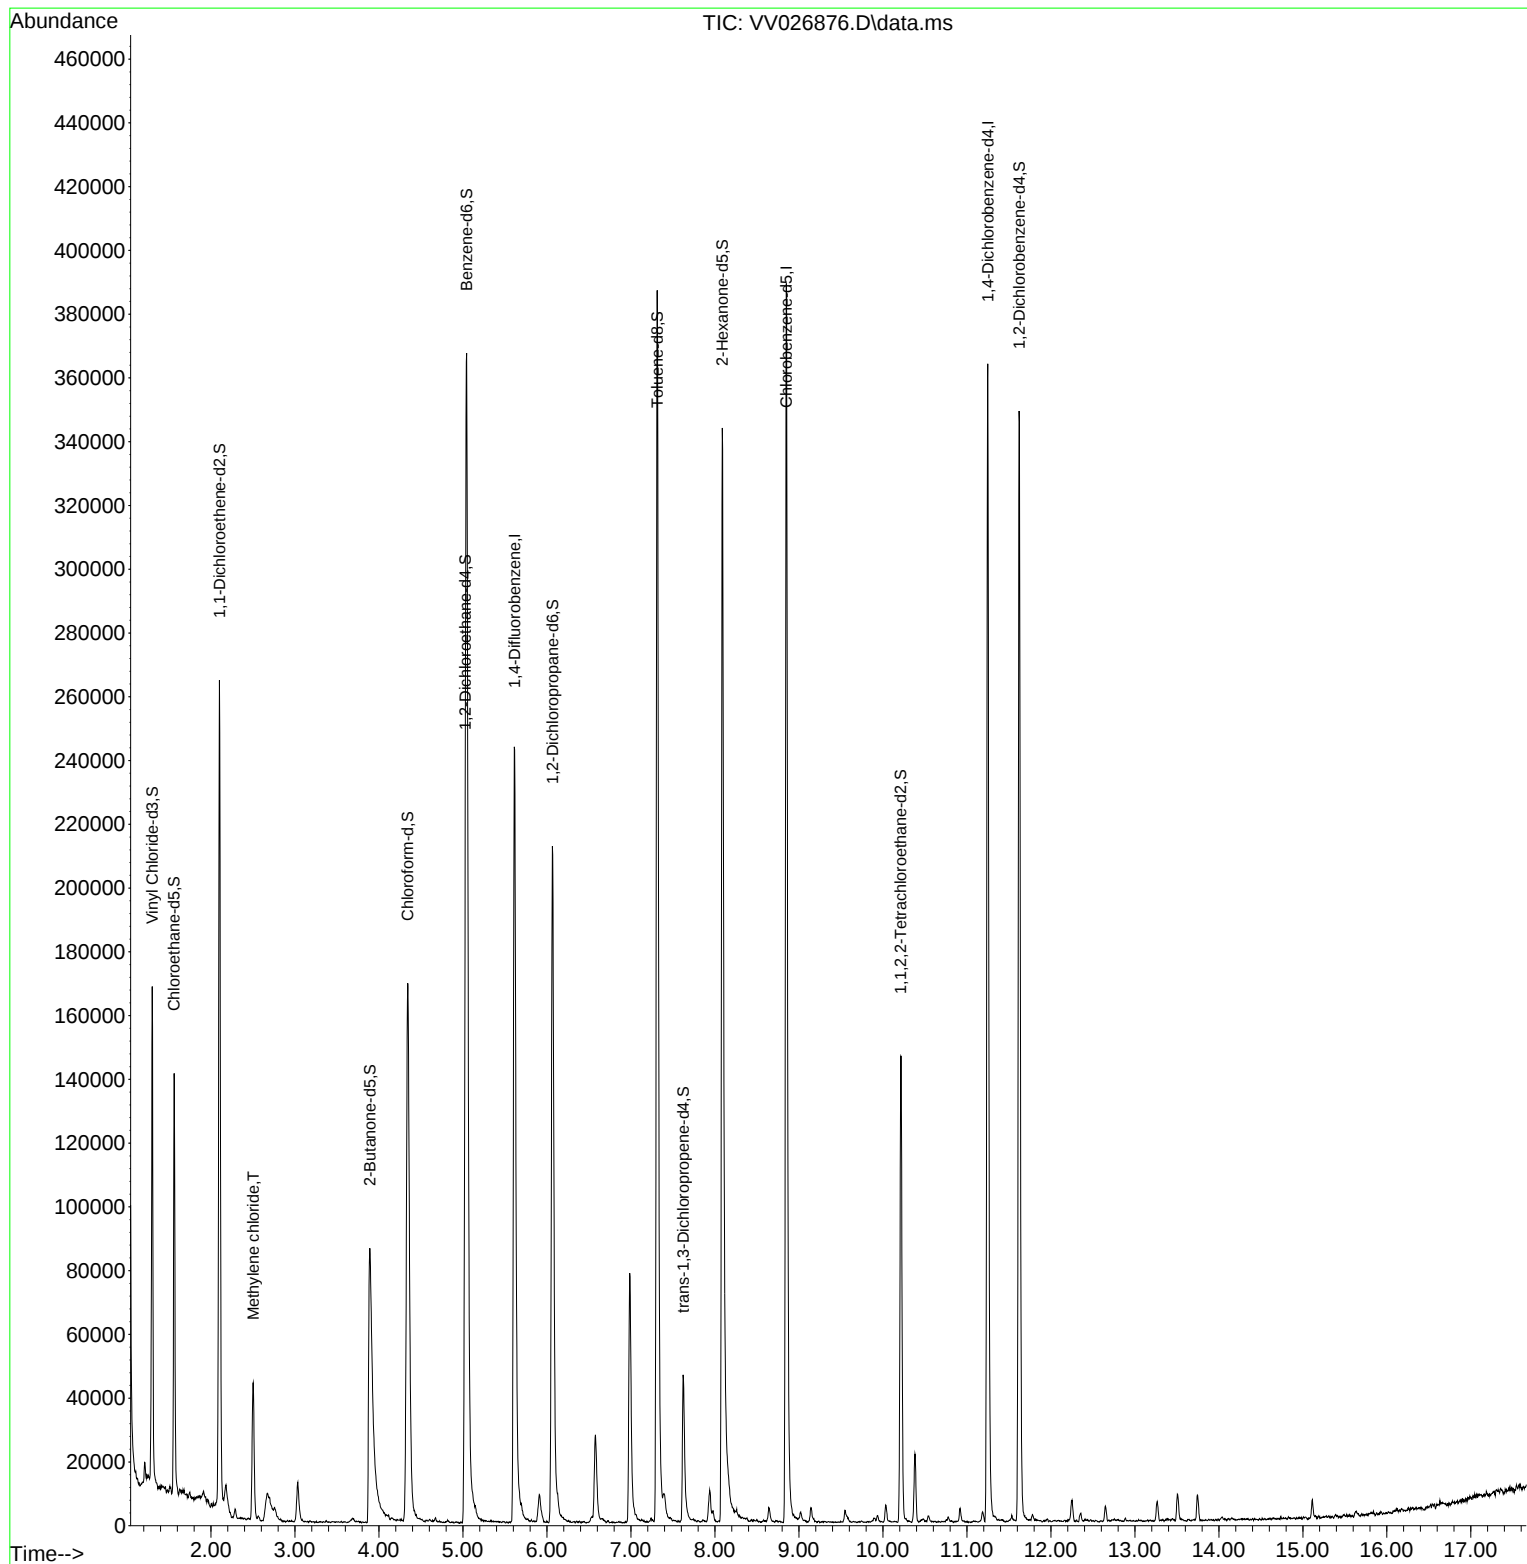

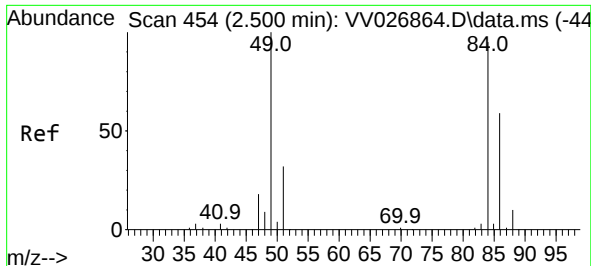

#16
Methylene chloride
Concen: 0.847 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026876.D
Acq: 21 Jul 2022 15:56

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

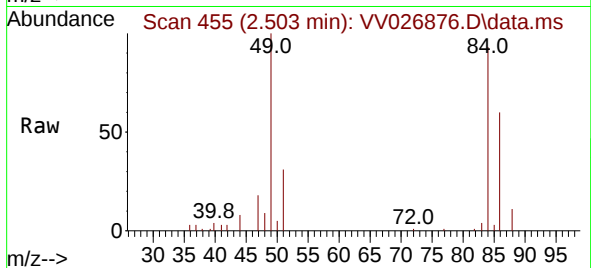

Tgt Ion: 84 Resp: 19564
Ion Ratio Lower Upper
84 100
86 65.0 44.8 83.2
49 107.6 78.7 146.1

