

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
 Data File : VV026869.D
 Acq On : 21 Jul 2022 12:51
 Operator : SY/MD
 Sample : N3802-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBHW6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	103130	112250	6.23%	1.064%
2	1.565	156	163	174	rVB	102154	116898	6.49%	1.108%
3	1.944	271	281	291	rVB2	76451	110634	6.15%	1.049%
4	2.111	320	333	350	rBV2	640129	1126074	62.55%	10.678%
5	2.767	525	537	554	rBV2	26692	56588	3.14%	0.537%
6	3.902	875	890	937	rBV2	221858	742118	41.22%	7.037%
7	4.346	1010	1028	1064	rBV	146965	378583	21.03%	3.590%
8	5.043	1228	1245	1283	rBV2	280784	726319	40.34%	6.887%
9	5.616	1411	1423	1453	rBV	239188	501026	27.83%	4.751%
10	5.912	1501	1515	1551	rBV	911592	1800349	100.00%	17.072%
11	6.069	1551	1564	1592	rVB	189987	397766	22.09%	3.772%
12	6.989	1839	1850	1873	rBV	63434	125168	6.95%	1.187%
13	7.317	1940	1952	1977	rBV	251467	467508	25.97%	4.433%
14	7.625	2038	2048	2064	rBV2	37746	71438	3.97%	0.677%
15	7.973	2132	2156	2182	rBV	610172	1041748	57.86%	9.878%
16	8.088	2182	2192	2234	rBV	403598	786992	43.71%	7.463%
17	8.850	2418	2429	2453	rBV	391021	649153	36.06%	6.156%
18	10.214	2840	2853	2870	rBV	163654	260277	14.46%	2.468%
19	10.384	2895	2906	2917	rBV	20590	34280	1.90%	0.325%
20	11.249	3164	3175	3194	rBV	360418	556854	30.93%	5.280%
21	11.622	3279	3291	3310	rBV	298145	483818	26.87%	4.588%




Sum of corrected areas: 10545841

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
Data File : VV026869.D
Acq On : 21 Jul 2022 12:51
Operator : SY/MD
Sample : N3802-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBHW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

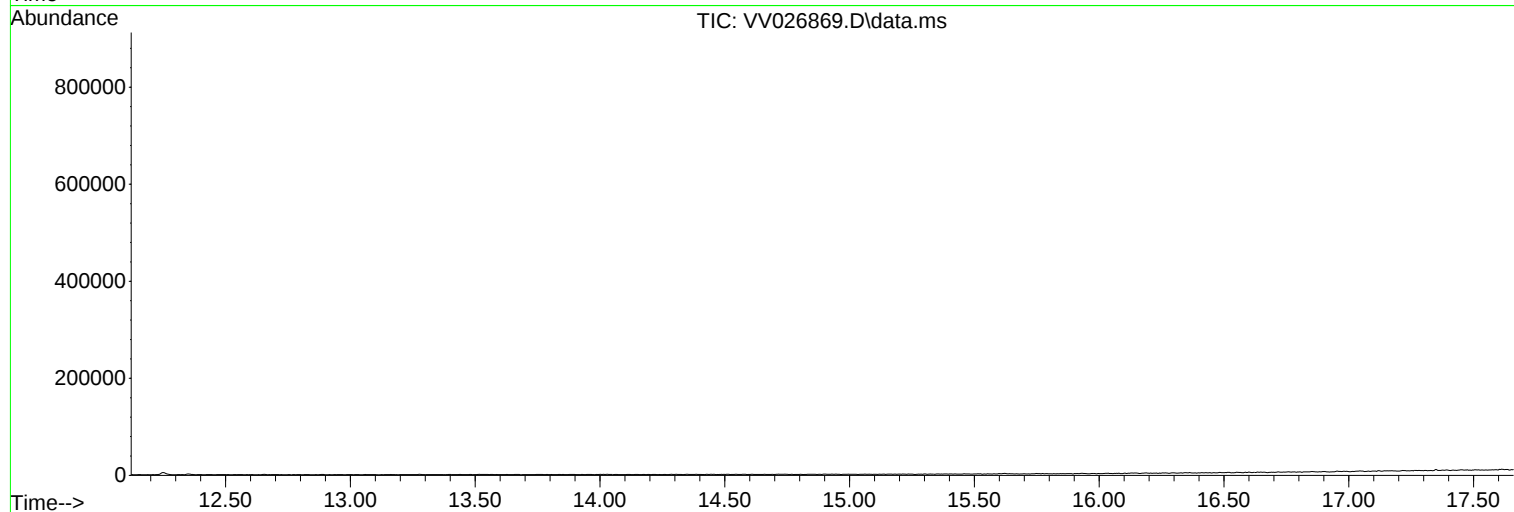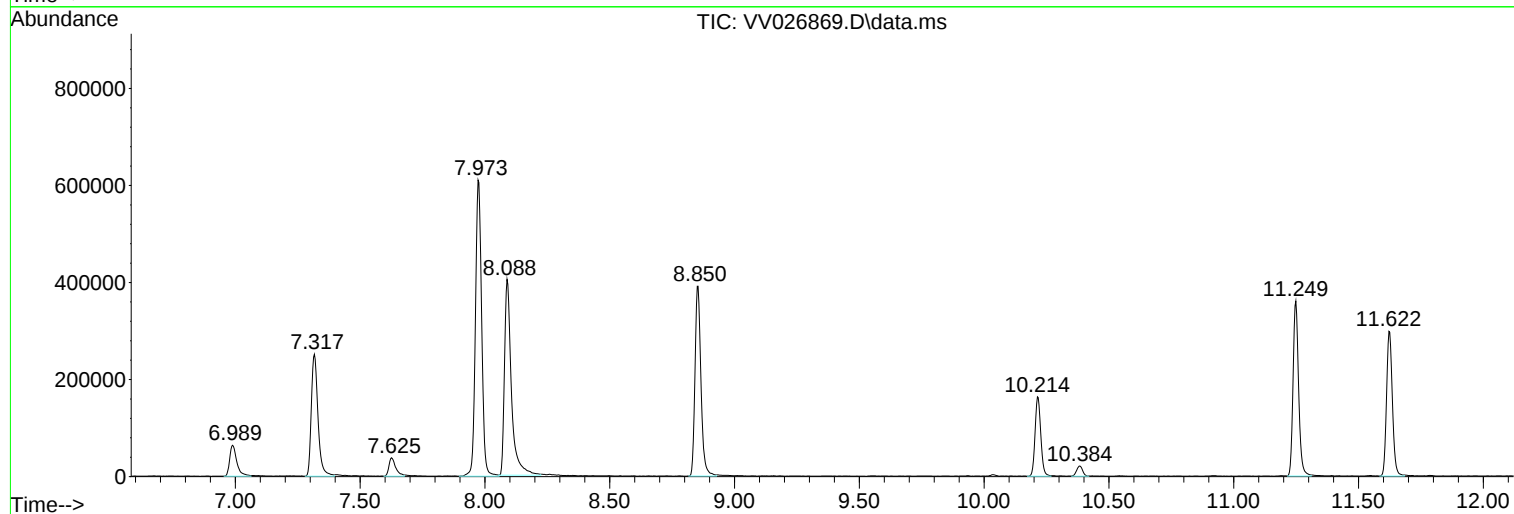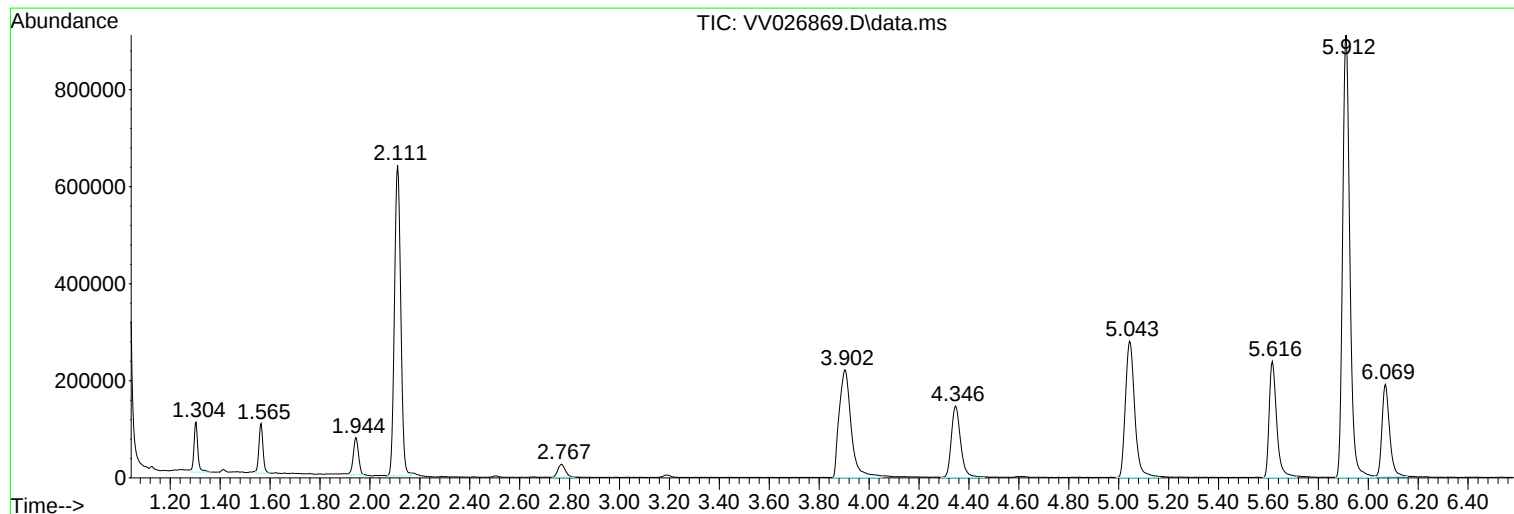

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
Data File : VV026869.D
Acq On : 21 Jul 2022 12:51
Operator : SY/MD
Sample : N3802-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBHW6









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,2-dichloro-1,1,2-... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.944	1.10 ug/L	110634	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	91
2			Methyl 2-butynoate	98	C5H6O2	023326-27-4	9
3			Cyclopropane, 1,2-dimethyl-3-met...	82	C6H10	062338-02-7	9
4			1,4-Pentadiene, 3-methyl-	82	C6H10	001115-08-8	9
5			Fluorodichloromethane	102	CHCl2F	000075-43-4	9

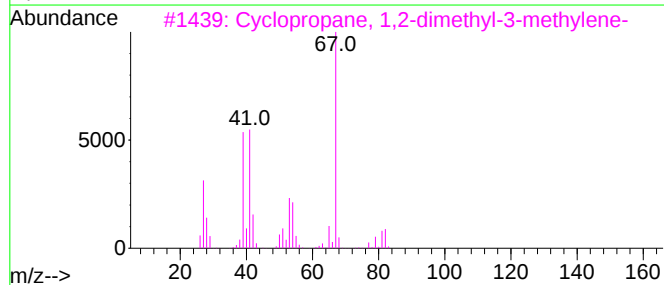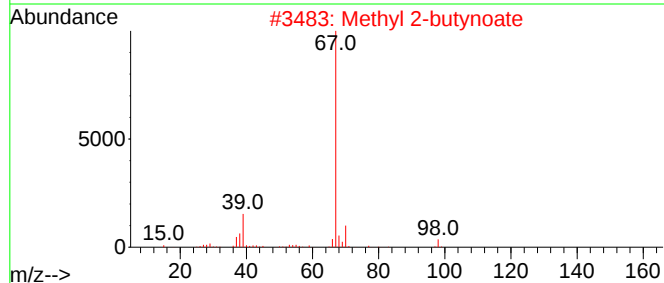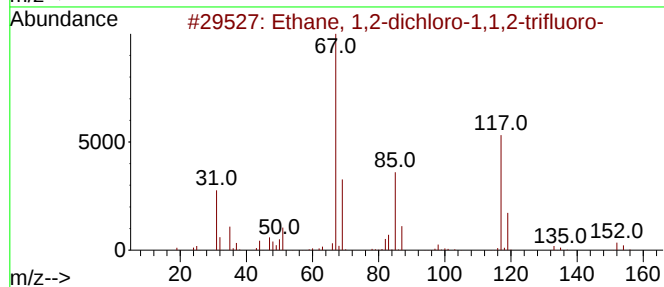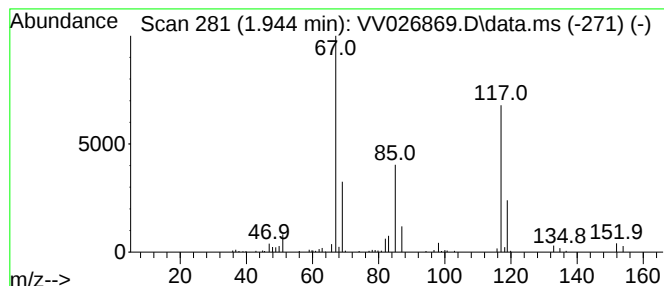

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
Data File : VV026869.D
Acq On : 21 Jul 2022 12:51
Operator : SY/MD
Sample : N3802-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBHW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,2-dic...	1.944	1.1	ug/L	110634	1	5.616	501026	5.0