
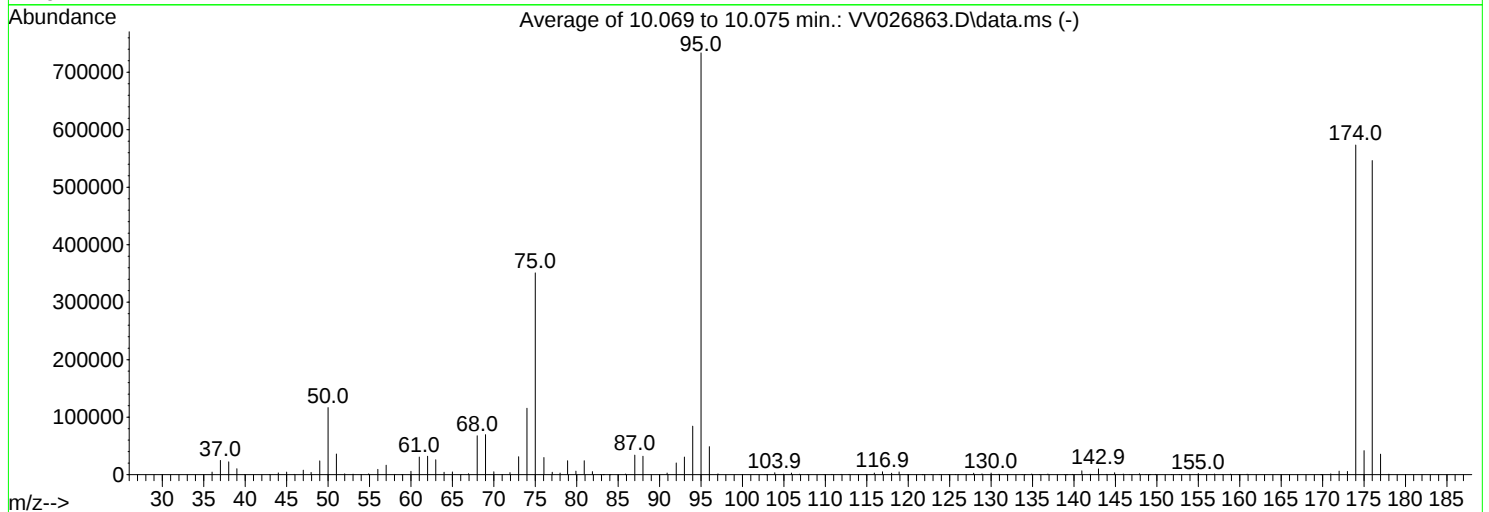


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072122\
Data File : VV026863.D
Acq On : 21 Jul 2022 09:33
Operator : SY/MD
Sample : BFB350
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB350

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jul 22 05:53:14 2022

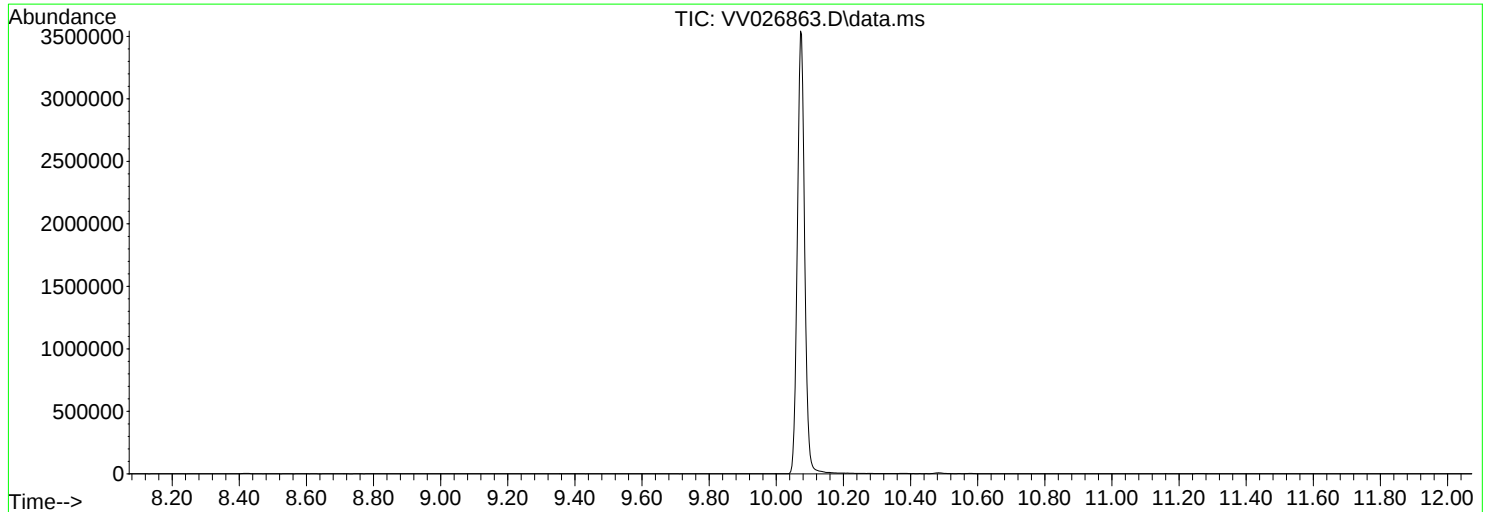

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	116640	PASS
75	95	30	80	47.8	351061	PASS
95	95	100	100	100.0	733803	PASS
96	95	5	9	6.6	48704	PASS
173	174	0.00	2	1.0	5723	PASS
174	95	50	120	78.2	573547	PASS
175	174	5	9	7.3	41811	PASS
176	174	95	105	95.3	546389	PASS
177	176	5	10	6.5	35587	PASS

m/z	Abundance
39.90	425.0
44.00	472.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

m/z	Abundance
36.00	4094.0
37.00	23464.0
38.00	21552.0
39.00	9793.0
40.00	847.0
42.90	319.0
44.00	3355.0
45.00	4244.0
45.90	745.0
47.00	7640.0
47.90	3828.0
49.00	22720.0
50.00	109280.0
51.00	34688.0
52.00	1511.0
53.00	802.0
54.00	452.0
54.90	1493.0
56.00	9062.0
57.00	15040.0
58.00	669.0
59.00	130.0
60.00	5490.0
61.00	29352.0
62.00	30720.0
63.00	24992.0
64.00	4443.0
65.00	5046.0
66.10	440.0
67.00	1478.0
68.00	64000.0
69.00	65568.0
70.00	4883.0
70.90	189.0
72.00	3606.0
73.00	29912.0
74.00	107936.0
75.00	330496.0
76.10	28784.0
77.00	3993.0
78.00	2594.0
78.90	23992.0
79.90	6096.0
80.90	23768.0
81.90	4824.0
82.90	454.0
85.90	977.0
87.00	31624.0
88.00	30216.0
90.90	2461.0
92.00	18824.0
93.00	28784.0
94.00	78768.0
95.00	683648.0
96.00	45600.0
97.10	1677.0
102.70	302.0
103.90	2856.0
104.90	785.0
105.90	2736.0
106.90	684.0
107.80	414.0
109.90	371.0
110.80	619.0
111.90	540.0
112.80	465.0
114.90	634.0
115.90	2553.0
116.90	4830.0
118.00	2442.0
118.90	4480.0
120.00	126.0
121.70	136.0
122.00	129.0
122.80	208.0
123.80	331.0
124.80	194.0
125.70	310.0
127.00	235.0
127.90	2261.0
128.90	1114.0
130.00	2556.0
130.90	878.0
131.90	133.0
133.80	147.0
134.00	149.0
134.90	926.0
135.80	172.0
136.90	1042.0
138.90	256.0
139.90	493.0
141.00	6383.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

141.90	864.0
142.90	9706.0
144.00	813.0
144.90	3823.0
145.90	1036.0
146.70	345.0
147.90	1473.0
148.70	327.0
149.90	586.0
151.80	350.0
152.80	369.0
154.00	477.0
155.00	1791.0
156.00	216.0
156.90	1152.0
157.90	144.0
158.90	770.0
160.90	716.0
169.80	137.0
171.00	1368.0
172.00	6073.0
173.00	5429.0
174.00	520832.0
175.00	39208.0
176.00	494400.0
177.00	33040.0
178.00	874.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

m/z	Abundance
36.00	4545.0
37.00	25744.0
38.00	23128.0
39.00	10608.0
40.00	770.0
42.90	259.0
44.00	3561.0
45.00	4578.0
45.90	656.0
47.00	8121.0
48.00	4193.0
49.00	24864.0
50.00	121456.0
51.00	37416.0
52.00	1613.0
53.00	790.0
54.00	434.0
54.90	1615.0
56.00	9571.0
57.00	16880.0
58.10	701.0
58.90	122.0
60.00	6057.0
61.00	31680.0
62.00	33280.0
63.00	26928.0
64.00	4258.0
65.00	5011.0
66.10	440.0
67.00	1650.0
68.00	70416.0
69.00	72440.0
70.00	5133.0
71.00	183.0
72.00	3823.0
73.00	32472.0
74.00	120000.0
75.00	365632.0
76.10	31048.0
77.10	4400.0
78.00	2788.0
78.90	25176.0
79.90	6540.0
80.90	25264.0
81.90	5504.0
82.90	462.0
84.00	128.0
85.90	1103.0
87.00	35288.0
88.00	33304.0
90.90	2832.0
92.00	21360.0
93.00	31584.0
94.00	87752.0
95.00	762304.0
96.00	50704.0
97.10	1629.0
102.70	342.0
103.90	3371.0
105.00	956.0
105.90	2935.0
106.90	783.0
107.90	378.0
109.80	432.0
110.80	696.0
111.90	615.0
112.80	595.0
114.90	669.0
115.90	2821.0
116.90	5225.0
118.00	2630.0
118.90	4878.0
120.00	147.0
122.00	172.0
122.80	226.0
123.80	422.0
124.90	204.0
125.70	276.0
126.10	284.0
127.00	242.0
127.90	2648.0
128.90	1353.0
130.00	2981.0
130.90	1037.0
131.90	150.0
133.70	172.0
134.90	1122.0
135.80	214.0
136.80	1230.0
138.80	257.0
139.90	579.0
141.00	6993.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

141.90	959.0
142.90	10182.0
144.00	762.0
144.90	3493.0
146.00	1121.0
146.80	449.0
147.90	1768.0
148.70	406.0
149.90	576.0
151.80	394.0
152.70	413.0
154.00	495.0
155.00	1984.0
155.90	326.0
156.90	1304.0
157.90	181.0
158.90	837.0
159.90	107.0
160.90	884.0
169.80	141.0
171.00	1344.0
172.00	6502.0
173.00	5903.0
174.00	595520.0
175.00	43464.0
176.00	567232.0
177.00	36848.0
178.00	919.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

m/z	Abundance
36.00	4582.0
37.00	25096.0
38.00	22120.0
39.00	10319.0
39.90	729.0
43.00	220.0
44.00	3583.0
45.00	4503.0
45.90	551.0
47.00	7668.0
48.00	4110.0
49.00	24184.0
50.00	119184.0
51.00	35968.0
52.00	1405.0
53.00	631.0
54.00	389.0
54.90	1549.0
56.00	8942.0
57.00	17224.0
58.10	649.0
58.80	123.0
60.00	5959.0
61.00	30672.0
62.00	31736.0
63.00	25864.0
64.00	3633.0
65.00	4440.0
66.00	454.0
66.90	1637.0
68.00	68632.0
69.00	70712.0
70.00	5093.0
71.10	228.0
71.90	3549.0
73.00	31488.0
74.00	118736.0
75.00	357056.0
76.00	29856.0
77.10	4165.0
78.00	2747.0
78.90	23832.0
79.90	6176.0
80.90	24072.0
81.90	5415.0
82.90	417.0
83.20	466.0
84.00	148.0
85.90	1052.0
87.00	34992.0
88.00	32512.0
90.90	2805.0
92.00	21248.0
93.00	31688.0
94.00	86320.0
95.00	755456.0
96.00	49808.0
97.00	1347.0
102.90	327.0
103.90	3500.0
105.00	993.0
105.90	2841.0
106.90	788.0
107.90	358.0
109.80	431.0
110.80	716.0
111.90	582.0
112.90	607.0
114.90	650.0
115.90	2676.0
116.90	5085.0
118.00	2586.0
118.90	4587.0
119.90	152.0
122.00	186.0
122.80	224.0
123.80	465.0
125.00	187.0
126.10	284.0
127.00	233.0
127.90	2815.0
128.90	1407.0
130.00	2982.0
131.00	1018.0
131.90	128.0
133.70	166.0
134.90	1169.0
135.90	258.0
136.80	1363.0
139.10	240.0
139.80	555.0
140.90	7006.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350

142.00	940.0
143.00	9955.0
143.90	593.0
144.90	2699.0
145.90	1024.0
146.80	464.0
147.90	1927.0
148.70	400.0
149.10	391.0
149.80	542.0
151.80	386.0
152.70	480.0
153.90	440.0
155.00	1919.0
155.90	400.0
157.00	1364.0
157.90	191.0
158.90	798.0
159.90	118.0
160.90	892.0
169.80	158.0
171.00	1142.0
172.00	6144.0
173.00	5837.0
174.00	604288.0
175.00	42760.0
176.00	577536.0
177.00	36872.0
178.00	947.0

Instrument :
MSVOA_V
ClientSampleId :
BFB350