
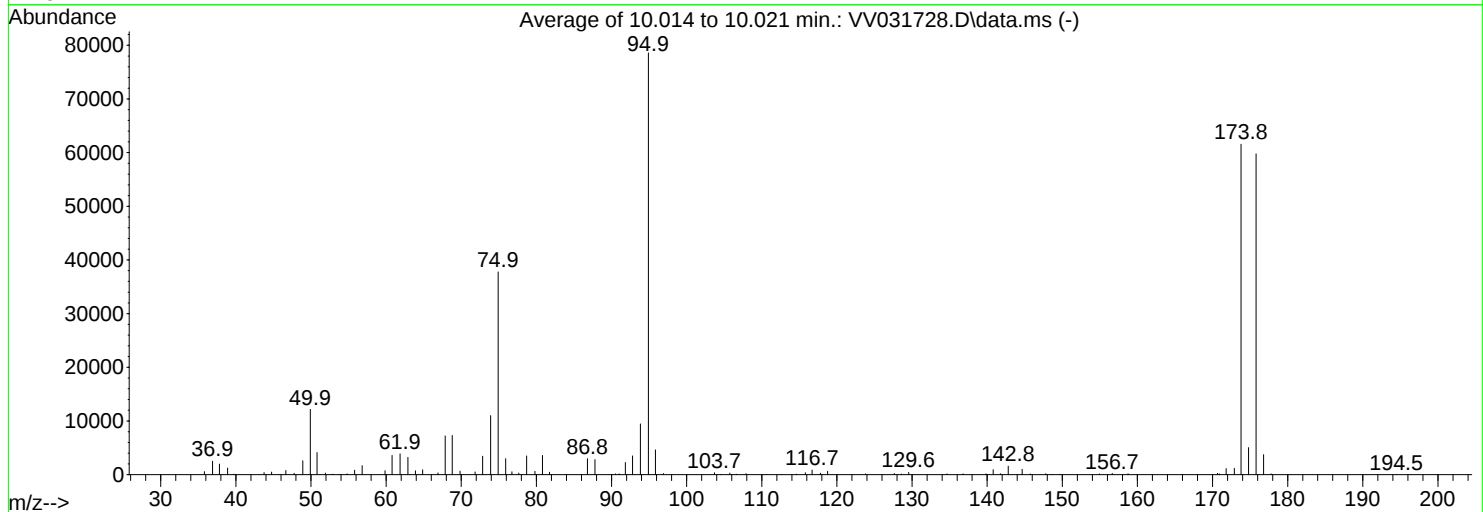


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072123\
Data File : VV031728.D
Acq On : 21 Jul 2023 11:06
Operator : SY/MD
Sample : BFB243
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB243

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM071923.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 20 05:08:22 2023

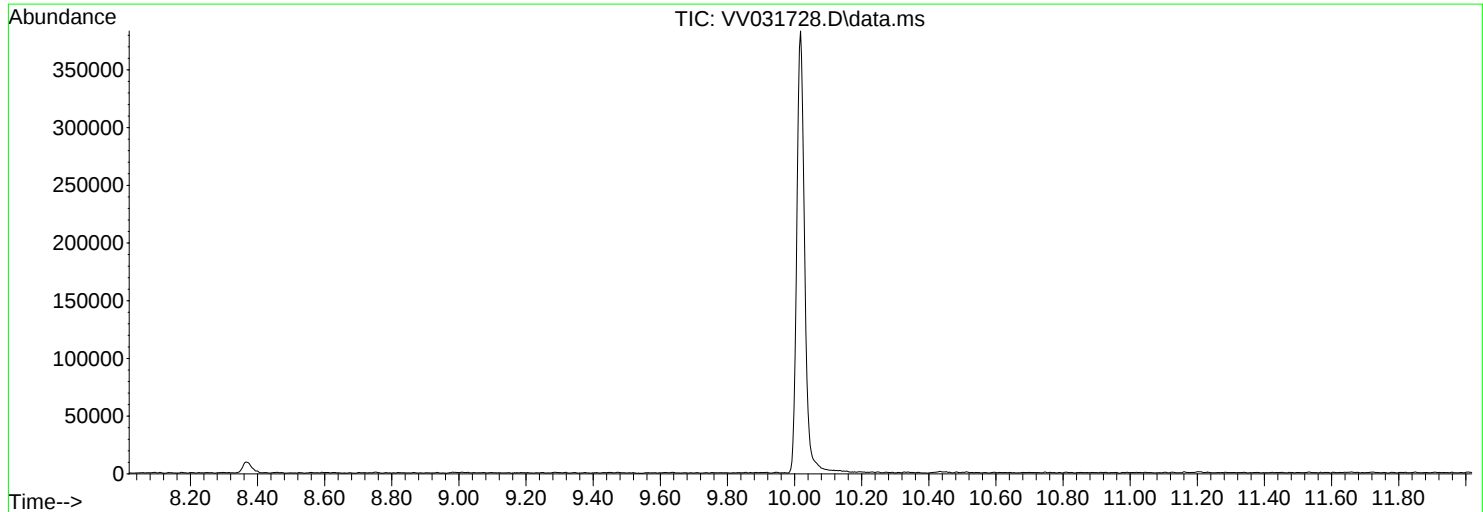

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	12159	PASS
75	95	30	80	48.1	37779	PASS
95	95	100	100	100.0	78587	PASS
96	95	5	9	5.9	4626	PASS
173	174	0.00	2	1.9	1187	PASS
174	95	50	120	78.3	61568	PASS
175	174	5	9	8.2	5042	PASS
176	174	95	101	97.1	59768	PASS
177	176	5	9	6.2	3729	PASS

m/z	Abundance
39.70	215.0
43.70	658.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
35.80	646.0
36.90	2612.0
37.80	2230.0
38.90	1353.0
39.80	265.0
43.80	907.0
44.80	458.0
46.70	768.0
47.80	394.0
48.90	2956.0
49.90	12023.0
50.80	4096.0
51.90	238.0
54.80	195.0
55.80	879.0
56.80	1737.0
59.90	757.0
60.80	3409.0
61.90	3872.0
62.90	3630.0
63.90	743.0
64.90	908.0
66.90	335.0
67.90	7122.0
68.80	7445.0
69.80	706.0
71.90	522.0
72.80	3539.0
73.90	11334.0
74.90	37888.0
75.90	2805.0
76.80	565.0
77.70	336.0
78.70	3533.0
79.80	621.0
80.80	3358.0
81.70	410.0
86.80	3125.0
87.80	3206.0
90.60	179.0
91.80	2251.0
92.80	3460.0
93.80	9400.0
94.90	78696.0
95.90	4902.0
96.90	268.0
103.70	387.0
105.80	258.0
107.90	118.0
112.70	106.0
114.60	146.0
115.80	370.0
116.70	910.0
117.80	253.0
118.80	678.0
123.80	217.0
127.60	195.0
128.60	130.0
129.70	443.0
134.60	124.0
136.90	129.0
139.80	115.0
140.80	1004.0
141.80	172.0
142.90	1404.0
144.60	867.0
147.80	180.0
154.90	150.0
156.70	239.0
158.70	152.0
170.60	333.0
171.80	952.0
172.90	1266.0
173.80	59896.0
174.80	4560.0
175.80	58200.0
176.80	3622.0
177.80	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
35.80	626.0
36.90	2577.0
37.80	1968.0
38.90	1266.0
39.90	305.0
43.80	1097.0
44.70	506.0
46.60	777.0
47.70	383.0
48.90	2740.0
49.90	12569.0
50.80	4280.0
51.90	317.0
52.90	116.0
54.80	164.0
55.80	866.0
56.80	1719.0
59.80	718.0
60.80	3708.0
61.90	3979.0
62.90	3306.0
63.90	792.0
64.80	936.0
66.90	365.0
67.80	7404.0
68.80	7398.0
69.80	671.0
71.80	526.0
72.90	3518.0
73.90	11124.0
74.90	39104.0
75.90	3087.0
76.80	522.0
77.70	299.0
78.70	3569.0
79.80	650.0
80.80	3711.0
81.80	445.0
86.80	3067.0
87.80	2741.0
90.60	130.0
91.00	212.0
91.80	2358.0
92.80	3648.0
93.90	9889.0
94.90	81720.0
95.90	4680.0
96.90	198.0
103.70	358.0
105.80	306.0
106.60	142.0
107.90	195.0
114.60	123.0
115.80	354.0
116.70	907.0
117.80	266.0
118.80	637.0
123.80	160.0
127.70	208.0
128.60	116.0
129.50	444.0
134.70	139.0
136.80	129.0
139.90	151.0
140.80	924.0
141.80	194.0
142.80	1631.0
144.70	1033.0
145.80	150.0
147.80	165.0
155.00	156.0
156.70	250.0
158.70	193.0
170.70	391.0
171.80	1150.0
172.90	1199.0
173.80	63840.0
174.80	5276.0
175.80	61784.0
176.80	3826.0
177.80	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
35.80	475.0
36.90	2345.0
37.80	1691.0
38.90	1044.0
39.90	367.0
43.80	1149.0
44.70	519.0
45.70	126.0
46.60	799.0
48.90	2101.0
49.90	11885.0
50.80	4004.0
51.90	328.0
52.90	161.0
53.80	165.0
54.80	104.0
55.80	789.0
56.80	1549.0
59.80	744.0
60.80	3577.0
61.80	3771.0
62.90	2767.0
63.90	658.0
64.80	858.0
66.90	321.0
67.80	7098.0
68.80	7074.0
69.90	591.0
71.80	488.0
72.90	3250.0
73.90	10505.0
74.90	36344.0
75.90	3061.0
76.70	525.0
77.60	253.0
78.70	3373.0
79.80	619.0
80.80	3659.0
81.80	471.0
86.80	2761.0
87.80	2466.0
90.50	156.0
91.00	247.0
91.90	2163.0
92.80	3379.0
93.90	9088.0
94.90	75344.0
95.80	4295.0
96.90	122.0
103.70	341.0
104.50	104.0
105.70	326.0
106.60	157.0
107.90	234.0
110.60	109.0
115.80	331.0
116.70	767.0
117.80	299.0
118.70	613.0
123.80	101.0
127.70	267.0
128.60	115.0
129.50	414.0
134.70	187.0
136.70	155.0
139.90	160.0
140.80	807.0
141.70	172.0
142.70	1746.0
144.70	1069.0
145.70	204.0
147.80	163.0
148.70	120.0
149.70	131.0
154.90	140.0
156.60	212.0
158.80	223.0
170.90	453.0
171.80	1279.0
172.90	1096.0
173.80	60968.0
174.80	5290.0
175.80	59320.0
176.80	3738.0
177.80	134.0
194.50	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243