

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072219\
 Data File : VV011956.D
 Acq On : 22 Jul 2019 19:12
 Operator : SY/MD
 Sample : K3823-19 50X
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A52J8

Quant Time: Jul 23 07:36:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 23 07:18:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	137774	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	133515	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	63701	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	33728	4.71	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.20%
7) Chloroethane-d5	1.59	69	26702	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.80%
11) 1,1-Dichloroethene-d2	2.13	63	53787	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.96	46	105082	50.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.40%
24) Chloroform-d	4.40	84	88225	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.08	65	49000	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
32) Benzene-d6	5.10	84	180284	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.12	67	51110	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.36	98	158358	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.67	79	19727	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
46) 2-Hexanone-d5	8.13	63	85870	49.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.90%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35528	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	63501	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
19) 1,1-Dichloroethane	3.23	63	6422	0.372 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072219\
Data File : VV011956.D
Acq On : 22 Jul 2019 19:12
Operator : SY/MD
Sample : K3823-19 50X
Misc : 25ML/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52J8

Quant Time: Jul 23 07:36:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 23 07:18:43 2019
Response via : Initial Calibration

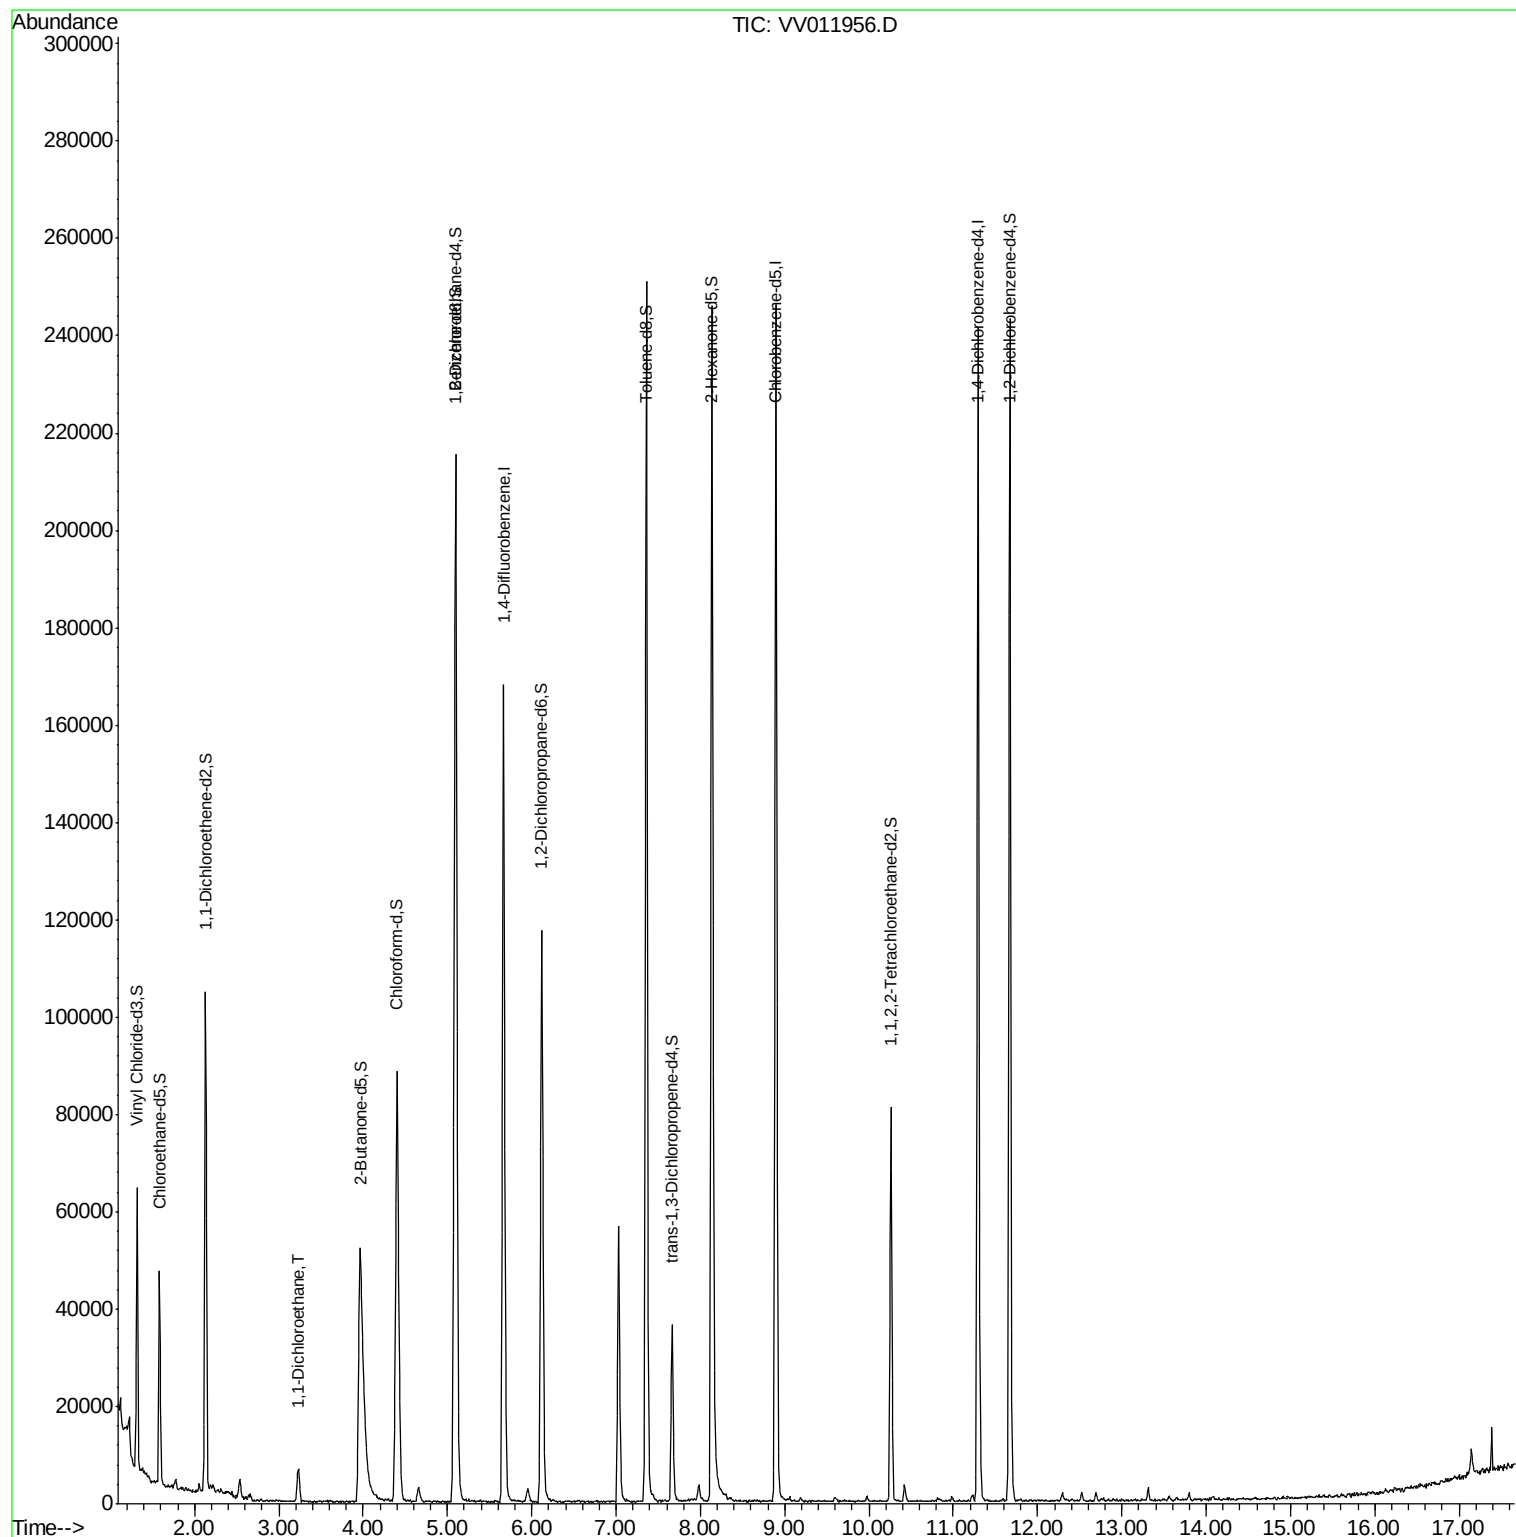

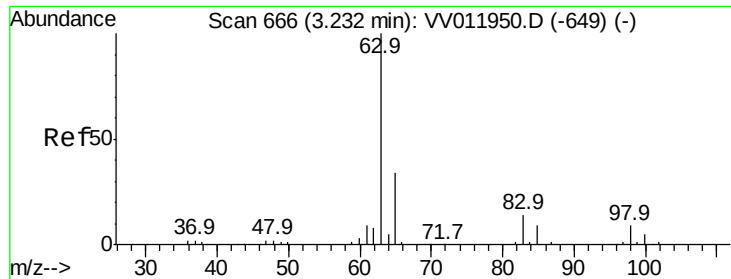

#19

1,1-Dichloroethane

Concen: 0.372 ug/L

RT: 3.23 min Scan# 666

Delta R.T. -0.00 min

Lab File: VV011956.D

Acq: 22 Jul 2019 19:12

Instrument :

MSVOA_V

ClientSampleId :

A52J8

Tot Ion: 63 Resp: 6422

Ion Ratio Lower Upper

63 100

65 33.9 23.5 43.7

83 15.6 9.7 18.1

