


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072219\
 Data File : VV011947.D
 Acq On : 22 Jul 2019 14:23
 Operator : SY/MD
 Sample : BFB36
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB36

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 25 04:12:02 2019

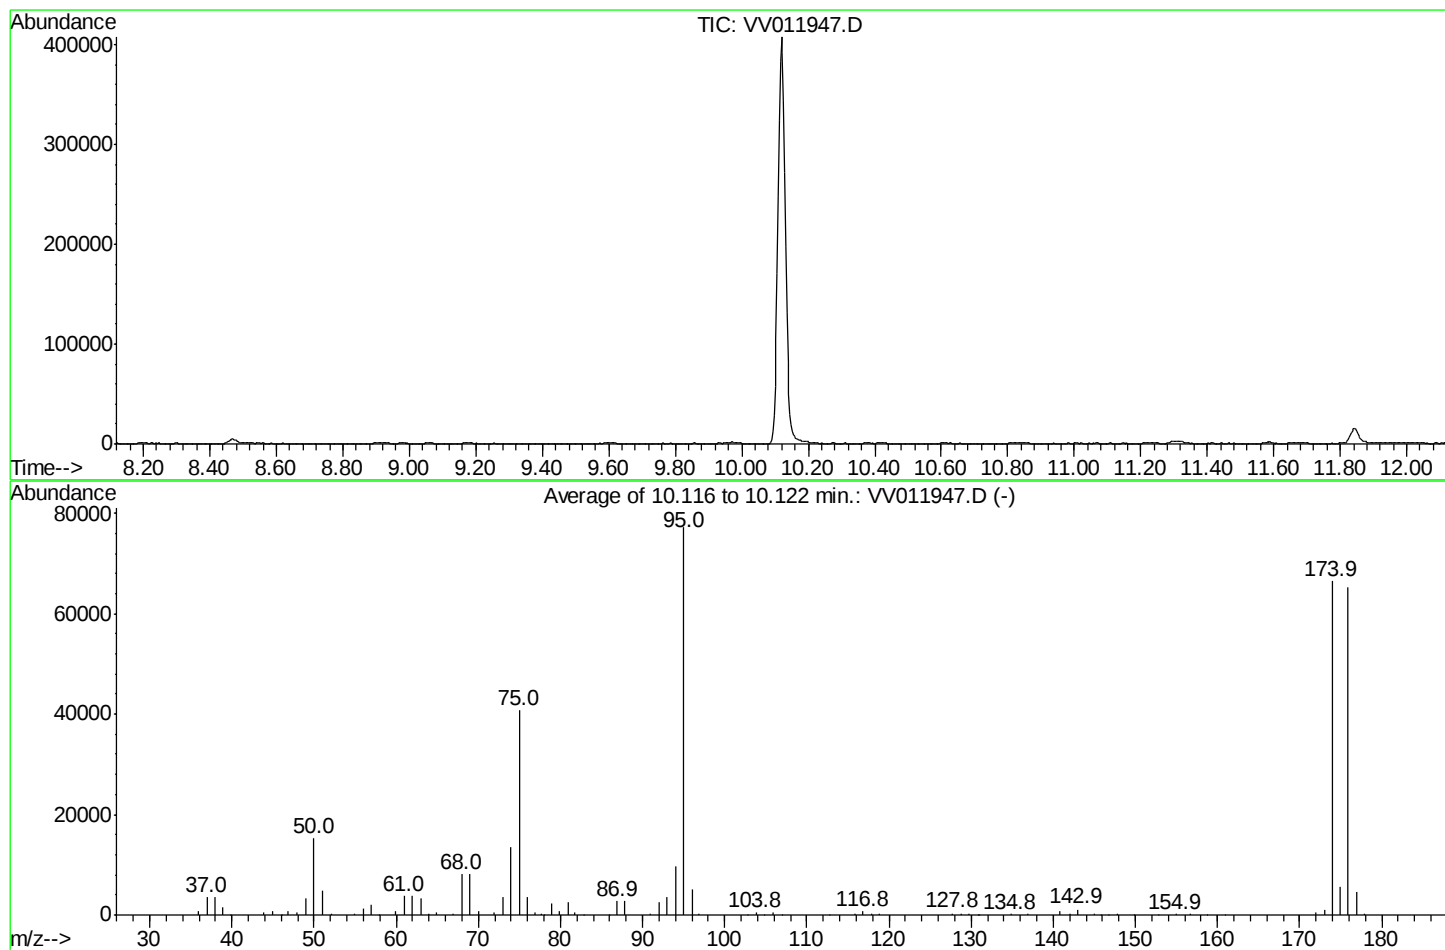

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	15176	PASS
75	95	30	80	52.7	40712	PASS
95	95	100	100	100.0	77186	PASS
96	95	5	9	6.7	5163	PASS
173	174	0.00	2	1.6	1074	PASS
174	95	50	120	86.2	66514	PASS
175	174	5	9	8.3	5533	PASS
176	174	95	101	98.2	65349	PASS
177	176	5	9	7.0	4550	PASS

Scan 2794 (10.074 min): VV011947.D
BFB36

m/z	Abundance
39.80	247.0
43.80	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	677.0
36.90	3535.0
38.00	3527.0
38.90	1426.0
39.90	289.0
44.00	694.0
44.90	946.0
46.90	776.0
47.90	575.0
49.00	3462.0
50.00	14954.0
51.00	4810.0
52.20	240.0
55.00	205.0
56.00	1293.0
57.00	2080.0
57.80	125.0
60.00	836.0
60.90	3624.0
61.90	3888.0
63.00	3202.0
64.00	336.0
65.00	462.0
67.00	334.0
68.00	7793.0
68.90	7782.0
70.00	777.0
71.80	471.0
72.90	3459.0
74.00	13131.0
75.00	40400.0
76.00	3822.0
76.80	550.0
78.00	283.0
78.80	2477.0
79.90	737.0
80.90	2349.0
81.80	544.0
86.90	2803.0
87.80	2717.0
90.80	359.0
92.00	2391.0
92.90	3430.0
94.00	9534.0
95.00	75560.0
96.00	5277.0
96.90	108.0
102.80	103.0
103.90	400.0
105.80	446.0
106.90	104.0
115.80	300.0
116.80	688.0
117.90	325.0
118.80	392.0
127.80	298.0
128.80	179.0
129.70	287.0
130.80	111.0
134.80	196.0
136.90	131.0
140.80	800.0
141.90	209.0
142.90	1030.0
144.90	195.0
145.70	109.0
146.70	103.0
147.90	181.0
154.90	194.0
156.70	140.0
160.90	113.0
172.00	595.0
173.00	1029.0
173.90	63008.0
174.90	5564.0
175.90	62448.0
176.90	4473.0
177.80	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	707.0
37.00	3606.0
38.00	3608.0
38.90	1499.0
39.90	268.0
43.90	739.0
44.90	935.0
46.90	773.0
48.00	587.0
49.00	3555.0
50.00	15777.0
51.00	4964.0
52.10	259.0
55.00	242.0
56.00	1385.0
57.00	2147.0
57.90	128.0
59.90	895.0
61.00	3897.0
62.00	4042.0
63.00	3398.0
64.00	315.0
64.90	463.0
66.90	352.0
68.00	8322.0
69.00	8307.0
70.00	808.0
71.90	556.0
73.00	3750.0
74.00	14131.0
75.00	42080.0
76.00	3810.0
76.80	594.0
77.70	299.0
78.90	2513.0
79.90	794.0
80.90	2494.0
81.80	571.0
86.90	2820.0
87.90	2858.0
90.80	371.0
91.90	2583.0
92.90	3677.0
94.00	9983.0
95.00	79544.0
96.00	5368.0
96.90	150.0
103.90	447.0
104.80	110.0
105.90	428.0
115.80	356.0
116.80	764.0
117.90	380.0
118.80	392.0
127.70	350.0
128.80	187.0
129.80	324.0
130.80	129.0
131.00	124.0
134.90	204.0
136.80	156.0
140.80	895.0
142.00	199.0
142.90	1086.0
145.00	184.0
145.70	114.0
146.70	113.0
147.80	211.0
149.80	158.0
152.80	105.0
154.90	225.0
156.70	164.0
158.80	127.0
160.90	114.0
172.00	618.0
173.00	1121.0
173.90	68680.0
174.90	5718.0
175.90	67648.0
176.90	4695.0
177.80	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
35.90	651.0
37.00	3444.0
38.00	3381.0
38.90	1359.0
39.90	229.0
43.90	730.0
44.90	809.0
46.00	118.0
46.90	822.0
47.90	514.0
49.00	3181.0
50.00	14797.0
51.00	4649.0
52.10	229.0
55.00	212.0
56.00	1271.0
56.90	2040.0
57.90	119.0
59.80	810.0
61.00	3848.0
62.00	3855.0
63.00	3152.0
63.90	313.0
64.90	415.0
66.90	347.0
68.00	8141.0
69.00	8027.0
70.00	705.0
71.90	552.0
73.00	3658.0
74.00	13646.0
75.00	39656.0
76.00	3396.0
76.90	535.0
77.70	317.0
78.90	2286.0
79.90	817.0
80.90	2471.0
81.80	580.0
82.80	148.0
86.00	123.0
86.90	2690.0
87.90	2722.0
90.90	350.0
91.90	2487.0
92.90	3577.0
94.00	9602.0
95.00	76456.0
96.00	4844.0
96.90	194.0
103.80	434.0
104.70	131.0
105.90	363.0
112.70	104.0
115.80	360.0
116.80	757.0
117.90	359.0
118.80	373.0
127.70	347.0
128.90	183.0
129.80	331.0
130.70	141.0
134.90	199.0
136.80	172.0
140.90	880.0
142.10	181.0
142.90	1021.0
144.90	113.0
145.80	120.0
147.80	200.0
149.90	170.0
152.90	105.0
155.00	238.0
156.80	191.0
158.70	149.0
172.00	606.0
173.00	1072.0
173.90	67856.0
174.90	5319.0
175.90	65952.0
176.90	4484.0
177.90	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36