

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072220\
 Data File : VV017583.D
 Acq On : 22 Jul 2020 11:51
 Operator : SY/MD
 Sample : L3314-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4C30DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	148073	151904	12.41%	1.529%
2	1.579	145	152	166	rVB	111421	125384	10.25%	1.262%
3	2.019	287	289	294	rBV5	1428	1225	0.10%	0.012%
4	2.126	311	322	348	rVB2	387084	680830	55.64%	6.854%
5	2.309	373	379	383	rBV6	1751	2127	0.17%	0.021%
6	2.454	422	424	428	rVB4	810	473	0.04%	0.005%
7	2.521	439	445	448	rBV5	1885	2471	0.20%	0.025%
8	2.582	462	464	466	rVV3	783	372	0.03%	0.004%
9	2.817	535	537	539	rBV2	908	465	0.04%	0.005%
10	2.830	539	541	544	rVV	800	422	0.03%	0.004%
11	3.064	610	614	619	rVV5	553	597	0.05%	0.006%
12	3.161	640	644	646	rVB2	588	461	0.04%	0.005%
13	3.190	650	653	655	rBV4	1105	691	0.06%	0.007%
14	3.270	673	678	681	rBV2	971	882	0.07%	0.009%
15	3.363	704	707	708	rBV2	670	438	0.04%	0.004%
16	3.479	740	743	746	rBV2	1191	850	0.07%	0.009%
17	3.592	775	778	780	rBV3	770	431	0.04%	0.004%
18	3.634	789	791	794	rBV3	692	433	0.04%	0.004%
19	3.704	811	813	816	rBV2	596	493	0.04%	0.005%
20	3.820	845	849	853	rBV3	907	736	0.06%	0.007%
21	3.910	866	877	910	rBV2	82161	254962	20.84%	2.567%
22	4.196	963	966	968	rBV2	1275	857	0.07%	0.009%
23	4.270	987	989	992	rBV2	1024	630	0.05%	0.006%
24	4.380	1005	1023	1051	rBV	209894	510298	41.70%	5.137%
25	4.775	1144	1146	1151	rVB3	764	584	0.05%	0.006%
26	4.904	1184	1186	1189	rBV3	940	499	0.04%	0.005%
27	4.994	1211	1214	1216	rBV2	903	565	0.05%	0.006%
28	5.071	1220	1238	1261	rBV2	472398	1223646	100.00%	12.318%
29	5.344	1321	1323	1325	rBV2	846	324	0.03%	0.003%
30	5.360	1325	1328	1330	rVB4	1324	713	0.06%	0.007%
31	5.598	1398	1402	1403	rBV4	517	362	0.03%	0.004%
32	5.640	1403	1415	1439	rVV	384176	760797	62.17%	7.659%
33	5.842	1476	1478	1483	rVB4	1559	862	0.07%	0.009%
34	5.939	1496	1508	1527	rBV2	111846	223508	18.27%	2.250%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072220\
 Data File : VV017583.D
 Acq On : 22 Jul 2020 11:51
 Operator : SY/MD
 Sample : L3314-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4C30DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

35	6.093	1541	1556	1584	rBV	268946	554922	45.35%	5.586%
36	6.273	1609	1612	1617	rVB6	1172	988	0.08%	0.010%
37	6.360	1632	1639	1642	rBV5	955	1002	0.08%	0.010%
38	6.396	1646	1650	1654	rBV4	983	940	0.08%	0.009%
39	6.434	1660	1662	1665	rBV4	965	562	0.05%	0.006%
40	6.505	1681	1684	1688	rBV4	772	763	0.06%	0.008%
41	6.524	1688	1690	1695	rVB4	1141	771	0.06%	0.008%
42	6.656	1729	1731	1732	rBV2	882	500	0.04%	0.005%
43	6.791	1771	1773	1777	rBV3	1100	498	0.04%	0.005%
44	7.006	1830	1840	1858	rBV	166540	294991	24.11%	2.970%
45	7.338	1931	1943	1966	rBV	569260	985299	80.52%	9.919%
46	7.569	2013	2015	2017	rVB2	1037	396	0.03%	0.004%
47	7.640	2027	2037	2055	rBV	118032	207736	16.98%	2.091%
48	7.810	2088	2090	2092	rBV2	721	422	0.03%	0.004%
49	8.029	2156	2158	2160	rVB3	996	354	0.03%	0.004%
50	8.045	2162	2163	2166	rVB2	955	365	0.03%	0.004%
51	8.106	2172	2182	2215	rBV	299725	549317	44.89%	5.530%
52	8.434	2282	2284	2285	rBV2	789	381	0.03%	0.004%
53	8.614	2336	2340	2342	rBV	1008	693	0.06%	0.007%
54	8.662	2353	2355	2361	rVB6	833	599	0.05%	0.006%
55	8.823	2403	2405	2407	rBV2	693	393	0.03%	0.004%
56	8.875	2408	2421	2446	rVV	564169	929589	75.97%	9.358%
57	9.225	2527	2530	2531	rBV2	707	410	0.03%	0.004%
58	9.289	2548	2550	2555	rVB2	820	592	0.05%	0.006%
59	9.383	2574	2579	2582	rBV5	1121	1046	0.09%	0.011%
60	9.550	2627	2631	2633	rBV3	664	460	0.04%	0.005%
61	9.566	2633	2636	2638	rBV3	940	578	0.05%	0.006%
62	9.801	2705	2709	2711	rBV5	667	535	0.04%	0.005%
63	9.862	2724	2728	2729	rBV	851	533	0.04%	0.005%
64	9.997	2767	2770	2772	rBV2	571	420	0.03%	0.004%
65	10.132	2809	2812	2814	rBV4	635	417	0.03%	0.004%
66	10.170	2821	2824	2829	rVB5	1242	921	0.08%	0.009%
67	10.238	2829	2845	2862	rBV	363127	582523	47.61%	5.864%
68	10.511	2928	2930	2934	rBV2	629	372	0.03%	0.004%
69	10.675	2978	2981	2983	rBV3	943	462	0.04%	0.005%
70	10.730	2996	2998	3002	rVB3	678	404	0.03%	0.004%
71	10.807	3019	3022	3025	rBV2	721	518	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072220\
 Data File : VV017583.D
 Acq On : 22 Jul 2020 11:51
 Operator : SY/MD
 Sample : L3314-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4C30DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis

72	10.871	3039	3042	3043	rBV3	780	367	0.03%	0.004%
73	10.993	3076	3080	3081	rBV3	785	419	0.03%	0.004%
74	11.074	3103	3105	3109	rBV4	618	390	0.03%	0.004%
75	11.093	3109	3111	3114	rBV3	584	324	0.03%	0.003%
76	11.270	3155	3166	3184	rBV	576461	885397	72.36%	8.913%
77	11.646	3270	3283	3302	rBV	613959	959386	78.40%	9.658%
78	11.948	3376	3377	3381	rBV	582	370	0.03%	0.004%
79	12.109	3424	3427	3429	rBV3	1004	640	0.05%	0.006%
80	12.421	3519	3524	3526	rBV4	531	417	0.03%	0.004%
81	12.633	3589	3590	3592	rBV	762	324	0.03%	0.003%
82	12.672	3597	3602	3605	rBV3	1021	1048	0.09%	0.011%
83	12.797	3638	3641	3642	rBV2	721	401	0.03%	0.004%
84	12.807	3642	3644	3647	rVB3	1276	575	0.05%	0.006%
85	12.871	3663	3664	3669	rBV2	614	405	0.03%	0.004%
86	12.939	3682	3685	3686	rBV3	764	408	0.03%	0.004%
87	13.000	3701	3704	3707	rBV3	745	447	0.04%	0.004%
88	13.112	3734	3739	3741	rBV2	827	781	0.06%	0.008%
89	13.157	3751	3753	3754	rBV	845	323	0.03%	0.003%
90	13.218	3770	3772	3775	rVV2	677	434	0.04%	0.004%
91	13.263	3783	3786	3788	rBV3	748	470	0.04%	0.005%
92	13.292	3788	3795	3802	rVV8	2502	3720	0.30%	0.037%
93	13.476	3850	3852	3854	rBV2	615	358	0.03%	0.004%
94	13.582	3882	3885	3886	rBV2	681	341	0.03%	0.003%
95	13.646	3903	3905	3908	rVB2	1038	519	0.04%	0.005%
96	13.855	3968	3970	3973	rBV2	1111	613	0.05%	0.006%
97	13.955	3997	4001	4003	rBV2	950	686	0.06%	0.007%
98	14.225	4083	4085	4087	rBV	1135	510	0.04%	0.005%
99	14.369	4127	4130	4135	rBV4	753	668	0.05%	0.007%
100	15.643	4524	4526	4529	rBV3	1108	720	0.06%	0.007%


Sum of corrected areas: 9933425

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072220\
Data File : VV017583.D
Acq On : 22 Jul 2020 11:51
Operator : SY/MD
Sample : L3314-05DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4C30DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

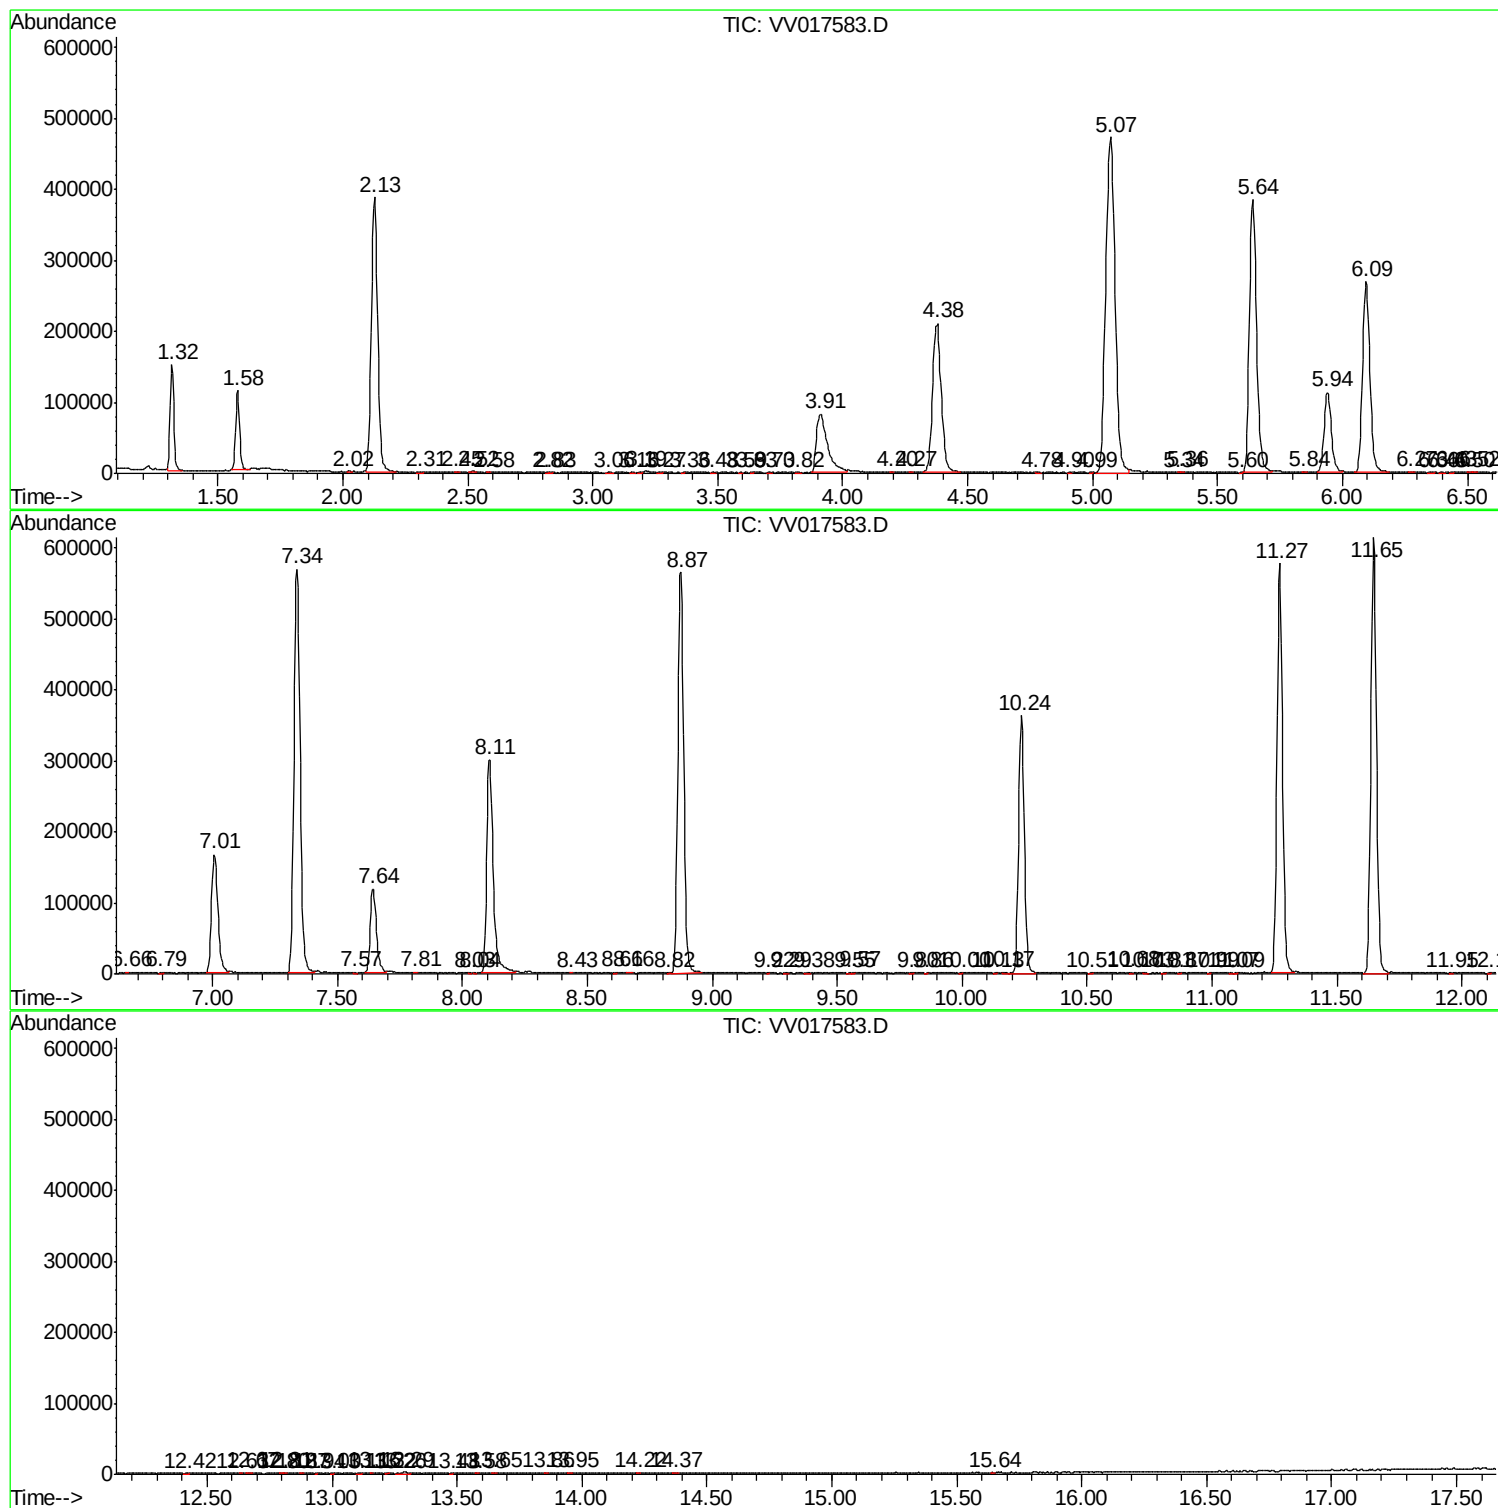

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV072220\
Data File : VV017583.D
Acq On : 22 Jul 2020 11:51
Operator : SY/MD
Sample : L3314-05DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F4C30DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV072220\
Data File : VV017583.D
Acq On : 22 Jul 2020 11:51
Operator : SY/MD
Sample : L3314-05DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F4C30DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM072120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc