


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072220\
 Data File : VV017578.D
 Acq On : 22 Jul 2020 09:13
 Operator : SY/MD
 Sample : BFB65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072120WMA.M
 Title : VOC Analysis
 Last Update : Thu Jul 23 05:23:23 2020

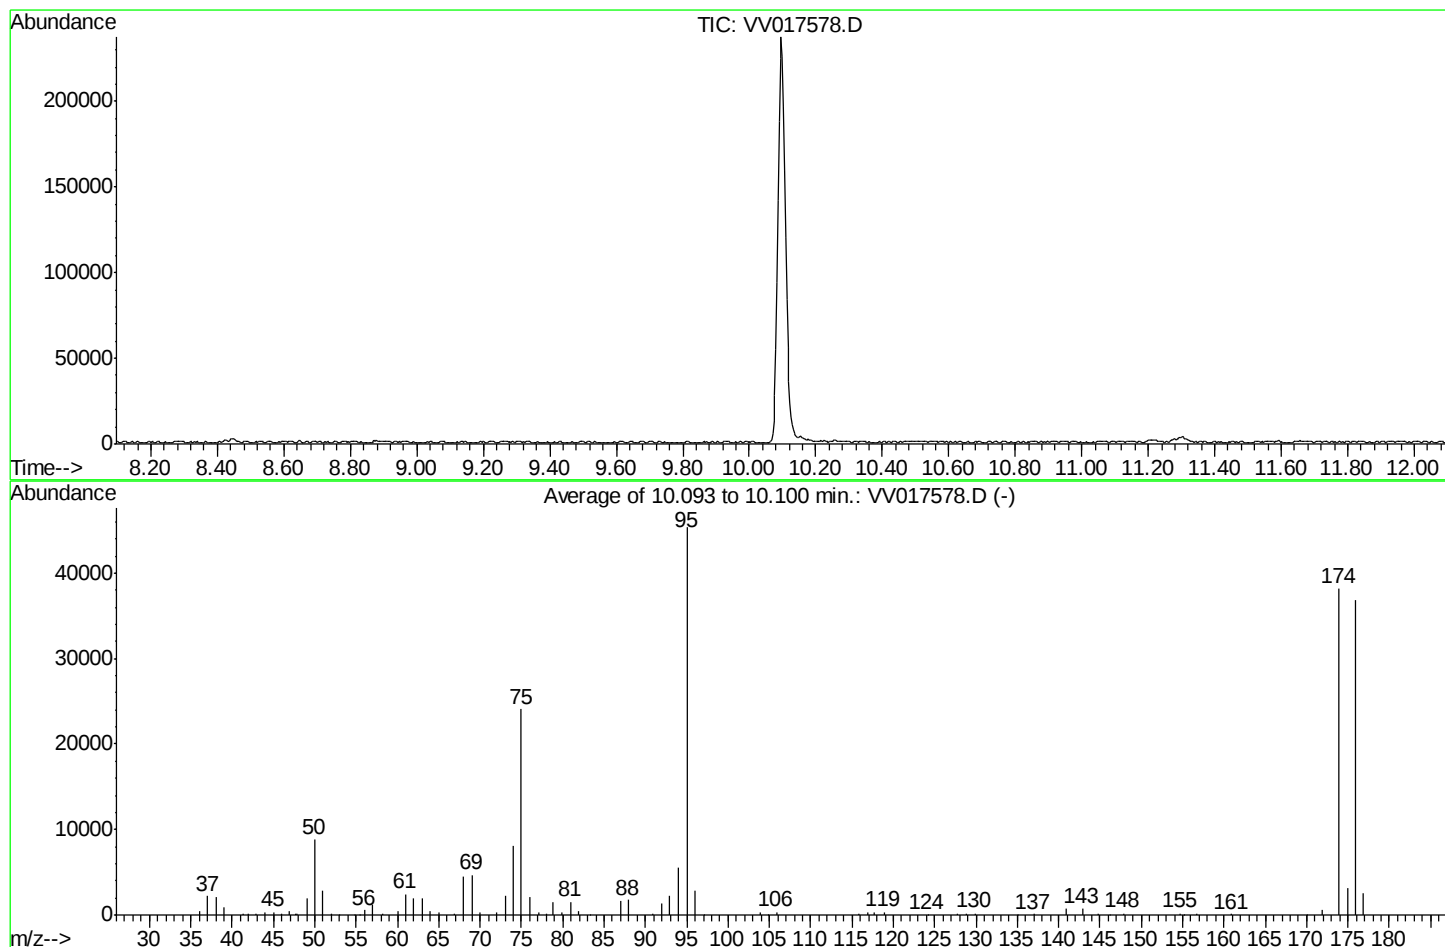

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	8771	PASS
75	95	30	80	53.1	24106	PASS
95	95	100	100	100.0	45357	PASS
96	95	5	9	6.3	2861	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.1	38130	PASS
175	174	5	9	8.4	3201	PASS
176	174	95	101	96.8	36906	PASS
177	176	5	9	7.0	2590	PASS

m/z	Abundance
36.00	482.0
37.00	2158.0
38.00	2098.0
39.00	969.0
40.00	273.0
41.90	139.0
42.90	127.0
44.00	595.0
45.00	346.0
46.00	128.0
46.90	550.0
47.60	321.0
49.00	2059.0
50.00	8809.0
51.00	2933.0
52.00	149.0
55.40	228.0
56.00	603.0
57.00	1225.0
58.20	124.0
60.10	435.0
61.00	2587.0
62.00	2040.0
63.00	1756.0
64.00	392.0
65.10	334.0
66.90	170.0
68.00	4298.0
69.00	4654.0
70.00	387.0
72.10	207.0
73.00	2255.0
74.00	7948.0
75.00	23664.0
76.00	2049.0
77.00	257.0
78.00	138.0
78.80	1430.0
79.90	357.0
80.90	1441.0
81.90	462.0
86.90	1671.0
87.90	1587.0
91.00	206.0
92.00	1373.0
93.00	2218.0
94.00	5421.0
95.00	44648.0
96.00	2796.0
103.90	213.0
104.80	102.0
105.90	305.0
115.80	150.0
116.80	339.0
117.70	234.0
118.80	306.0
124.10	114.0
127.80	178.0
128.80	136.0
129.90	214.0
137.00	114.0
140.80	748.0
142.90	668.0
144.80	139.0
146.20	106.0
147.80	163.0
154.70	119.0
155.20	106.0
156.80	108.0
161.00	138.0
171.90	532.0
173.90	36512.0
175.00	3207.0
175.90	35504.0
176.90	2606.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	459.0
37.00	2276.0
38.00	2140.0
39.10	950.0
40.00	277.0
41.40	127.0
41.90	140.0
42.80	159.0
44.00	616.0
45.00	389.0
46.00	142.0
46.90	522.0
47.90	328.0
49.00	1960.0
50.00	9103.0
51.00	2935.0
52.00	147.0
56.00	598.0
57.00	1165.0
58.20	134.0
60.00	452.0
61.00	2547.0
62.00	2014.0
63.00	2081.0
64.00	416.0
65.00	395.0
66.90	199.0
68.00	4572.0
69.00	4927.0
70.00	374.0
72.00	229.0
73.00	2397.0
74.00	8392.0
75.00	25120.0
76.00	2136.0
77.00	240.0
78.00	176.0
78.80	1529.0
79.90	358.0
80.90	1623.0
81.90	503.0
83.30	105.0
87.00	1764.0
87.90	1827.0
91.00	218.0
92.00	1402.0
93.00	2262.0
94.00	5653.0
95.00	46816.0
96.00	2896.0
103.80	302.0
105.90	331.0
115.70	147.0
116.80	301.0
117.70	301.0
118.80	303.0
124.10	101.0
127.80	176.0
128.80	206.0
129.80	239.0
135.00	105.0
137.00	120.0
140.90	743.0
142.80	700.0
144.80	154.0
146.10	109.0
147.80	212.0
154.70	191.0
156.80	136.0
161.00	139.0
171.90	534.0
173.90	39576.0
174.90	3254.0
175.90	38272.0
176.90	2686.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	411.0
37.00	2119.0
38.00	1926.0
39.00	858.0
40.00	282.0
41.30	145.0
41.90	143.0
42.80	178.0
44.00	580.0
45.00	402.0
45.90	134.0
46.90	428.0
47.80	344.0
49.00	1648.0
50.00	8402.0
51.00	2687.0
52.00	143.0
53.00	103.0
54.80	120.0
56.00	578.0
57.00	1165.0
58.10	125.0
59.90	467.0
60.90	2229.0
62.00	1848.0
63.00	2055.0
64.00	377.0
65.00	394.0
67.00	225.0
68.00	4494.0
69.00	4589.0
70.00	327.0
72.00	272.0
73.00	2193.0
74.00	8022.0
75.00	23536.0
76.00	2017.0
77.10	223.0
78.00	193.0
78.90	1486.0
79.90	338.0
80.90	1550.0
81.90	421.0
87.00	1707.0
87.90	1901.0
90.90	204.0
92.00	1178.0
92.90	2157.0
94.00	5422.0
95.00	44608.0
96.00	2892.0
97.00	105.0
103.80	299.0
105.90	275.0
115.70	157.0
116.90	248.0
117.70	322.0
118.90	291.0
127.80	185.0
128.80	247.0
129.80	224.0
135.00	116.0
137.00	102.0
140.90	655.0
142.80	782.0
144.80	150.0
147.90	246.0
154.80	214.0
156.70	133.0
160.90	115.0
170.00	106.0
172.00	531.0
173.90	38304.0
175.00	3144.0
175.90	36944.0
176.90	2479.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Scan 2788 (10.055 min): VV017578.D
BFB65

m/z	Abundance
39.90	302.0
44.00	233.0
50.70	161.0
75.70	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65