

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072221\
 Data File : VV021697.D
 Acq On : 22 Jul 2021 11:36
 Operator : SY/MD
 Sample : M3107-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 23 01:17:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 23 01:17:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	446260	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	423843	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	210353	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	138004	43.714	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	87.420%	
7) Chloroethane-d5	1.558	69	112039	51.292	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.580%	
11) 1,1-Dichloroethene-d2	2.102	63	187998	35.737	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	71.480%	
21) 2-Butanone-d5	3.867	46	221831	91.166	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	91.170%	
24) Chloroform-d	4.343	84	275914	46.027	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.060%	
26) 1,2-Dichloroethane-d4	5.027	65	174739	49.213	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.420%	
32) Benzene-d6	5.044	84	577393	46.285	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.580%	
36) 1,2-Dichloropropane-d6	6.066	67	183142	46.955	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	93.900%	
41) Toluene-d8	7.314	98	524700	45.526	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.060%	
43) trans-1,3-Dichloroprop...	7.619	79	87082	44.788	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.580%	
47) 2-Hexanone-d5	8.085	63	142644	80.978	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	80.980%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	224331	43.542	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	87.080%	
66) 1,2-Dichlorobenzene-d4	11.625	152	204158	46.947	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.900%	
Target Compounds						
					Qvalue	
25) Chloroform	4.365	83	2873	0.525	ug/L #	61
48) 2-Hexanone	8.143	43	12514	3.519	ug/L #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072221\
Data File : VV021697.D
Acq On : 22 Jul 2021 11:36
Operator : SY/MD
Sample : M3107-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 23 01:17:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 23 01:17:03 2021
Response via : Initial Calibration




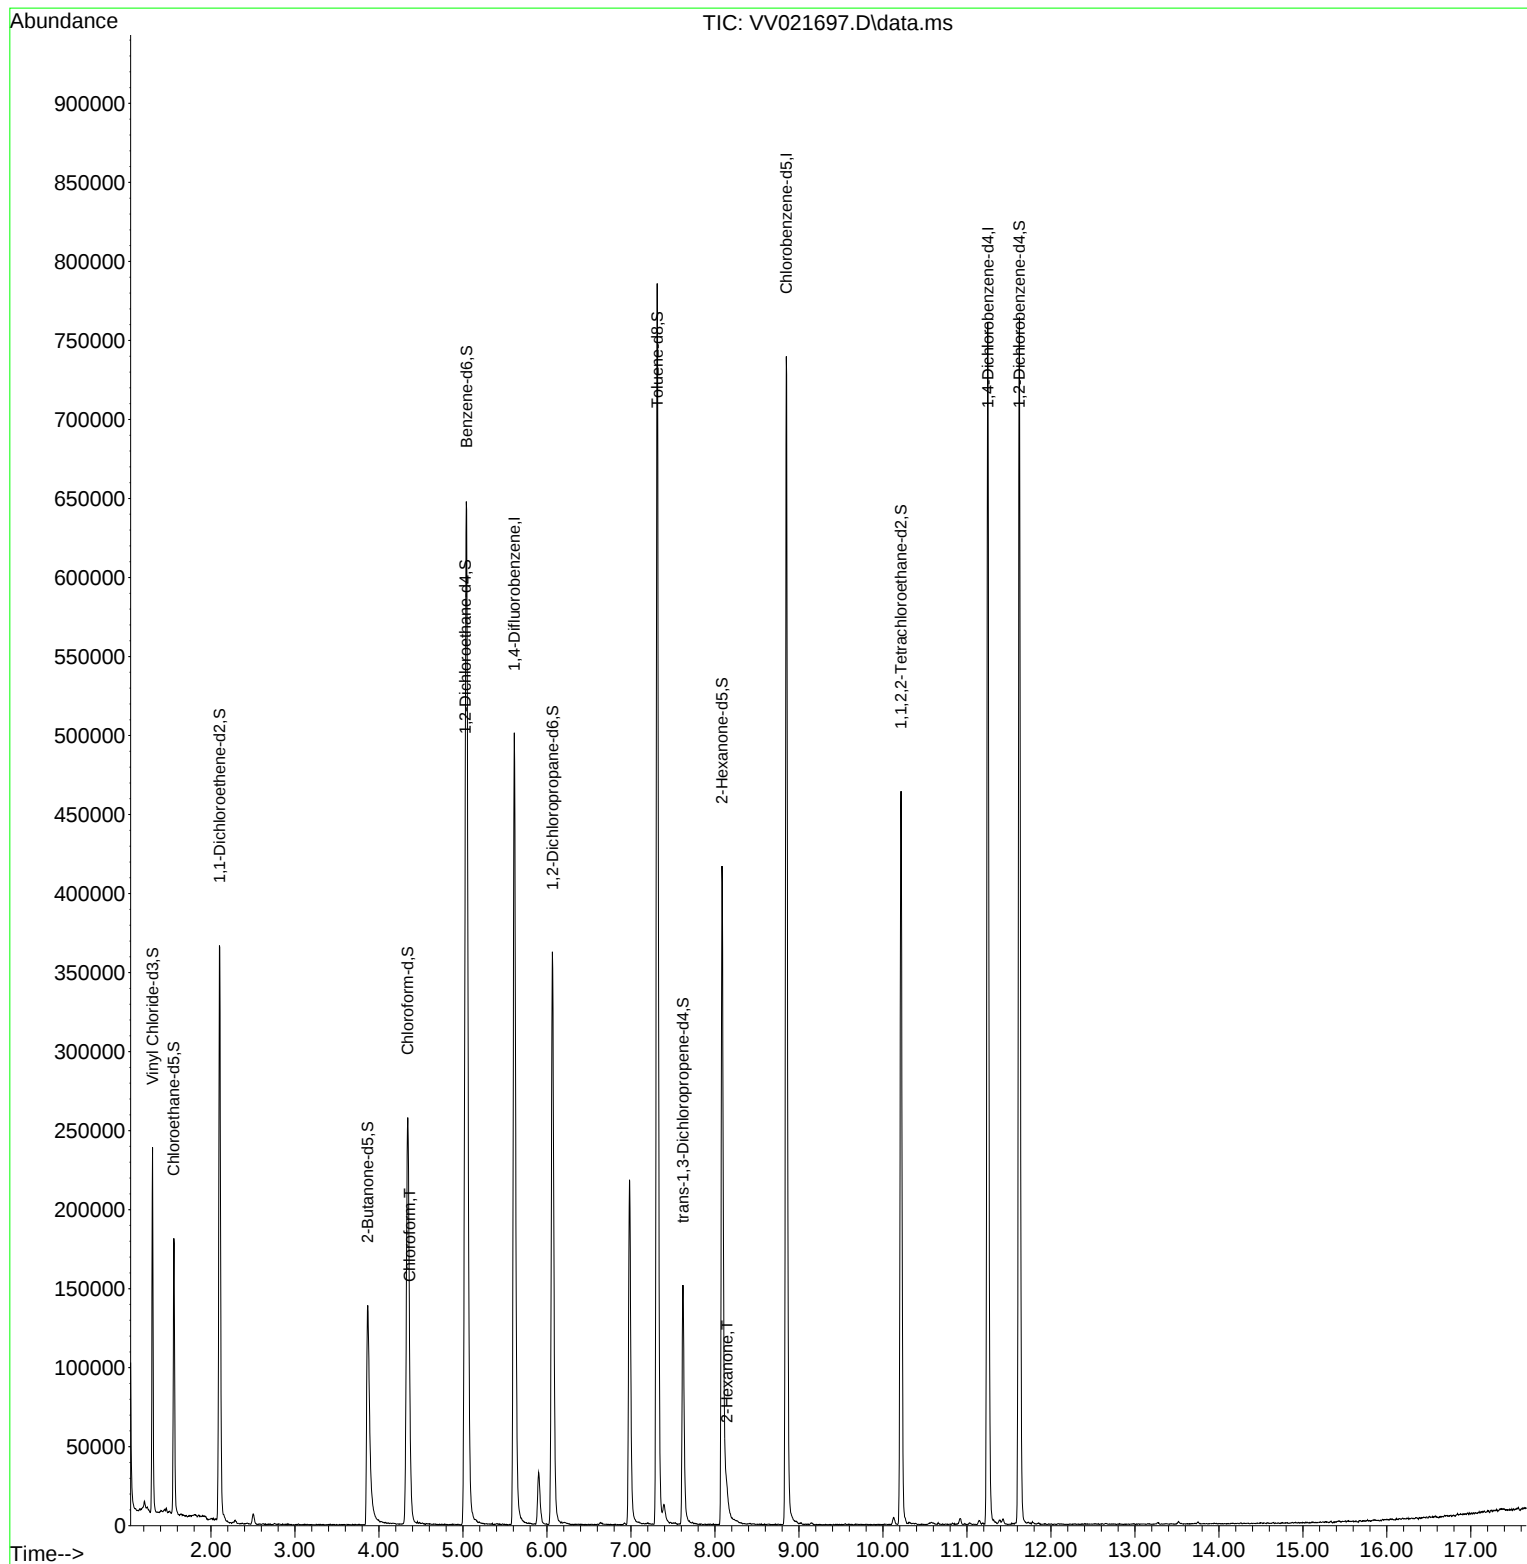


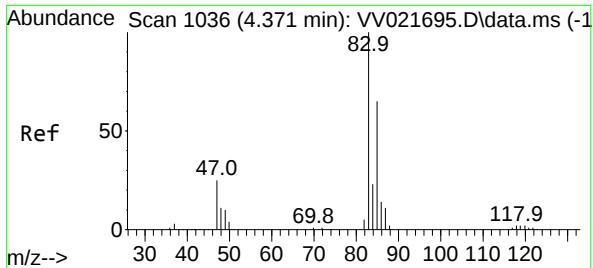

#25
Chloroform
Concen: 0.525 ug/L
RT: 4.365 min Scan# 1034
Delta R.T. -0.006 min
Lab File: VV021697.D
Acq: 22 Jul 2021 11:36

Instrument :
MSVOA_V
ClientSampled :

Tgt Ion: 83 Resp: 2873
Ion Ratio Lower Upper
83 100
85 92.5 43.8 81.4#

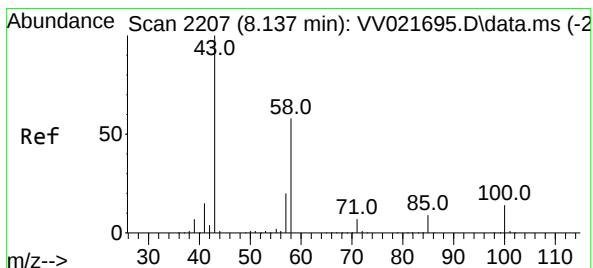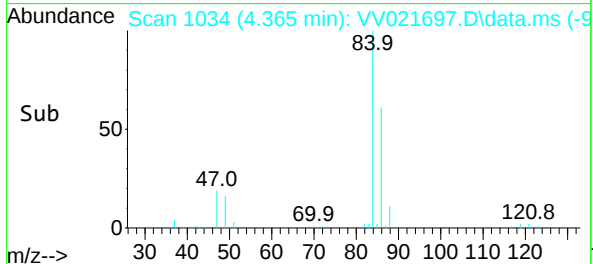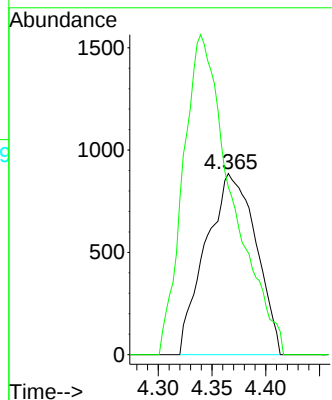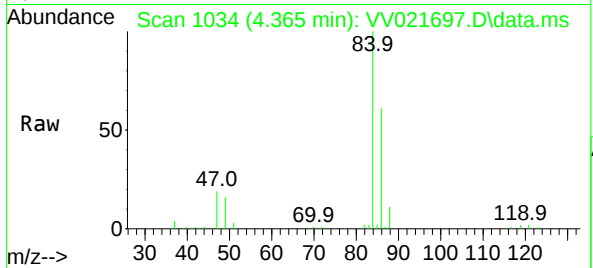

#48
2-Hexanone
Concen: 3.519 ug/L
RT: 8.143 min Scan# 2209
Delta R.T. 0.007 min
Lab File: VV021697.D
Acq: 22 Jul 2021 11:36

Tgt Ion: 43 Resp: 12514
Ion Ratio Lower Upper
43 100
58 41.8 46.0 69.0#
57 11.4 15.6 23.4#
100 5.7 11.0 16.4#

