


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072221\
Data File : VV021694.D
Acq On : 22 Jul 2021 09:08
Operator : SY/MD
Sample : BFB209
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB209

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071921WMA.M
Title : VOC Analysis
Last Update : Fri Jul 23 01:17:03 2021

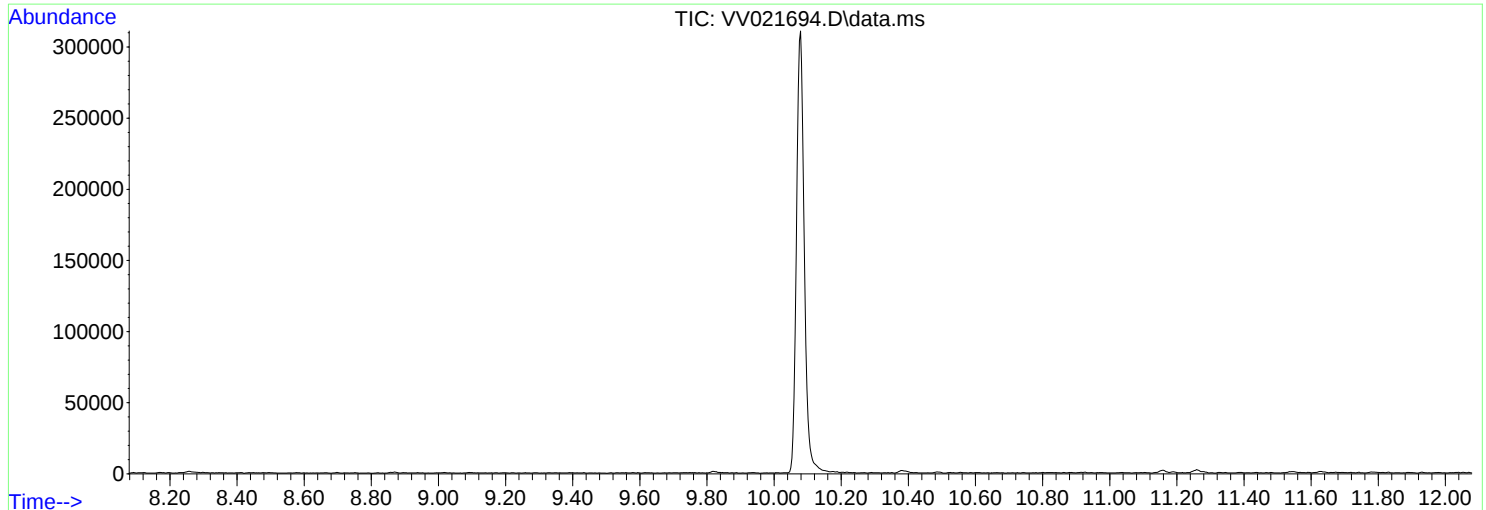

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	11379	PASS
75	95	30	80	49.2	31043	PASS
95	95	100	100	100.0	63131	PASS
96	95	5	9	6.9	4328	PASS
173	174	0.00	2	1.1	554	PASS
174	95	50	120	83.1	52440	PASS
175	174	5	9	6.9	3613	PASS
176	174	95	105	96.7	50688	PASS
177	176	5	10	6.7	3384	PASS

m/z	Abundance
36.00	449.0
37.00	2767.0
38.00	2373.0
39.00	1042.0
40.00	250.0
44.00	733.0
45.00	565.0
46.90	849.0
47.90	392.0
49.00	2451.0
50.00	11782.0
51.00	3169.0
51.90	197.0
55.10	235.0
56.00	765.0
57.00	1512.0
60.00	516.0
61.00	2746.0
62.00	2793.0
63.00	2371.0
64.00	208.0
64.80	168.0
66.90	179.0
68.00	5998.0
69.00	6393.0
70.10	476.0
72.00	370.0
73.00	2890.0
74.00	9639.0
75.00	32208.0
76.00	2582.0
76.90	335.0
77.90	304.0
78.90	1622.0
79.80	628.0
81.00	1726.0
81.80	438.0
82.70	107.0
85.80	116.0
87.00	2849.0
88.00	2777.0
90.90	254.0
91.90	1923.0
92.90	2688.0
94.00	7211.0
95.00	65176.0
96.00	4456.0
97.10	154.0
103.80	256.0
105.00	120.0
105.90	252.0
106.90	122.0
115.90	249.0
116.90	482.0
117.90	342.0
118.90	369.0
127.90	203.0
128.90	117.0
129.80	231.0
130.90	133.0
134.90	151.0
136.90	103.0
140.90	682.0
141.90	118.0
142.90	702.0
147.90	182.0
154.80	114.0
172.00	233.0
173.00	579.0
173.90	54056.0
175.00	3723.0
176.00	52304.0
177.00	3488.0
177.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	428.0
37.00	2436.0
38.00	2178.0
39.00	931.0
40.00	222.0
44.00	744.0
45.00	577.0
46.90	646.0
48.00	335.0
49.00	2276.0
50.00	10644.0
51.00	2760.0
51.90	165.0
55.10	272.0
56.00	700.0
57.00	1471.0
60.00	469.0
61.00	2541.0
62.00	2479.0
63.00	2070.0
64.00	176.0
64.80	133.0
67.00	140.0
68.00	5416.0
69.00	5994.0
70.10	385.0
72.00	331.0
73.00	2521.0
74.00	8885.0
75.00	29512.0
76.00	2372.0
76.90	332.0
77.90	296.0
78.90	1467.0
79.90	595.0
81.00	1556.0
81.90	406.0
82.70	132.0
85.90	102.0
87.00	2676.0
87.90	2718.0
90.90	246.0
92.00	1662.0
92.90	2467.0
94.00	6685.0
95.00	59776.0
96.00	4076.0
97.10	139.0
103.80	252.0
104.90	105.0
105.80	241.0
106.80	112.0
115.80	218.0
116.80	487.0
117.90	318.0
118.90	331.0
127.90	185.0
128.90	134.0
129.80	205.0
130.10	202.0
134.90	146.0
140.90	671.0
142.90	649.0
148.00	136.0
154.80	105.0
172.00	231.0
172.90	428.0
173.90	51472.0
175.00	3428.0
175.90	49728.0
177.00	3373.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

Scan 2798 (10.037 min): VV021694.D\data.ms
BFB209

m/z	Abundance
39.00	124.0
40.00	216.0
44.00	496.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	405.0
37.00	2871.0
38.00	2289.0
39.00	1072.0
40.00	228.0
44.00	686.0
44.90	510.0
46.90	912.0
47.90	398.0
49.00	2391.0
50.00	11712.0
51.00	3361.0
51.90	206.0
55.00	212.0
56.00	776.0
57.00	1460.0
59.90	505.0
61.00	2700.0
62.00	2829.0
62.90	2280.0
64.00	206.0
64.80	145.0
66.90	193.0
68.00	6027.0
69.00	6317.0
70.10	527.0
72.00	379.0
73.00	2930.0
74.00	9496.0
75.00	31408.0
76.00	2639.0
77.10	368.0
77.90	272.0
78.90	1598.0
79.90	619.0
80.90	1800.0
81.90	434.0
85.80	121.0
87.00	2764.0
88.00	2416.0
90.80	245.0
92.00	1973.0
93.00	2595.0
94.00	7341.0
95.00	64440.0
96.00	4452.0
97.00	145.0
103.80	248.0
105.00	147.0
105.90	249.0
107.00	101.0
115.90	253.0
116.90	448.0
117.90	319.0
118.90	332.0
127.90	252.0
129.80	261.0
130.80	166.0
134.80	127.0
136.90	133.0
140.90	622.0
141.90	119.0
142.90	671.0
147.90	210.0
154.80	124.0
156.80	110.0
171.90	204.0
173.00	656.0
174.00	51792.0
175.00	3688.0
176.00	50032.0
177.00	3292.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209