

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072222\
 Data File : VW026886.D
 Acq On : 22 Jul 2022 14:44
 Operator : SY/MD
 Sample : VW0722MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 23 00:23:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	570418	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	578722	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	260534	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	221286	46.254	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	92.500%		
7) Chloroethane-d5	1.561	69	182404	47.128	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.260%		
11) 1,1-Dichloroethene-d2	2.104	63	299747	34.826	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.660%		
21) 2-Butanone-d5	3.879	46	325150	100.830	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.830%		
24) Chloroform-d	4.342	84	428474	45.507	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.020%		
26) 1,2-Dichloroethane-d4	5.027	65	260835	48.430	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.860%		
32) Benzene-d6	5.046	84	863401	49.355	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.720%		
36) 1,2-Dichloropropane-d6	6.066	67	279485	49.576	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.160%		
41) Toluene-d8	7.313	98	703170	45.940	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.880%		
43) trans-1,3-Dichloroprop...	7.619	79	107024	45.307	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.620%		
47) 2-Hexanone-d5	8.088	63	248210	101.117	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.120%		
56) 1,1,2,2-Tetrachloroeth...	10.213	84	399296	46.624	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.240%		
66) 1,2-Dichlorobenzene-d4	11.622	152	269638	55.166	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.340%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.104	101	3423	0.725	ug/L #	32
39) cis-1,3-Dichloropropene	6.985	75	6701	0.997	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026886.D
Acq On : 22 Jul 2022 14:44
Operator : SY/MD
Sample : VV0722MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jul 23 00:23:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

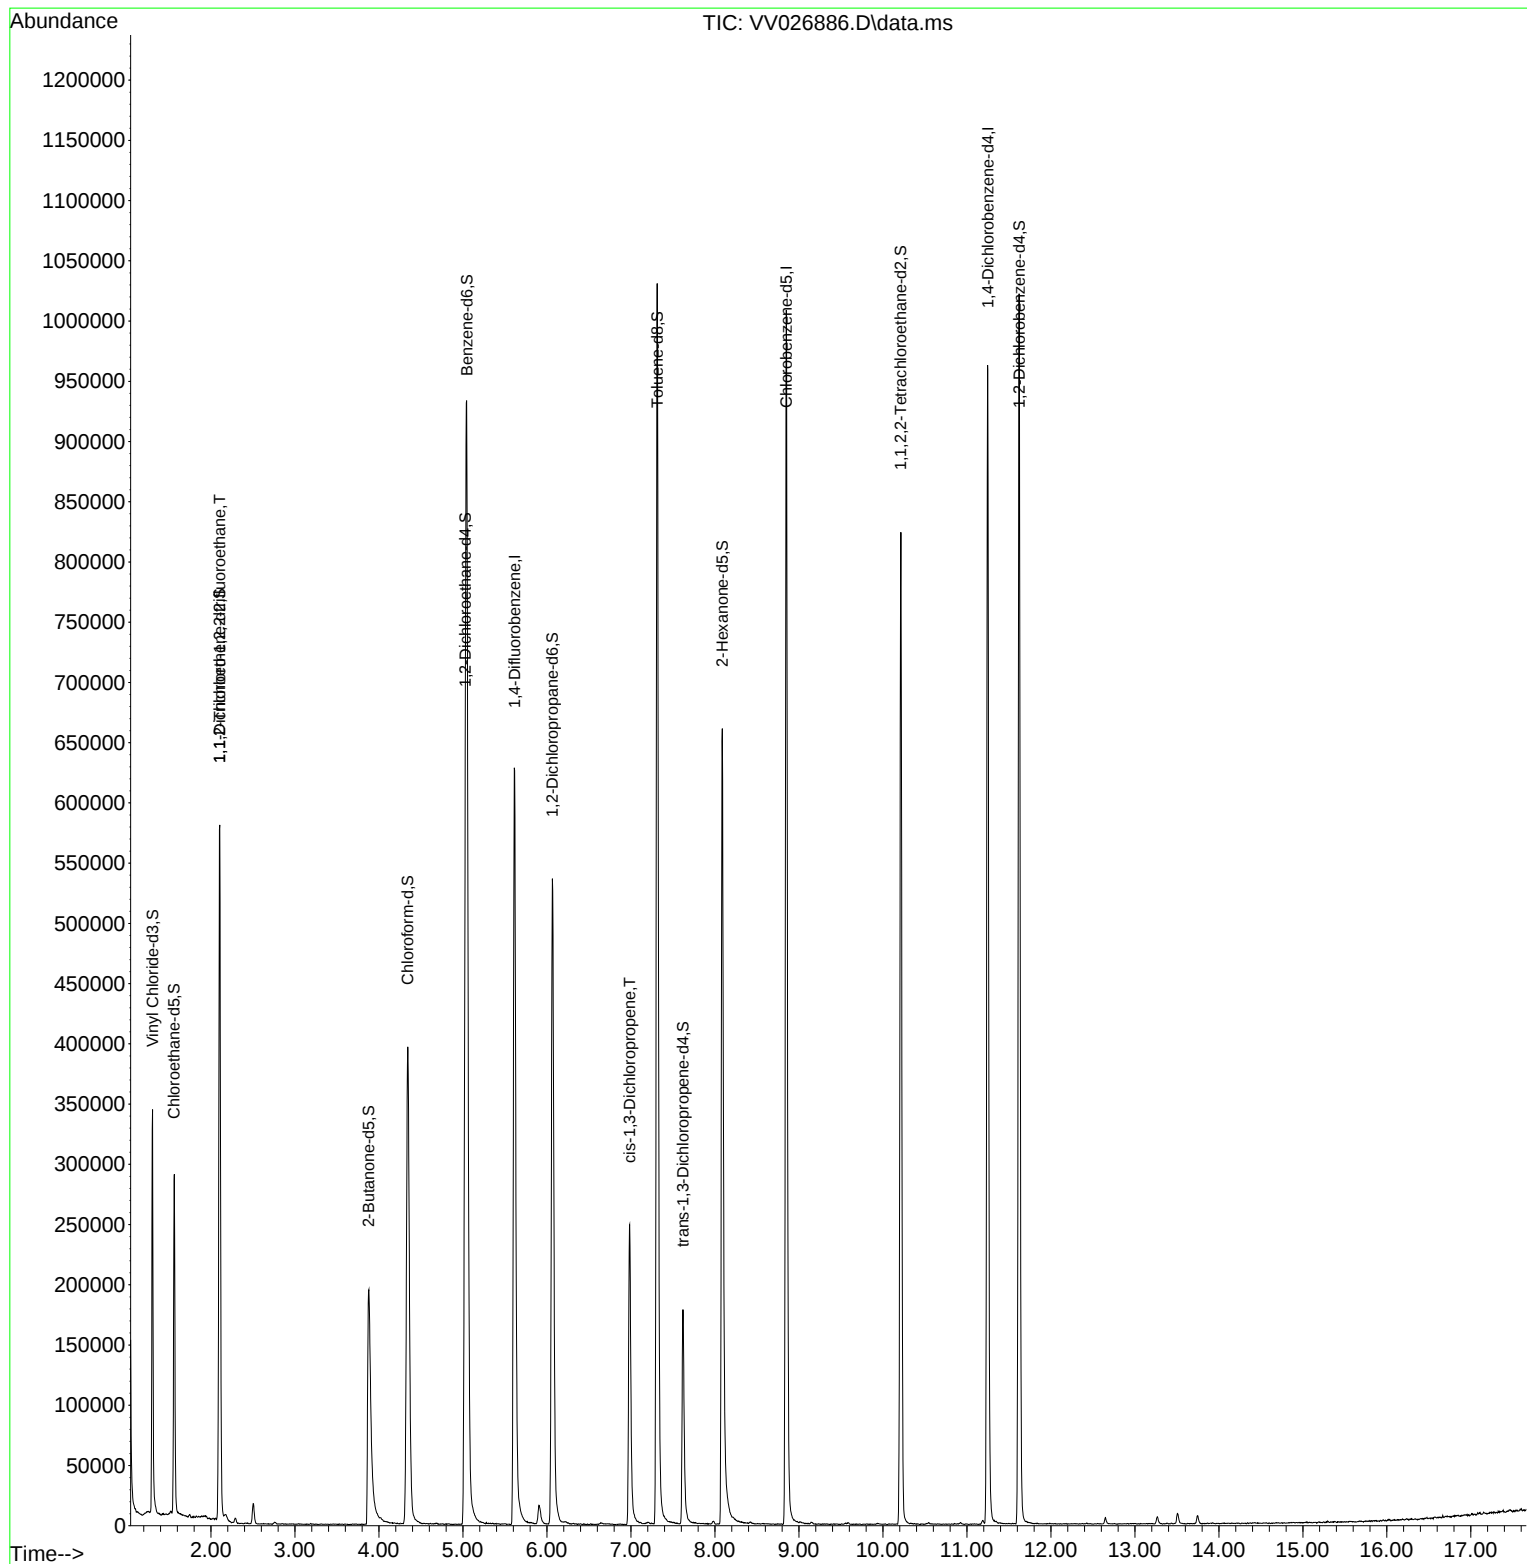



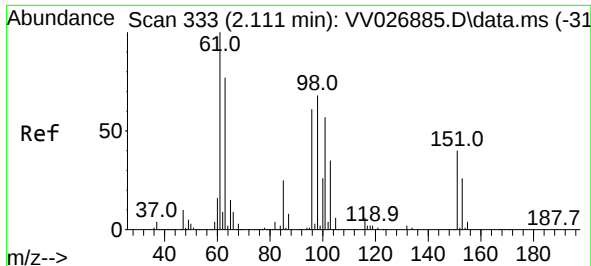


#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.725 ug/L
 RT: 2.104 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: VV026886.D
 Acq: 22 Jul 2022 14:44

Instrument :
 MSVOA_V
 ClientSampleId :

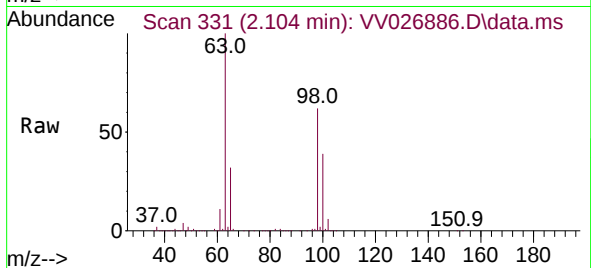

Tgt Ion:101 Resp: 3423
 Ion Ratio Lower Upper
 101 100
 85 7.5 33.1 49.7#
 151 8.1 57.1 85.7#

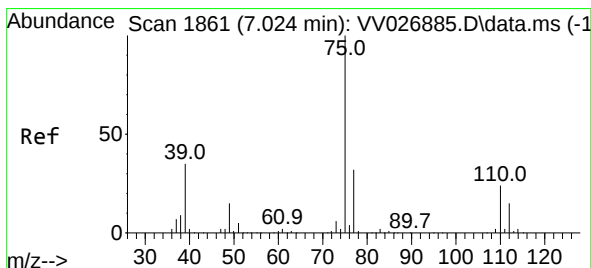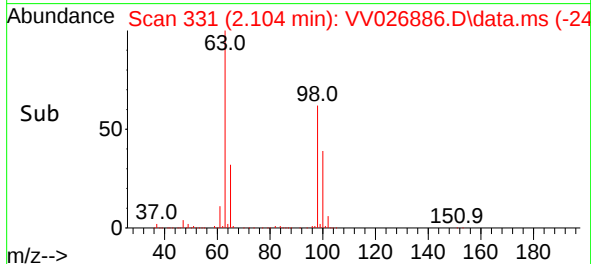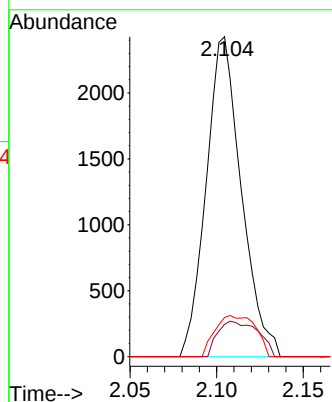

#39
 cis-1,3-Dichloropropene
 Concen: 0.997 ug/L
 RT: 6.985 min Scan# 1849
 Delta R.T. -0.039 min
 Lab File: VV026886.D
 Acq: 22 Jul 2022 14:44

Tgt Ion: 75 Resp: 6701
 Ion Ratio Lower Upper
 75 100
 77 52.2 22.4 41.6#

