

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026887.D
 Acq On : 22 Jul 2022 15:07
 Operator : SY/MD
 Sample : VV0722WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 23 00:23:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	541814	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	553574	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	240779	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	205298	45.178	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.360%		
7) Chloroethane-d5	1.565	69	173057	47.074	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.140%		
11) 1,1-Dichloroethene-d2	2.102	63	282052	34.500	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.000%		
21) 2-Butanone-d5	3.886	46	332696	108.617	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.620%		
24) Chloroform-d	4.346	84	410286	45.876	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.760%		
26) 1,2-Dichloroethane-d4	5.027	65	253538	49.560	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.120%		
32) Benzene-d6	5.047	84	817684	48.866	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.740%		
36) 1,2-Dichloropropane-d6	6.066	67	270626	50.185	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.380%		
41) Toluene-d8	7.314	98	665701	45.468	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.940%		
43) trans-1,3-Dichloroprop...	7.622	79	103908	45.986	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.980%		
47) 2-Hexanone-d5	8.088	63	247010	105.200	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.200%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	396670	48.422	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.840%		
66) 1,2-Dichlorobenzene-d4	11.622	152	252070	55.803	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	111.600%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.088	43	26651	6.210	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026887.D
Acq On : 22 Jul 2022 15:07
Operator : SY/MD
Sample : VV07222WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jul 23 00:23:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

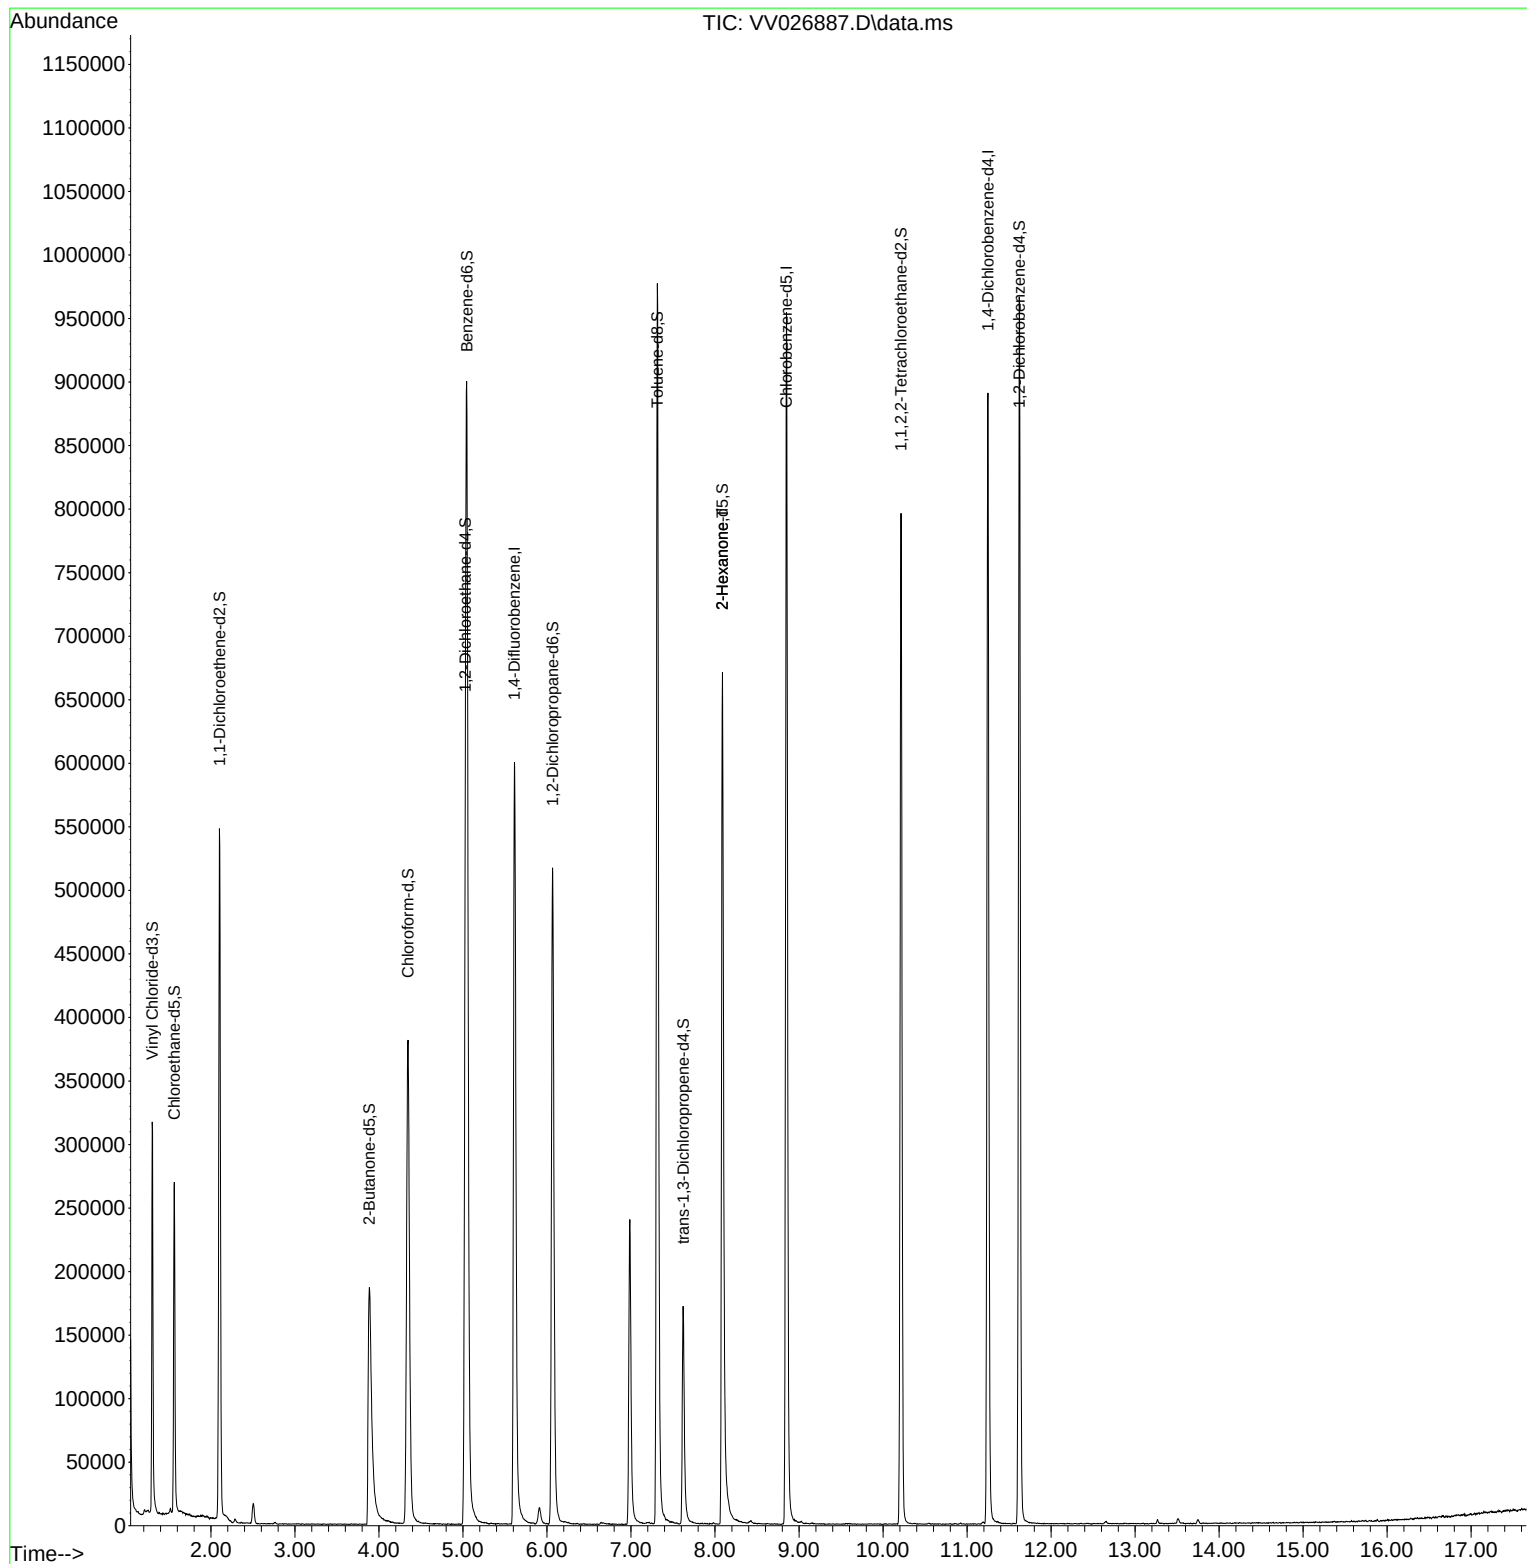

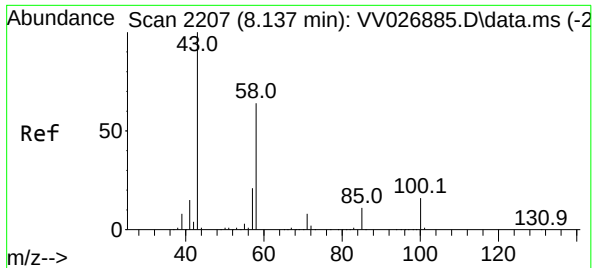

#48
 2-Hexanone
 Concen: 6.210 ug/L
 RT: 8.088 min Scan# 21
 Delta R.T. -0.048 min
 Lab File: VV026887.D
 Acq: 22 Jul 2022 15:07

Instrument :
 MSVOA_V
 ClientSampleId :

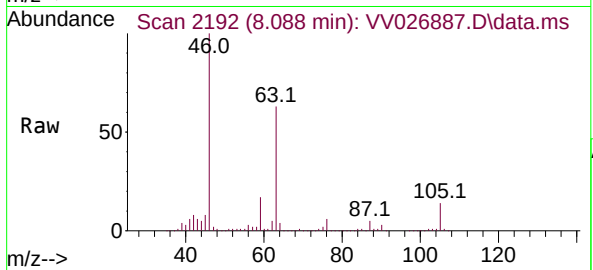

Tgt Ion: 43	Resp: 26651
Ion Ratio	Lower Upper
43 100	
58 35.3	48.8 73.2#
57 36.4	16.6 24.8#
100 4.0	11.6 17.4#

