

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072222\
 Data File : VW026891.D
 Acq On : 22 Jul 2022 16:46
 Operator : SY/MD
 Sample : N3709-15ME
 Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 23 04:55:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	622124	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	612896	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	271602	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	126659	24.274	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	48.540%#
7) Chloroethane-d5	1.552	69	52802	12.509	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	25.020%#
11) 1,1-Dichloroethene-d2	2.073	63	273567	29.142	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.280%#
21) 2-Butanone-d5	3.896	46	282733	80.390	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.390%
24) Chloroform-d	4.339	84	399206	38.875	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.740%
26) 1,2-Dichloroethane-d4	5.024	65	245723	41.832	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.660%
32) Benzene-d6	5.037	84	808060	43.616	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.240%
36) 1,2-Dichloropropane-d6	6.063	67	263263	44.095	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.180%
41) Toluene-d8	7.310	98	658559	40.627	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.260%
43) trans-1,3-Dichloroprop...	7.619	79	102914	41.138	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.280%
47) 2-Hexanone-d5	8.095	63	222318	85.519	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.520%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	362240	39.939	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.880%
66) 1,2-Dichlorobenzene-d4	11.625	152	243349	47.758	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.520%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.433	43	27728	5.091	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026891.D
Acq On : 22 Jul 2022 16:46
Operator : SY/MD
Sample : N3709-15ME
Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jul 23 04:55:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

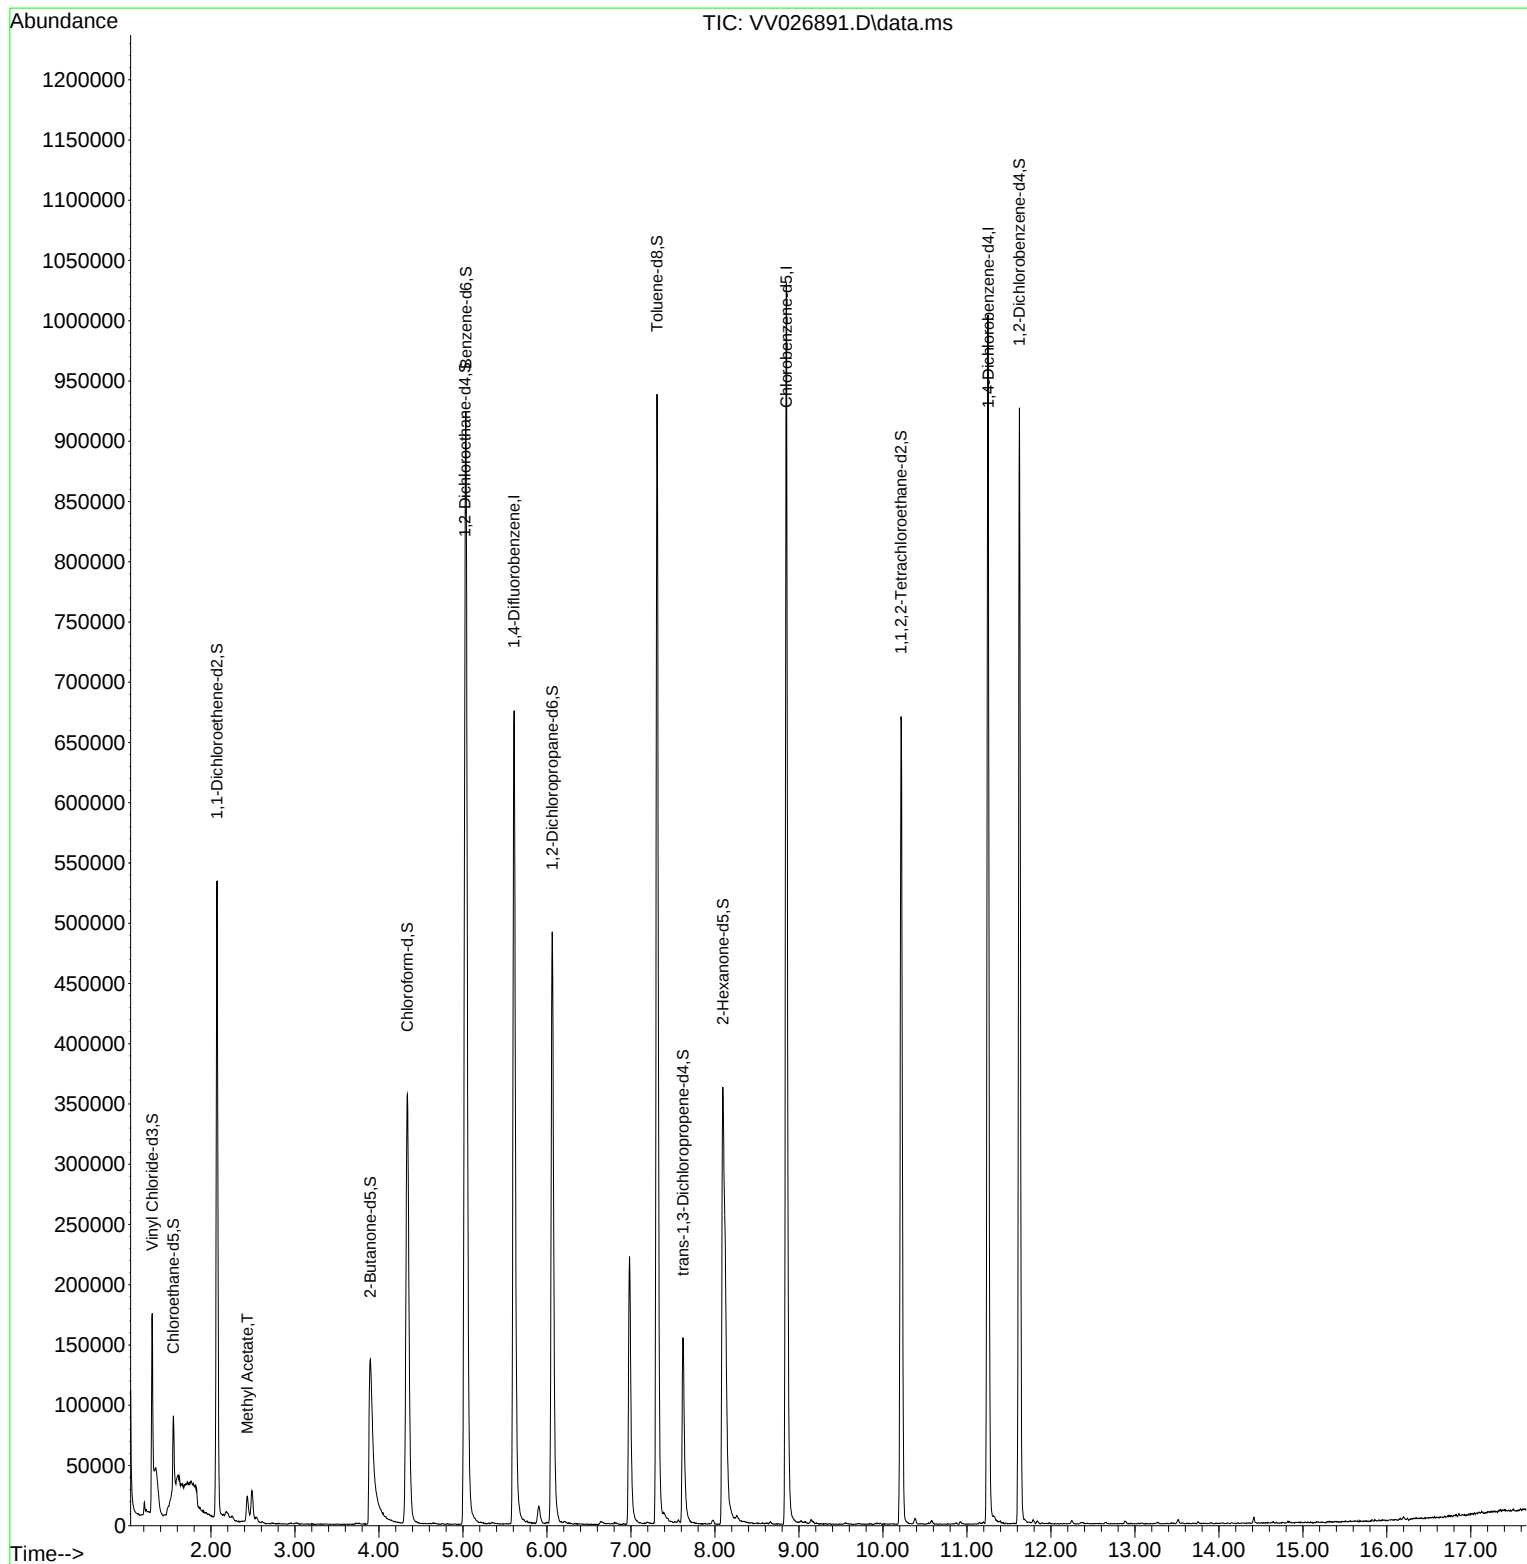

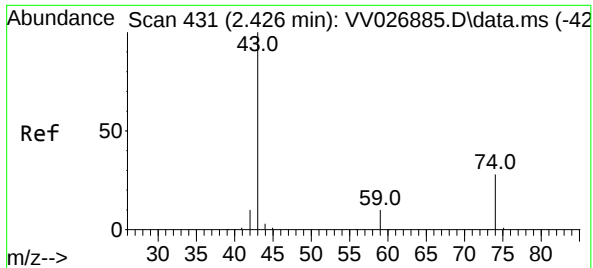

#15
Methyl Acetate
Concen: 5.091 ug/L
RT: 2.433 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV026891.D
Acq: 22 Jul 2022 16:46

Instrument :
MSVOA_V
ClientSampleId :

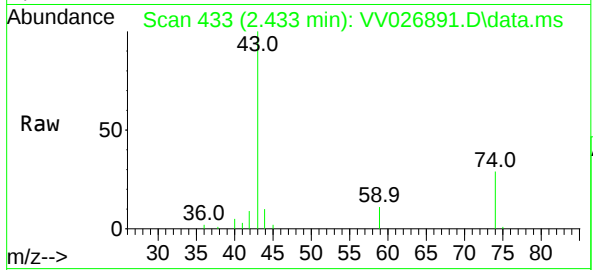

Tgt Ion: 43 Resp: 27728
Ion Ratio Lower Upper
43 100
74 29.4 22.1 33.1

