

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072222\
 Data File : VW026902.D
 Acq On : 22 Jul 2022 21:18
 Operator : SY/MD
 Sample : N3841-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jul 23 04:58:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	553949	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	557965	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	233642	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	205554	44.243	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.480%		
7) Chloroethane-d5	1.561	69	173689	46.211	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.420%		
11) 1,1-Dichloroethene-d2	2.101	63	287346	34.378	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.760%		
21) 2-Butanone-d5	3.879	46	336312	107.392	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	107.390%		
24) Chloroform-d	4.342	84	436916	47.784	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.560%		
26) 1,2-Dichloroethane-d4	5.027	65	263781	50.433	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.860%		
32) Benzene-d6	5.043	84	866888	51.398	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.800%		
36) 1,2-Dichloropropane-d6	6.066	67	283729	52.201	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.400%		
41) Toluene-d8	7.313	98	705337	47.796	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.600%		
43) trans-1,3-Dichloroprop...	7.619	79	103955	45.645	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.300%		
47) 2-Hexanone-d5	8.088	63	249076	105.245	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.240%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	412460	49.953	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.900%		
66) 1,2-Dichlorobenzene-d4	11.622	152	260804	59.500	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	119.000%		
Target Compounds					Qvalue	
13) Acetone	2.172	43	9476	4.309	ug/L	99
61) 1,2,3-Trichloropropane	11.249	75	27246	5.811	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026902.D
Acq On : 22 Jul 2022 21:18
Operator : SY/MD
Sample : N3841-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jul 23 04:58:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

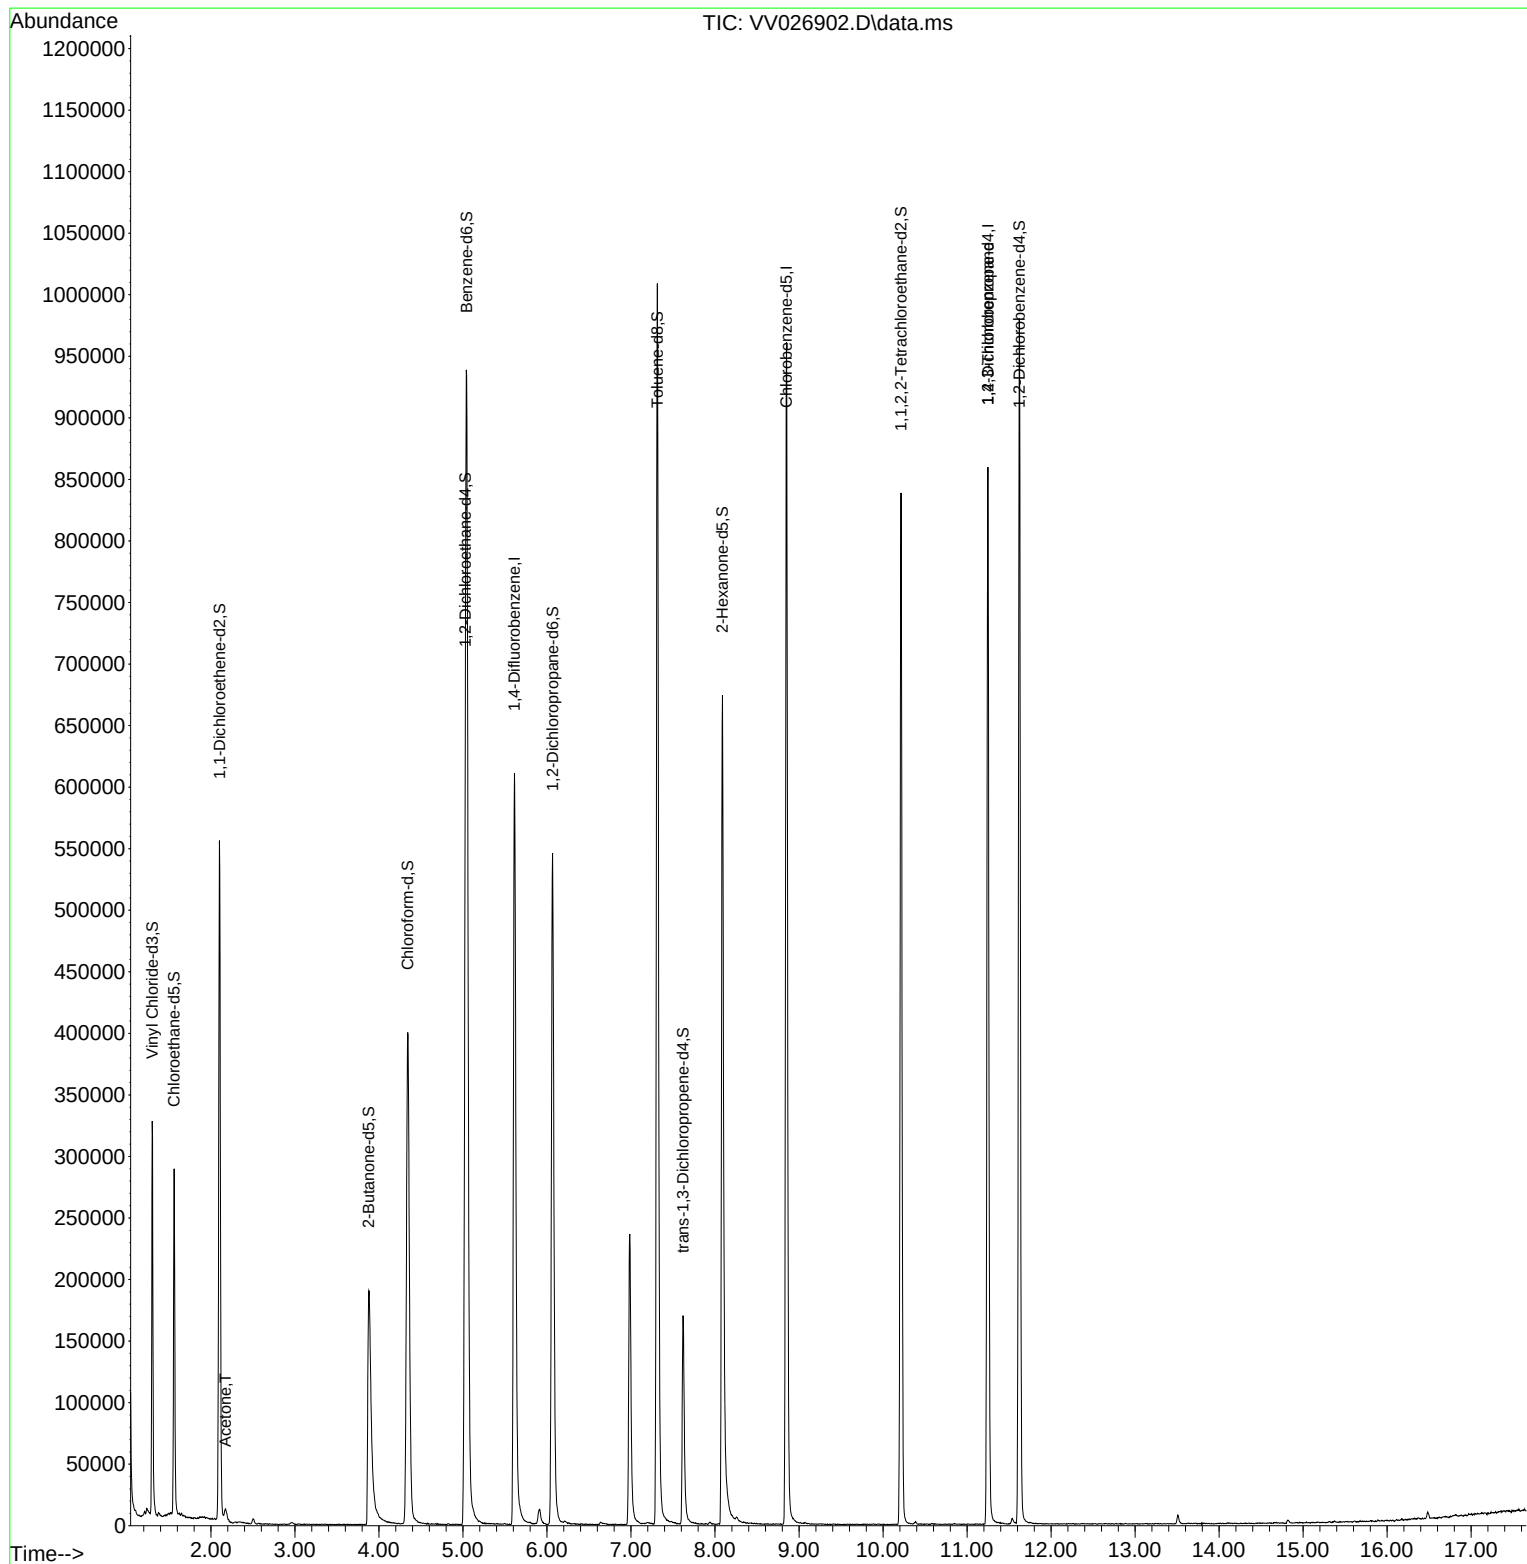

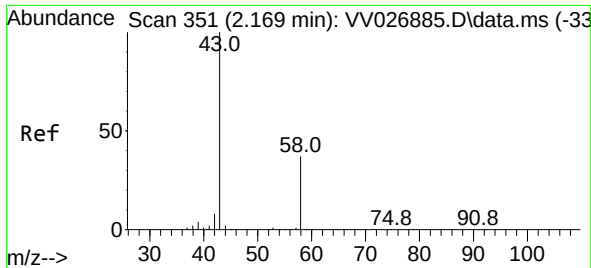

#13

Acetone

Concen: 4.309 ug/L

RT: 2.172 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV026902.D

Acq: 22 Jul 2022 21:18

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 9476

Ion Ratio Lower Upper

43 100

58 36.0 0.0 72.6

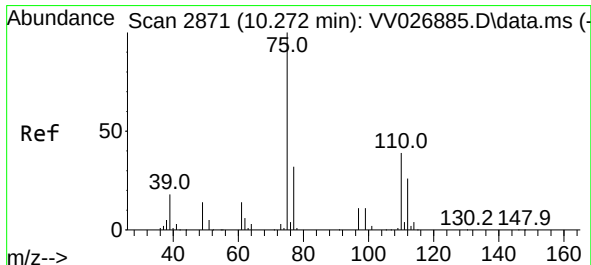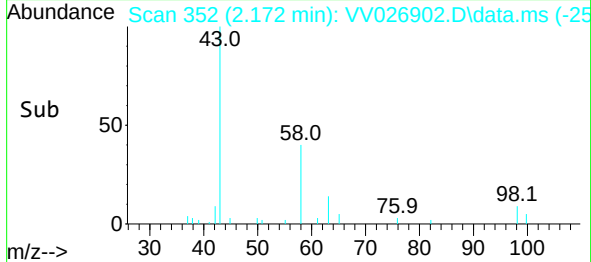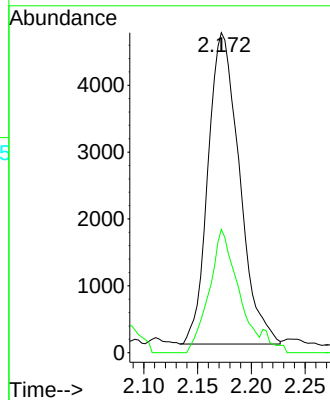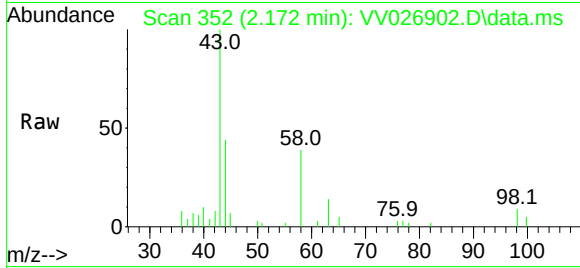

#61

1,2,3-Trichloropropane

Concen: 5.811 ug/L

RT: 11.249 min Scan# 3175

Delta R.T. 0.977 min

Lab File: VV026902.D

Acq: 22 Jul 2022 21:18

Tgt Ion: 75 Resp: 27246

Ion Ratio Lower Upper

75 100

77 29.0 25.6 38.4

110 2.9 31.7 47.5#

