

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072222\
 Data File : VW026890.D
 Acq On : 22 Jul 2022 16:22
 Operator : SY/MD
 Sample : N3709-14ME
 Misc : 4.87g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B28ME

Quant Time: Jul 23 04:55:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Krupa Patel 07/23/2022
 Supervised By :Semsettin Yesilyurt 07/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	614150	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	603483	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	267830	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	200057m	38.839	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.680%		
7) Chloroethane-d5	1.558	69	89978m	21.593	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	43.180%#		
11) 1,1-Dichloroethene-d2	2.072	63	273299	29.492	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	58.980%#		
21) 2-Butanone-d5	3.899	46	293600	84.563	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.560%		
24) Chloroform-d	4.339	84	395277	38.992	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.980%		
26) 1,2-Dichloroethane-d4	5.024	65	244600	42.182	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.360%		
32) Benzene-d6	5.037	84	808218	44.305	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.620%		
36) 1,2-Dichloropropane-d6	6.063	67	258537	43.978	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.960%		
41) Toluene-d8	7.313	98	656703	41.144	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.280%		
43) trans-1,3-Dichloroprop...	7.622	79	103680	42.091	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.180%		
47) 2-Hexanone-d5	8.095	63	218067	85.193	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.190%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	360444	40.361	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.720%		
66) 1,2-Dichlorobenzene-d4	11.625	152	243441	48.449	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.900%		
Target Compounds						Qvalue
15) Methyl Acetate	2.436	43	11243	2.091	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026890.D
Acq On : 22 Jul 2022 16:22
Operator : SY/MD
Sample : N3709-14ME
Misc : 4.87g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
H0B28ME

Quant Time: Jul 23 04:55:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/23/2022
Supervised By :Semsettin Yesilyurt 07/24/2022

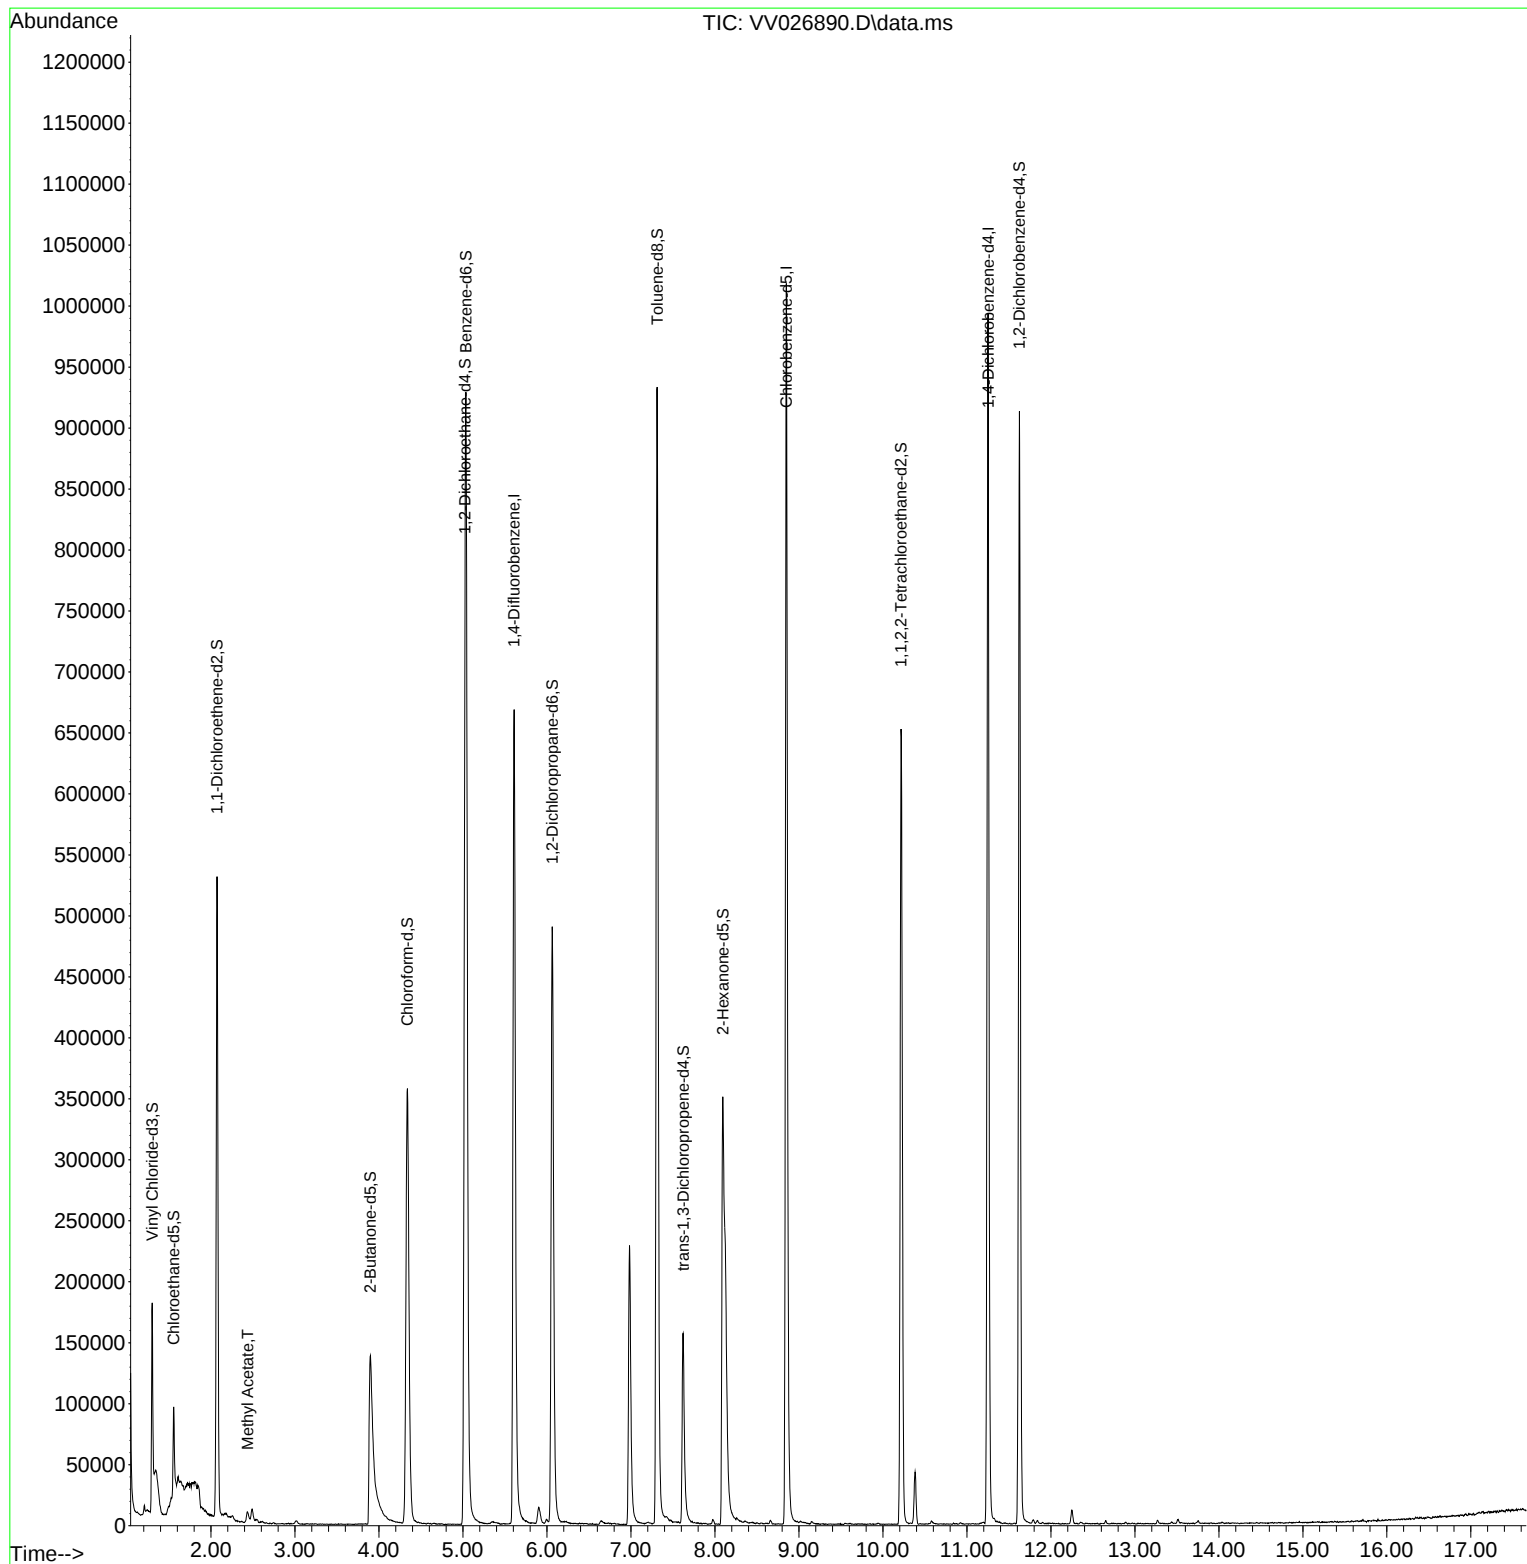

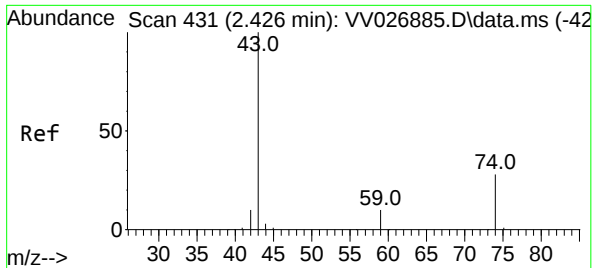

#15
Methyl Acetate
Concen: 2.091 ug/L
RT: 2.436 min Scan# 41
Delta R.T. 0.009 min
Lab File: VV026890.D
Acq: 22 Jul 2022 16:22

Instrument :
MSVOA_V
ClientSampleId :
H0B28ME

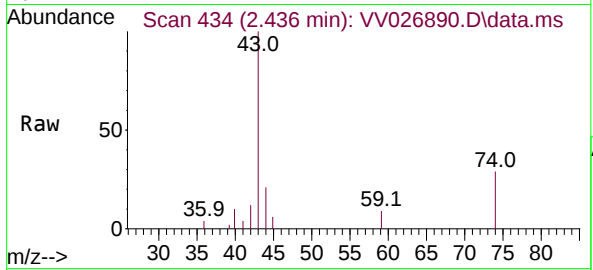

Tgt Ion: 43 Resp: 1124
Ion Ratio Lower Upper
43 100
74 29.5 22.1 33.1

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 07/23/2022
Supervised By :Semsettin Yesilyurt 07/24/2022

