

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072222\
 Data File : VW026892.D
 Acq On : 22 Jul 2022 17:11
 Operator : SY/MD
 Sample : N3823-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B68

Quant Time: Jul 23 04:56:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	566135	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	571794	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	240900	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	220859	46.514	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.020%
7) Chloroethane-d5	1.561	69	182304	47.459	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.920%
11) 1,1-Dichloroethene-d2	2.101	63	299010	35.003	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.000%
21) 2-Butanone-d5	3.876	46	329964	103.097	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.100%
24) Chloroform-d	4.342	84	435311	46.583	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.160%
26) 1,2-Dichloroethane-d4	5.027	65	266759	49.905	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.800%
32) Benzene-d6	5.043	84	875976	50.681	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.360%
36) 1,2-Dichloropropane-d6	6.066	67	286814	51.492	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.980%
41) Toluene-d8	7.313	98	710860	47.006	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.020%
43) trans-1,3-Dichloroprop...	7.619	79	108716	46.581	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.160%
47) 2-Hexanone-d5	8.088	63	250326	103.215	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.220%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	398279	47.069	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.140%
66) 1,2-Dichlorobenzene-d4	11.622	152	263122	58.220	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.440%
Target Compounds						
13) Acetone	2.166	43	14987	6.669	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026892.D
Acq On : 22 Jul 2022 17:11
Operator : SY/MD
Sample : N3823-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B68

Quant Time: Jul 23 04:56:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

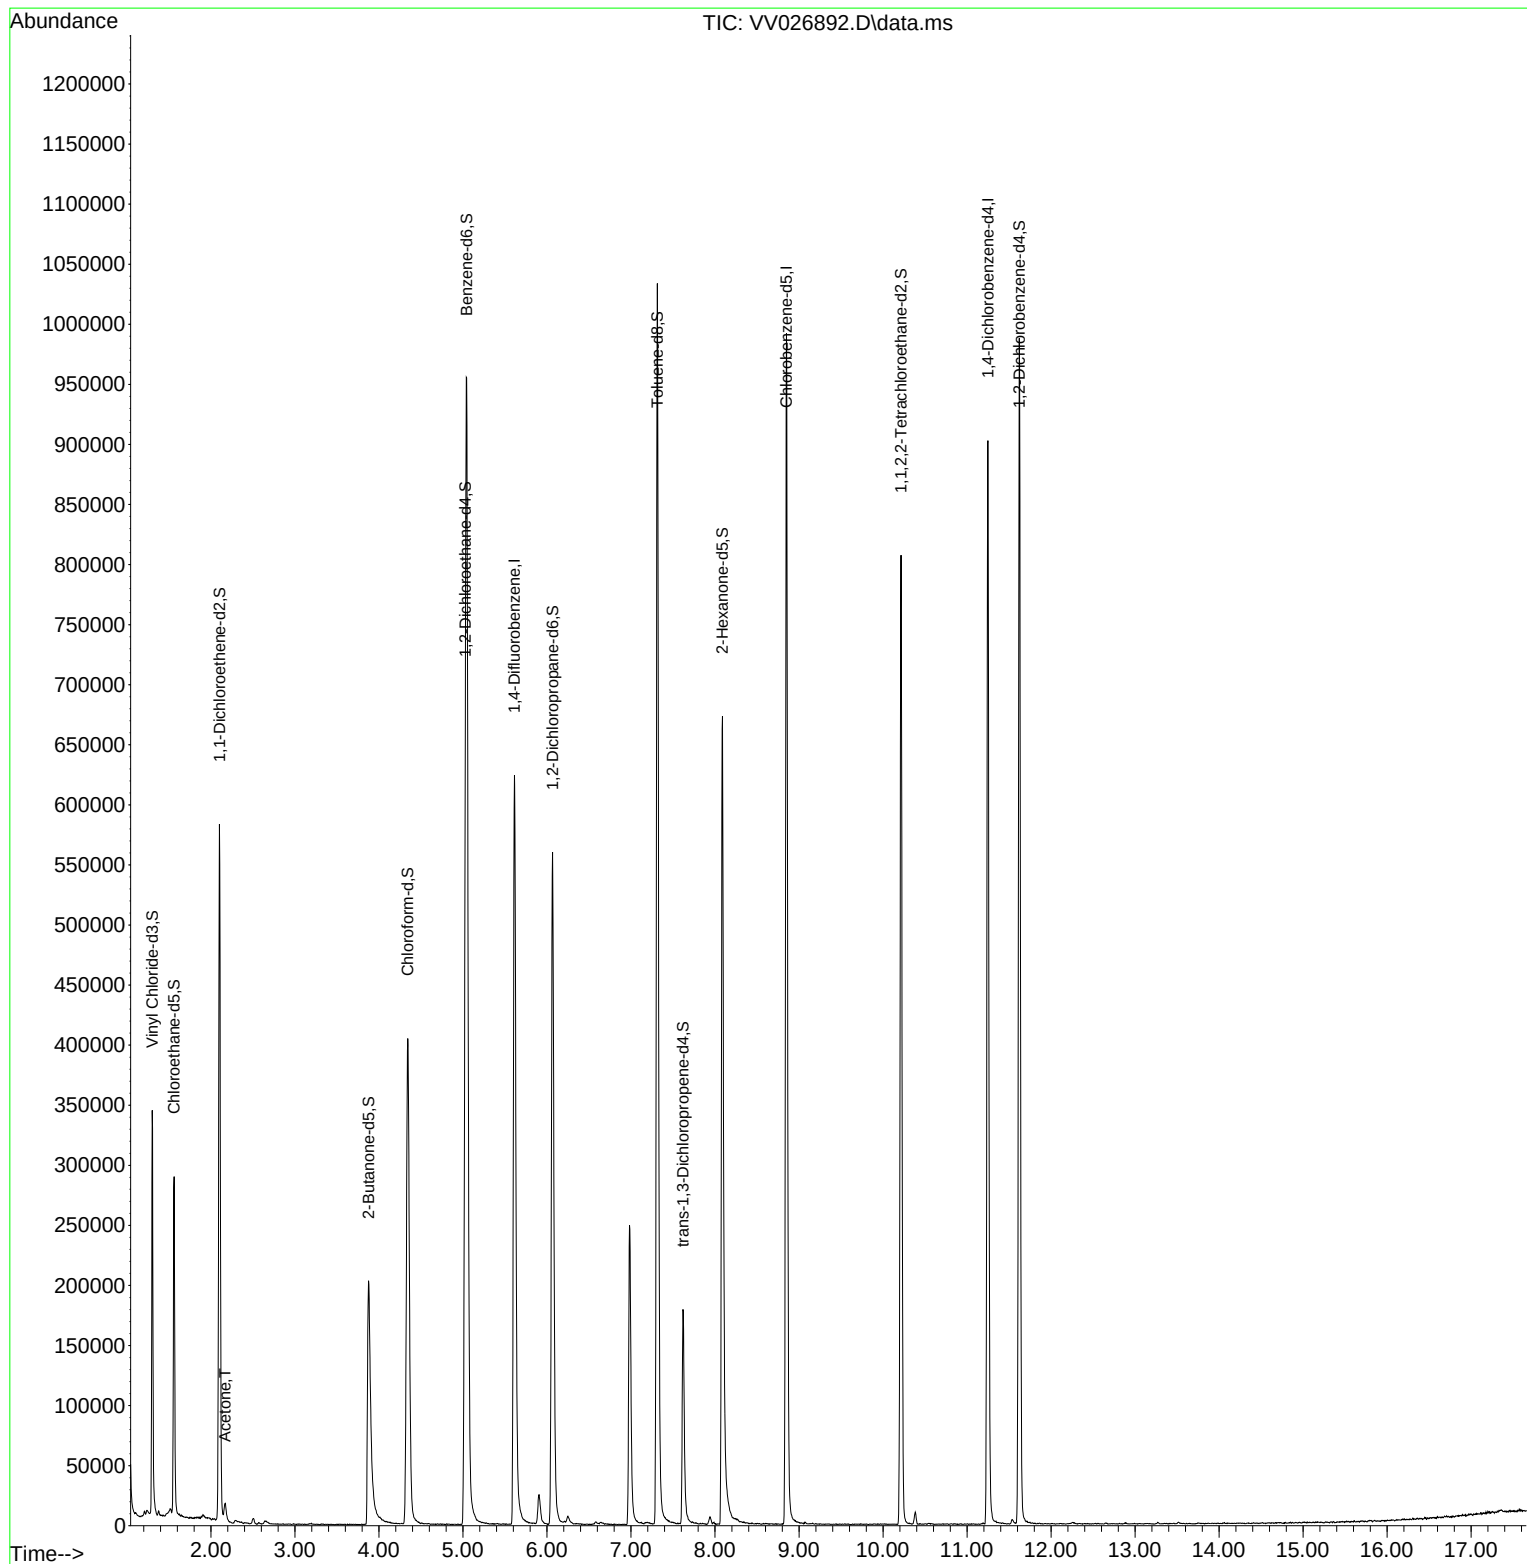

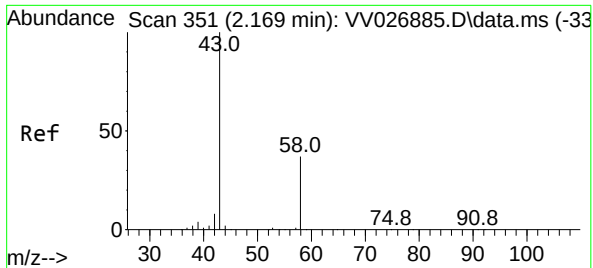

#13
 Acetone
 Concen: 6.669 ug/L
 RT: 2.166 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV026892.D
 Acq: 22 Jul 2022 17:11

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B68

Tgt Ion: 43 Resp: 14987
 Ion Ratio Lower Upper
 43 100
 58 42.4 0.0 72.6

