

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072222\
 Data File : VW026901.D
 Acq On : 22 Jul 2022 20:53
 Operator : SY/MD
 Sample : N3841-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD5

Quant Time: Jul 23 04:58:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	565626	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	563680	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	242462	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	198953	41.938	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.880%		
7) Chloroethane-d5	1.561	69	172256	44.884	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.760%		
11) 1,1-Dichloroethene-d2	2.102	63	279855	32.790	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.580%		
21) 2-Butanone-d5	3.883	46	323190	101.071	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.070%		
24) Chloroform-d	4.343	84	430779	46.140	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.280%		
26) 1,2-Dichloroethane-d4	5.027	65	262723	49.194	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.380%		
32) Benzene-d6	5.047	84	845597	49.628	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.260%		
36) 1,2-Dichloropropane-d6	6.066	67	280523	51.088	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.180%		
41) Toluene-d8	7.314	98	681182	45.691	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.380%		
43) trans-1,3-Dichloroprop...	7.619	79	101340	44.046	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.100%		
47) 2-Hexanone-d5	8.088	63	252144	105.461	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.460%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	408690	48.995	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.980%		
66) 1,2-Dichlorobenzene-d4	11.622	152	260146	57.191	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	114.380%		
Target Compounds					Qvalue	
13) Acetone	2.172	43	5553	2.473	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026901.D
Acq On : 22 Jul 2022 20:53
Operator : SY/MD
Sample : N3841-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD5

Quant Time: Jul 23 04:58:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

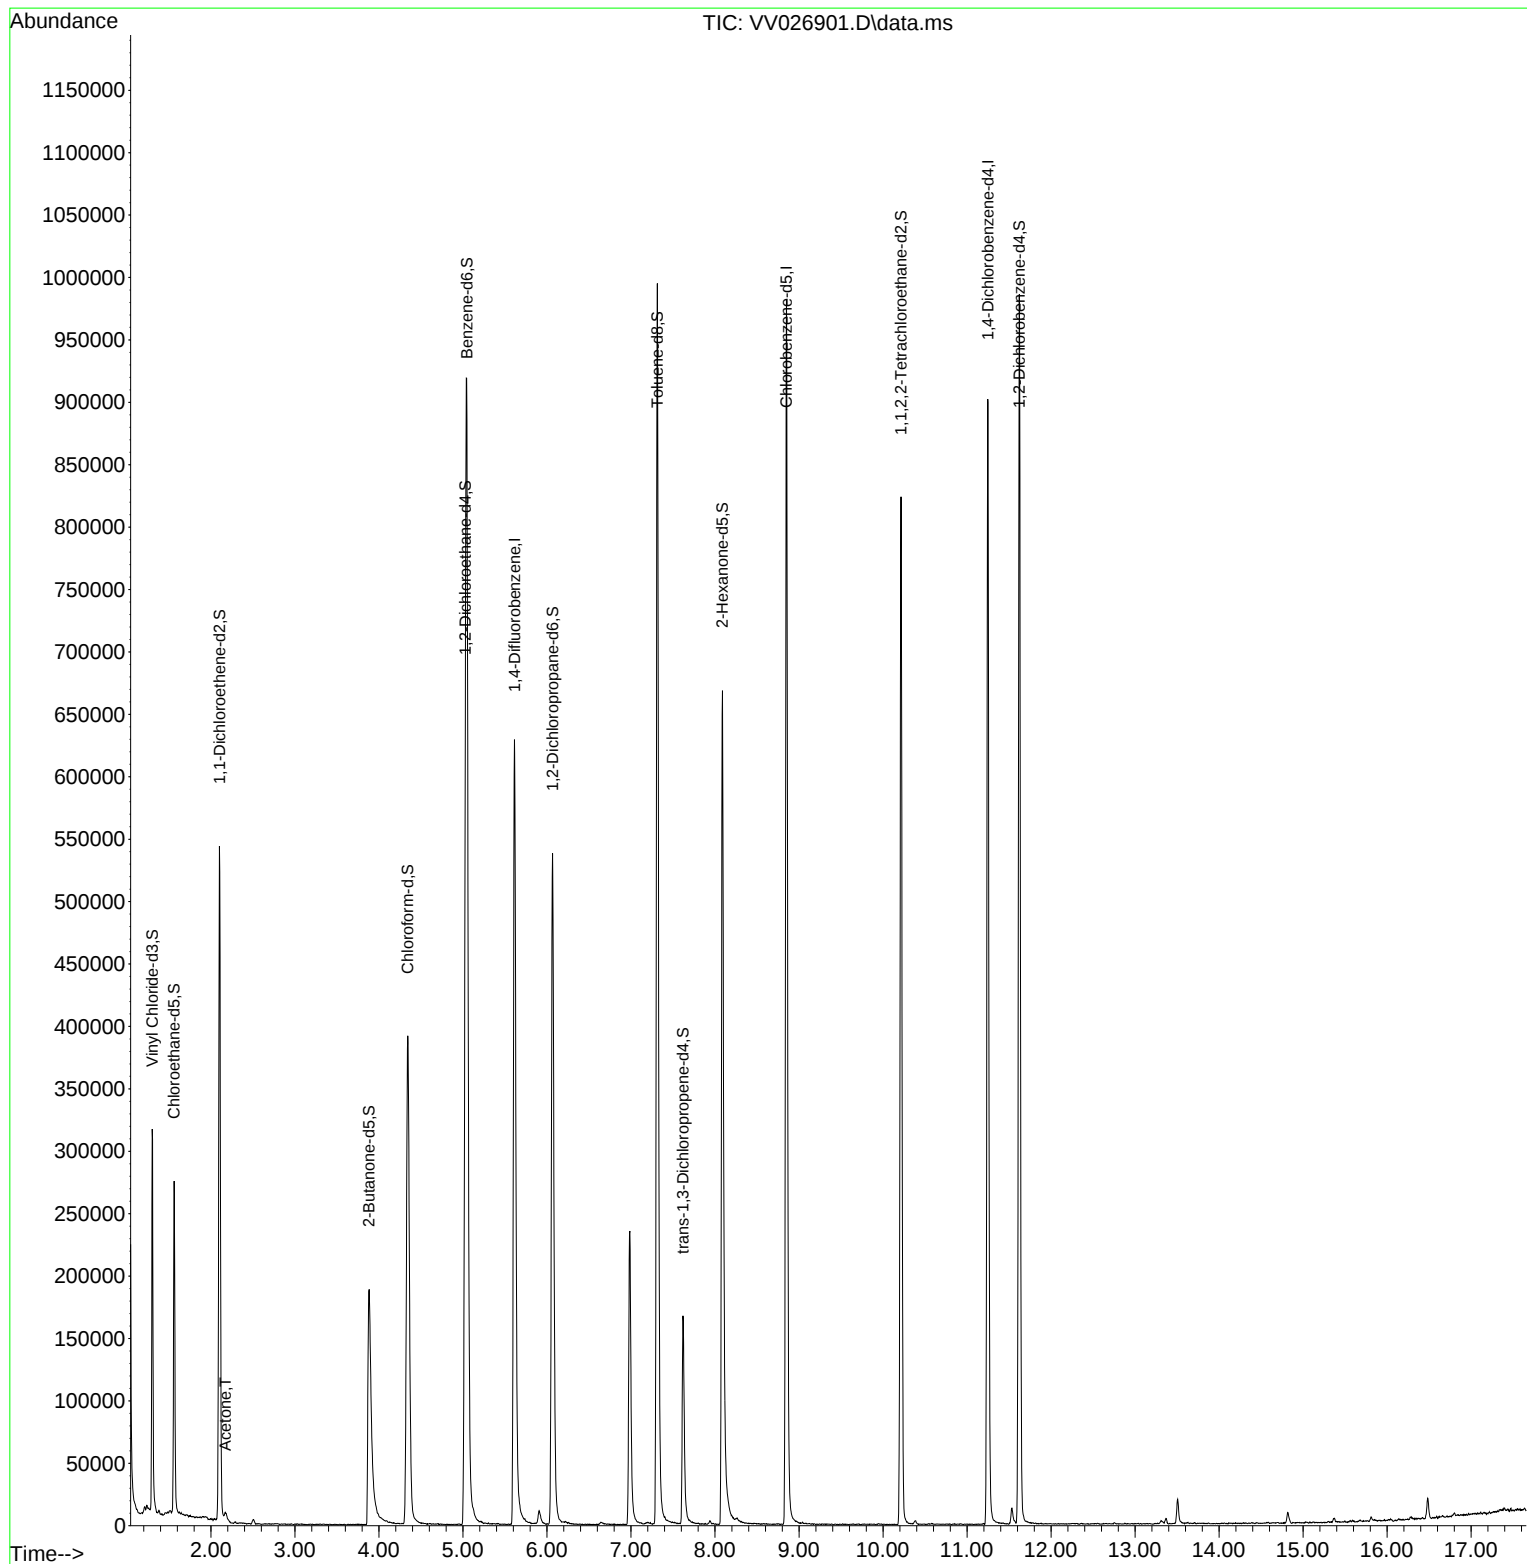

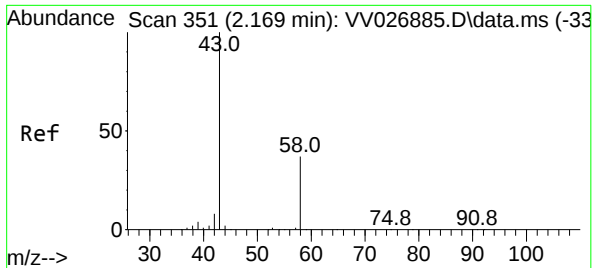

#13
 Acetone
 Concen: 2.473 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV026901.D
 Acq: 22 Jul 2022 20:53

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD5

Tgt Ion: 43 Resp: 5553
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 72.6

