

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072222\
 Data File : VW026902.D
 Acq On : 22 Jul 2022 21:18
 Operator : SY/MD
 Sample : N3841-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD6

Quant Time: Jul 23 04:58:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 23 00:23:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	553949	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	557965	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	233642	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	205554	44.243	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.480%
7) Chloroethane-d5	1.561	69	173689	46.211	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.420%
11) 1,1-Dichloroethene-d2	2.101	63	287346	34.378	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.760%
21) 2-Butanone-d5	3.879	46	336312	107.392	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.390%
24) Chloroform-d	4.342	84	436916	47.784	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.560%
26) 1,2-Dichloroethane-d4	5.027	65	263781	50.433	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.860%
32) Benzene-d6	5.043	84	866888	51.398	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.800%
36) 1,2-Dichloropropane-d6	6.066	67	283729	52.201	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.400%
41) Toluene-d8	7.313	98	705337	47.796	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.600%
43) trans-1,3-Dichloroprop...	7.619	79	103955	45.645	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.300%
47) 2-Hexanone-d5	8.088	63	249076	105.245	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.240%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	412460	49.953	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.900%
66) 1,2-Dichlorobenzene-d4	11.622	152	260804	59.500	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	119.000%
Target Compounds						
					Qvalue	
13) Acetone	2.172	43	9476	4.309	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026902.D
Acq On : 22 Jul 2022 21:18
Operator : SY/MD
Sample : N3841-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD6

Quant Time: Jul 23 04:58:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 23 00:23:15 2022
Response via : Initial Calibration

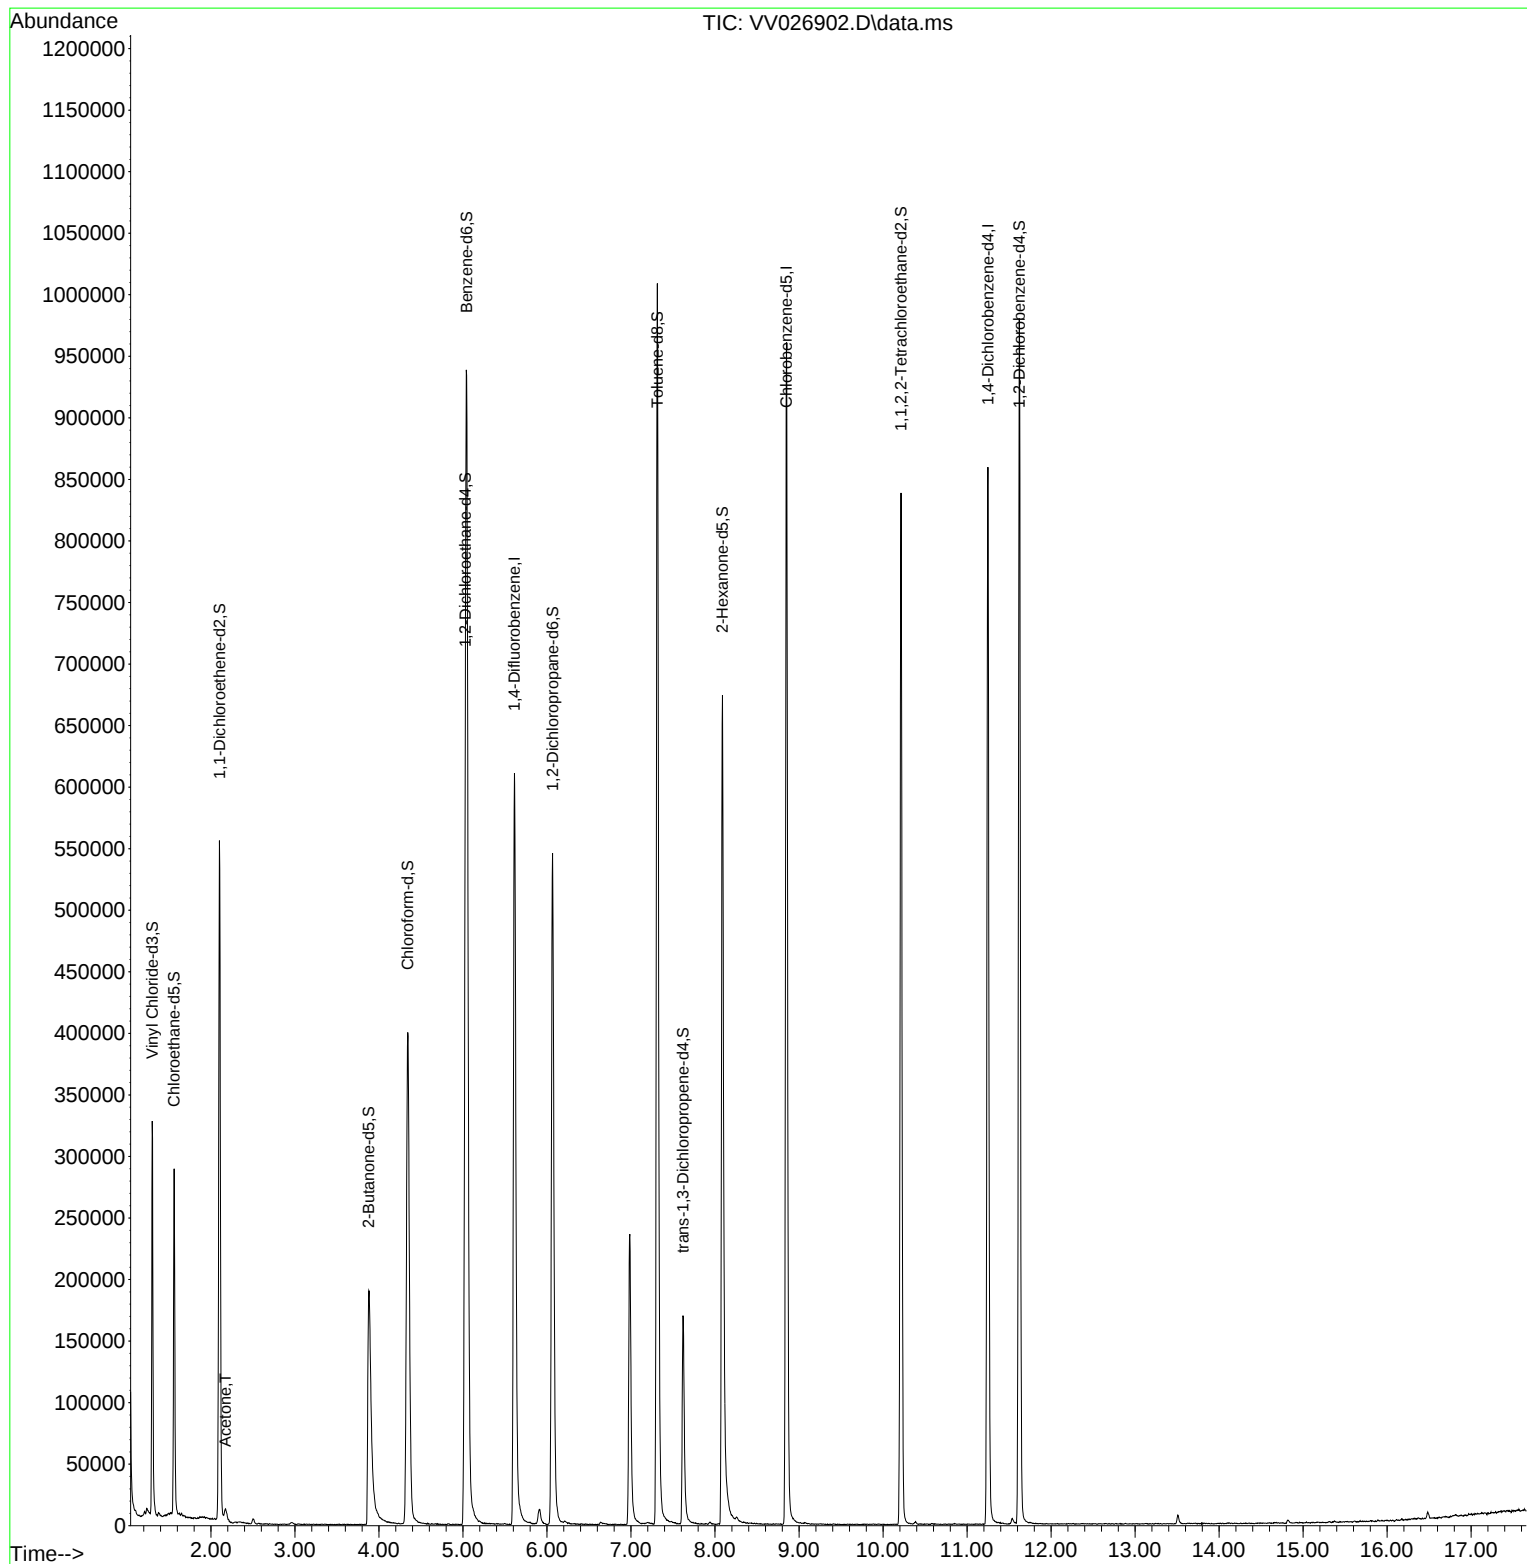

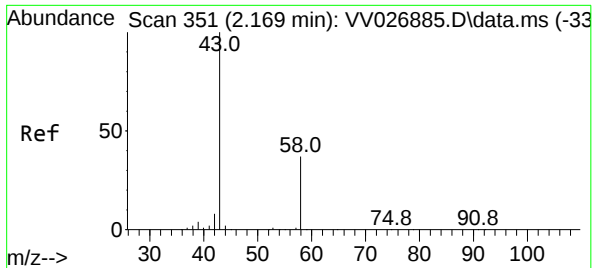

#13
 Acetone
 Concen: 4.309 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV026902.D
 Acq: 22 Jul 2022 21:18

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD6

Tgt Ion: 43 Resp: 9476
 Ion Ratio Lower Upper
 43 100
 58 36.0 0.0 72.6

