

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026898.D
 Acq On : 22 Jul 2022 19:39
 Operator : SY/MD
 Sample : N3841-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M

Title : VOC Analysis

Signal : TIC: VV026898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	99	rVB	322311	329949	13.77%	1.921%
2	1.561	155	162	178	rVB	276237	308307	12.87%	1.795%
3	2.102	319	330	347	rBV	557196	791303	33.03%	4.606%
4	2.343	403	405	410	rVB3	586	399	0.02%	0.002%
5	2.372	411	414	419	rBV2	588	487	0.02%	0.003%
6	2.426	429	431	436	rVB3	404	291	0.01%	0.002%
7	2.500	448	454	463	rVB7	3027	4889	0.20%	0.028%
8	2.568	466	475	476	rBV5	1986	2353	0.10%	0.014%
9	2.735	522	527	529	rBV3	364	311	0.01%	0.002%
10	2.809	547	550	553	rBV	397	298	0.01%	0.002%
11	2.918	581	584	589	rBV3	418	431	0.02%	0.003%
12	2.944	589	592	598	rVB2	495	324	0.01%	0.002%
13	2.973	598	601	604	rBV2	542	356	0.01%	0.002%
14	3.011	610	613	615	rBV2	496	294	0.01%	0.002%
15	3.224	676	679	687	rVB3	442	593	0.02%	0.003%
16	3.384	726	729	732	rBV3	385	316	0.01%	0.002%
17	3.429	738	743	748	rVB2	246	317	0.01%	0.002%
18	3.462	749	753	756	rBV2	358	295	0.01%	0.002%
19	3.587	789	792	799	rBV3	351	403	0.02%	0.002%
20	3.883	873	884	937	rBV	187195	589060	24.59%	3.429%
21	4.269	1002	1004	1007	rVB3	576	301	0.01%	0.002%
22	4.343	1007	1027	1064	rBV	397840	991093	41.37%	5.769%
23	4.664	1124	1127	1130	rBV3	416	290	0.01%	0.002%
24	4.735	1145	1149	1153	rVB3	609	422	0.02%	0.002%
25	4.780	1159	1163	1166	rBV2	372	317	0.01%	0.002%
26	4.867	1185	1190	1200	rVB4	579	856	0.04%	0.005%
27	4.944	1211	1214	1217	rVB2	494	308	0.01%	0.002%
28	5.040	1227	1244	1287	rBV2	929093	2395968	100.00%	13.946%
29	5.236	1304	1305	1311	rVB4	1065	556	0.02%	0.003%
30	5.378	1345	1349	1350	rBV4	568	367	0.02%	0.002%
31	5.426	1361	1364	1368	rVB2	512	368	0.02%	0.002%
32	5.487	1378	1383	1385	rBV4	413	325	0.01%	0.002%
33	5.500	1385	1387	1391	rVB2	652	346	0.01%	0.002%
34	5.535	1393	1398	1400	rBV2	537	311	0.01%	0.002%
35	5.613	1410	1422	1455	rBV	601529	1234805	51.54%	7.187%
36	5.815	1482	1485	1488	rBV3	585	396	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026898.D
 Acq On : 22 Jul 2022 19:39
 Operator : SY/MD
 Sample : N3841-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	5.905	1502	1513	1530	rBV2	24762	51115	2.13%	0.298%
38	6.066	1548	1563	1600	rBV	534393	1113309	46.47%	6.480%
39	6.375	1657	1659	1664	rVB2	609	404	0.02%	0.002%
40	6.410	1667	1670	1673	rVB2	569	372	0.02%	0.002%
41	6.487	1689	1694	1696	rBV3	420	322	0.01%	0.002%
42	6.539	1705	1710	1712	rVB3	637	427	0.02%	0.002%
43	6.635	1735	1740	1742	rBV4	1630	1461	0.06%	0.009%
44	6.738	1770	1772	1776	rVV2	453	348	0.01%	0.002%
45	6.780	1783	1785	1789	rVB2	479	299	0.01%	0.002%
46	6.812	1789	1795	1798	rBV3	448	465	0.02%	0.003%
47	6.847	1804	1806	1812	rVB2	402	308	0.01%	0.002%
48	6.879	1812	1816	1821	rBV	388	362	0.02%	0.002%
49	6.982	1836	1848	1877	rBV	228125	433248	18.08%	2.522%
50	7.143	1895	1898	1900	rBV	388	314	0.01%	0.002%
51	7.314	1939	1951	1980	rBV	991969	1735472	72.43%	10.102%
52	7.619	2035	2046	2079	rBV	163874	298438	12.46%	1.737%
53	7.793	2098	2100	2105	rVB3	907	594	0.02%	0.003%
54	7.838	2112	2114	2118	rVB3	755	489	0.02%	0.003%
55	7.937	2137	2145	2153	rVV4	5689	9720	0.41%	0.057%
56	8.088	2177	2192	2232	rBV	664166	1256095	52.43%	7.311%
57	8.532	2326	2330	2331	rVB2	674	326	0.01%	0.002%
58	8.555	2331	2337	2341	rBV4	518	773	0.03%	0.004%
59	8.850	2417	2429	2458	rBV	942883	1547792	64.60%	9.009%
60	9.079	2497	2500	2502	rBV3	721	425	0.02%	0.002%
61	9.098	2502	2506	2509	rBV4	446	453	0.02%	0.003%
62	9.381	2589	2594	2596	rBV3	441	382	0.02%	0.002%
63	9.494	2625	2629	2633	rBV3	263	293	0.01%	0.002%
64	9.545	2641	2645	2647	rBV2	446	304	0.01%	0.002%
65	9.754	2706	2710	2714	rVB3	574	523	0.02%	0.003%
66	9.776	2714	2717	2721	rBV	374	352	0.01%	0.002%
67	9.947	2767	2770	2775	rVB3	395	308	0.01%	0.002%
68	10.050	2799	2802	2806	rBV3	321	301	0.01%	0.002%
69	10.214	2841	2853	2878	rBV	792119	1251432	52.23%	7.284%
70	10.381	2895	2905	2913	rBV4	5357	8026	0.33%	0.047%
71	10.577	2961	2966	2971	rBV3	905	983	0.04%	0.006%
72	10.657	2988	2991	2995	rVB3	499	355	0.01%	0.002%
73	10.796	3032	3034	3039	rVB	559	370	0.02%	0.002%
74	10.883	3058	3061	3068	rBV3	449	454	0.02%	0.003%
75	10.924	3070	3074	3080	rVB4	361	432	0.02%	0.003%
76	11.027	3103	3106	3109	rBV3	463	351	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026898.D
 Acq On : 22 Jul 2022 19:39
 Operator : SY/MD
 Sample : N3841-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	11.188	3148	3156	3159	rBV2	777	1005	0.04%	0.006%
78	11.249	3163	3175	3209	rBV	825371	1300212	54.27%	7.568%
79	11.538	3261	3265	3266	rBV2	865	572	0.02%	0.003%
80	11.622	3279	3291	3315	rBV	942208	1492545	62.29%	8.688%
81	11.796	3343	3345	3349	rVB2	899	523	0.02%	0.003%
82	11.821	3350	3353	3356	rBV3	536	311	0.01%	0.002%
83	11.947	3389	3392	3396	rBV3	379	318	0.01%	0.002%
84	11.985	3401	3404	3408	rVB2	437	315	0.01%	0.002%
85	12.246	3480	3485	3486	rBV	797	644	0.03%	0.004%
86	12.423	3537	3540	3543	rBV	521	341	0.01%	0.002%
87	12.497	3559	3563	3566	rVB2	461	386	0.02%	0.002%
88	12.558	3578	3582	3587	rBV3	436	388	0.02%	0.002%
89	12.654	3608	3612	3619	rBV2	599	892	0.04%	0.005%
90	12.767	3643	3647	3651	rBV2	498	443	0.02%	0.003%
91	13.098	3748	3750	3758	rVB2	687	687	0.03%	0.004%
92	13.265	3797	3802	3806	rBV2	747	890	0.04%	0.005%
93	13.371	3831	3835	3838	rBV	418	377	0.02%	0.002%
94	13.567	3890	3896	3898	rBV3	514	551	0.02%	0.003%
95	13.580	3898	3900	3903	rVB	698	370	0.02%	0.002%
96	13.599	3903	3906	3911	rVB2	570	513	0.02%	0.003%
97	13.635	3914	3917	3920	rBV2	504	352	0.01%	0.002%
98	14.159	4078	4080	4083	rVB2	613	319	0.01%	0.002%
99	14.744	4259	4262	4264	rBV2	625	439	0.02%	0.003%
100	15.271	4423	4426	4427	rBV2	686	396	0.02%	0.002%




Sum of corrected areas: 17179991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026898.D
Acq On : 22 Jul 2022 19:39
Operator : SY/MD
Sample : N3841-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

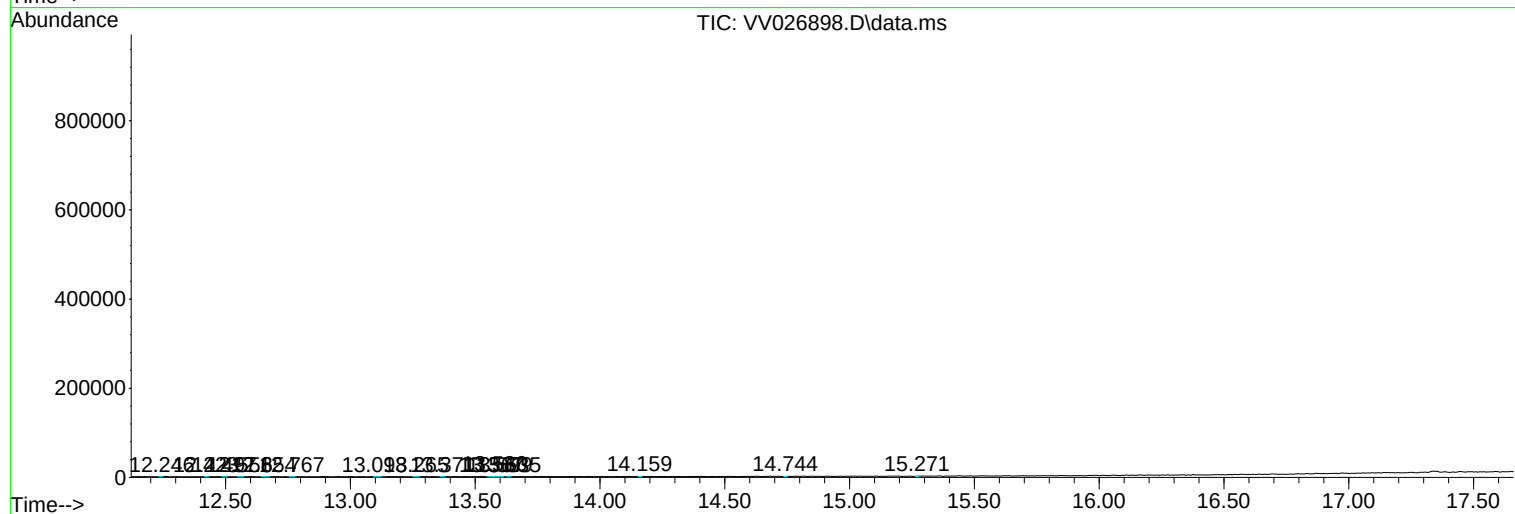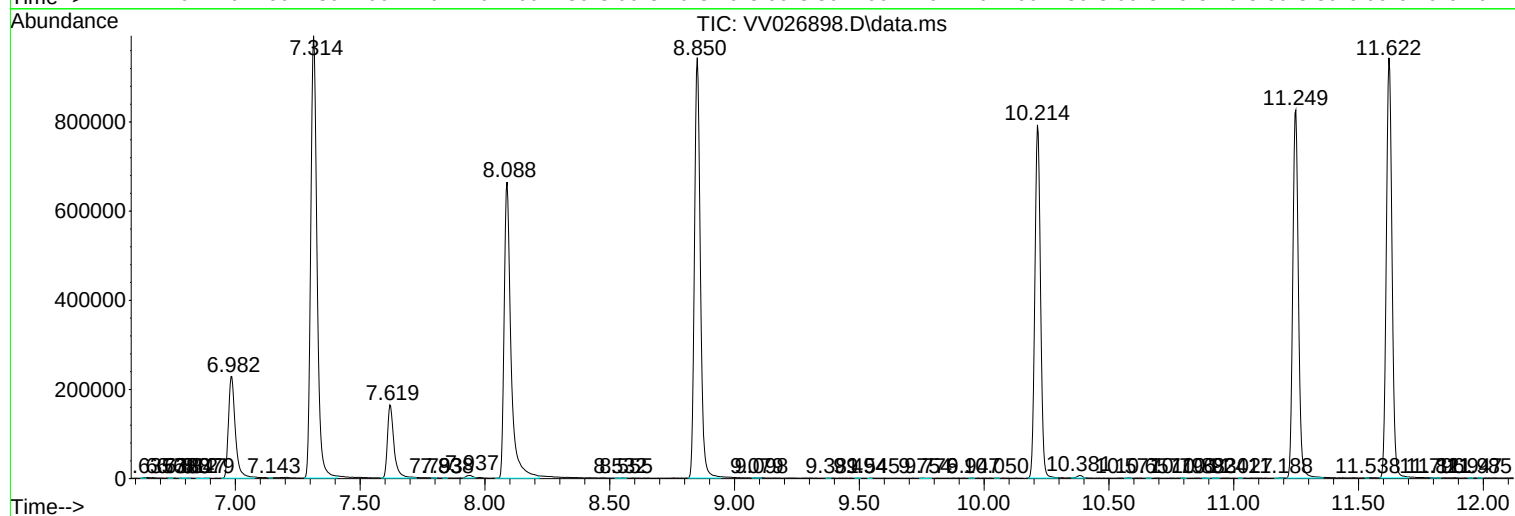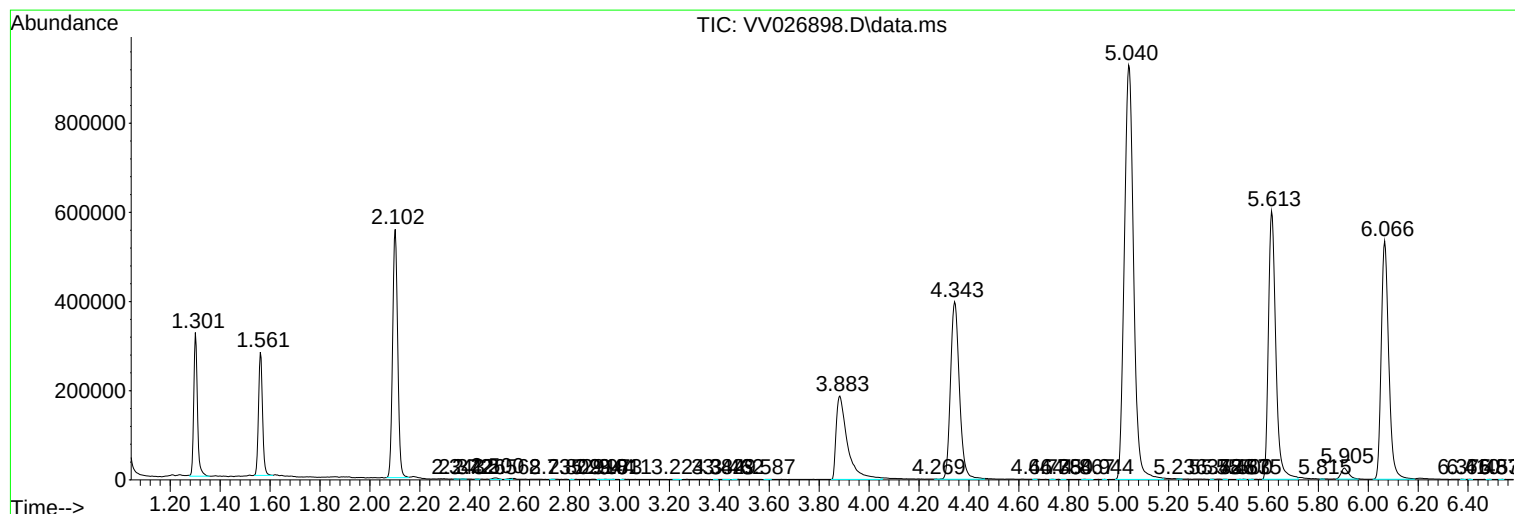

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026898.D
Acq On : 22 Jul 2022 19:39
Operator : SY/MD
Sample : N3841-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026898.D
Acq On : 22 Jul 2022 19:39
Operator : SY/MD
Sample : N3841-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
