

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026901.D
 Acq On : 22 Jul 2022 20:53
 Operator : SY/MD
 Sample : N3841-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	306913	317625	13.32%	1.819%
2	1.561	155	162	177	rVB	265381	297828	12.49%	1.706%
3	2.102	319	330	346	rBV	539349	768497	32.24%	4.401%
4	2.507	446	456	464	rVB3	3848	6485	0.27%	0.037%
5	2.957	594	596	603	rVB	579	528	0.02%	0.003%
6	2.999	605	609	612	rBV3	523	420	0.02%	0.002%
7	3.179	663	665	669	rVV	383	309	0.01%	0.002%
8	3.410	734	737	745	rVB2	376	471	0.02%	0.003%
9	3.590	785	793	796	rVB3	455	530	0.02%	0.003%
10	3.883	873	884	926	rBV	188499	566831	23.78%	3.246%
11	4.343	1011	1027	1078	rVV	390819	977949	41.02%	5.601%
12	4.645	1116	1121	1123	rBV4	523	414	0.02%	0.002%
13	4.738	1144	1150	1152	rBV2	447	430	0.02%	0.002%
14	5.040	1226	1244	1291	rBV2	918608	2384014	100.00%	13.653%
15	5.304	1322	1326	1329	rVB4	895	625	0.03%	0.004%
16	5.362	1340	1344	1346	rBV3	355	328	0.01%	0.002%
17	5.423	1360	1363	1369	rVB3	696	581	0.02%	0.003%
18	5.613	1410	1422	1458	rBV	628548	1292819	54.23%	7.404%
19	5.905	1503	1513	1529	rBV2	10164	21097	0.88%	0.121%
20	5.998	1539	1542	1548	rBV5	693	538	0.02%	0.003%
21	6.066	1548	1563	1596	rBV	537407	1109250	46.53%	6.353%
22	6.256	1619	1622	1628	rVB7	1022	851	0.04%	0.005%
23	6.458	1679	1685	1688	rVB3	482	505	0.02%	0.003%
24	6.484	1688	1693	1694	rBV	470	383	0.02%	0.002%
25	6.642	1734	1742	1749	rBV3	1904	3506	0.15%	0.020%
26	6.687	1754	1756	1764	rVB4	659	822	0.03%	0.005%
27	6.725	1764	1768	1775	rBV3	535	523	0.02%	0.003%
28	6.770	1779	1782	1788	rVB3	401	401	0.02%	0.002%
29	6.986	1836	1849	1880	rBV	235212	442947	18.58%	2.537%
30	7.269	1933	1937	1938	rBV3	542	441	0.02%	0.003%
31	7.314	1939	1951	1978	rBV	993476	1726699	72.43%	9.889%
32	7.619	2036	2046	2068	rBV	166594	295886	12.41%	1.695%
33	7.799	2100	2102	2108	rVB4	996	857	0.04%	0.005%
34	7.883	2126	2128	2136	rVB3	658	452	0.02%	0.003%
35	7.941	2136	2146	2153	rBV5	2894	4553	0.19%	0.026%
36	8.088	2179	2192	2225	rBV	668027	1251709	52.50%	7.168%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026901.D
 Acq On : 22 Jul 2022 20:53
 Operator : SY/MD
 Sample : N3841-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	8.522	2325	2327	2332	rVB3	733	599	0.03%	0.003%
38	8.548	2332	2335	2338	rBV	625	407	0.02%	0.002%
39	8.584	2343	2346	2348	rVB2	557	334	0.01%	0.002%
40	8.728	2387	2391	2394	rBV3	404	435	0.02%	0.002%
41	8.786	2405	2409	2411	rBV3	374	317	0.01%	0.002%
42	8.850	2416	2429	2464	rBV	980578	1604986	67.32%	9.192%
43	9.043	2486	2489	2493	rVB4	1004	599	0.03%	0.003%
44	9.182	2529	2532	2538	rVB4	577	596	0.02%	0.003%
45	9.246	2547	2552	2557	rBV5	388	396	0.02%	0.002%
46	9.281	2559	2563	2567	rVB3	448	425	0.02%	0.002%
47	9.333	2575	2579	2582	rBV3	560	519	0.02%	0.003%
48	9.387	2593	2596	2602	rVB2	463	400	0.02%	0.002%
49	9.429	2602	2609	2610	rBV2	452	376	0.02%	0.002%
50	9.484	2622	2626	2633	rBV3	506	719	0.03%	0.004%
51	9.519	2634	2637	2640	rVV2	614	350	0.01%	0.002%
52	9.567	2650	2652	2658	rVB3	324	314	0.01%	0.002%
53	9.706	2691	2695	2703	rVB3	593	725	0.03%	0.004%
54	9.892	2751	2753	2757	rVB2	541	354	0.01%	0.002%
55	9.944	2765	2769	2775	rBV4	611	762	0.03%	0.004%
56	9.982	2779	2781	2786	rVB2	487	380	0.02%	0.002%
57	10.011	2786	2790	2797	rBV2	402	449	0.02%	0.003%
58	10.079	2808	2811	2817	rBV2	324	306	0.01%	0.002%
59	10.214	2841	2853	2874	rBV	823476	1299222	54.50%	7.441%
60	10.387	2898	2907	2914	rVB5	2628	4297	0.18%	0.025%
61	10.442	2919	2924	2926	rBV3	310	334	0.01%	0.002%
62	10.545	2950	2956	2958	rBV2	563	535	0.02%	0.003%
63	10.580	2964	2967	2969	rBV3	688	406	0.02%	0.002%
64	10.638	2982	2985	2990	rBV2	311	310	0.01%	0.002%
65	10.747	3016	3019	3024	rBV	358	348	0.01%	0.002%
66	10.834	3041	3046	3050	rBV2	459	498	0.02%	0.003%
67	10.854	3050	3052	3057	rVB2	634	417	0.02%	0.002%
68	10.973	3084	3089	3093	rBV2	377	411	0.02%	0.002%
69	11.063	3112	3117	3120	rVB2	458	455	0.02%	0.003%
70	11.198	3156	3159	3163	rVB3	659	518	0.02%	0.003%
71	11.246	3163	3174	3198	rBV	901440	1388445	58.24%	7.952%
72	11.477	3243	3246	3251	rVB5	526	493	0.02%	0.003%
73	11.535	3252	3264	3279	rBV4	12896	25056	1.05%	0.143%
74	11.622	3279	3291	3315	rBV	984355	1548181	64.94%	8.866%
75	12.085	3431	3435	3439	rVB2	515	378	0.02%	0.002%
76	12.352	3513	3518	3519	rBV	563	442	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026901.D
 Acq On : 22 Jul 2022 20:53
 Operator : SY/MD
 Sample : N3841-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	12.362	3519	3521	3525	rVB2	533	408	0.02%	0.002%
78	12.551	3577	3580	3586	rBV4	443	492	0.02%	0.003%
79	12.690	3620	3623	3627	rBV2	428	385	0.02%	0.002%
80	12.751	3639	3642	3650	rVB5	1052	1233	0.05%	0.007%
81	12.879	3680	3682	3686	rVB3	668	365	0.02%	0.002%
82	12.966	3704	3709	3712	rVB2	444	449	0.02%	0.003%
83	13.101	3745	3751	3753	rBV3	467	474	0.02%	0.003%
84	13.310	3809	3816	3828	rVV5	2519	5244	0.22%	0.030%
85	13.368	3828	3834	3845	rVB6	4465	6444	0.27%	0.037%
86	13.506	3868	3877	3894	rBV	19314	33105	1.39%	0.190%
87	13.596	3902	3905	3908	rBV4	600	503	0.02%	0.003%
88	13.616	3908	3911	3913	rBV4	557	348	0.01%	0.002%
89	14.059	4047	4049	4056	rVB3	682	633	0.03%	0.004%
90	14.114	4064	4066	4069	rBV3	912	581	0.02%	0.003%
91	14.172	4081	4084	4087	rBV2	547	427	0.02%	0.002%
92	14.358	4137	4142	4143	rBV3	606	504	0.02%	0.003%
93	14.442	4164	4168	4169	rBV3	750	529	0.02%	0.003%
94	14.776	4271	4272	4276	rBV2	737	350	0.01%	0.002%
95	14.818	4276	4285	4297	rVB4	8674	14994	0.63%	0.086%
96	14.879	4300	4304	4306	rBV2	849	659	0.03%	0.004%
97	15.030	4347	4351	4352	rBV3	942	572	0.02%	0.003%
98	15.078	4364	4366	4369	rBV2	688	414	0.02%	0.002%
99	15.365	4451	4455	4456	rBV3	2158	1501	0.06%	0.009%
100	16.484	4794	4803	4817	rVB	16229	27156	1.14%	0.156%




Sum of corrected areas: 17461368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026901.D
Acq On : 22 Jul 2022 20:53
Operator : SY/MD
Sample : N3841-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

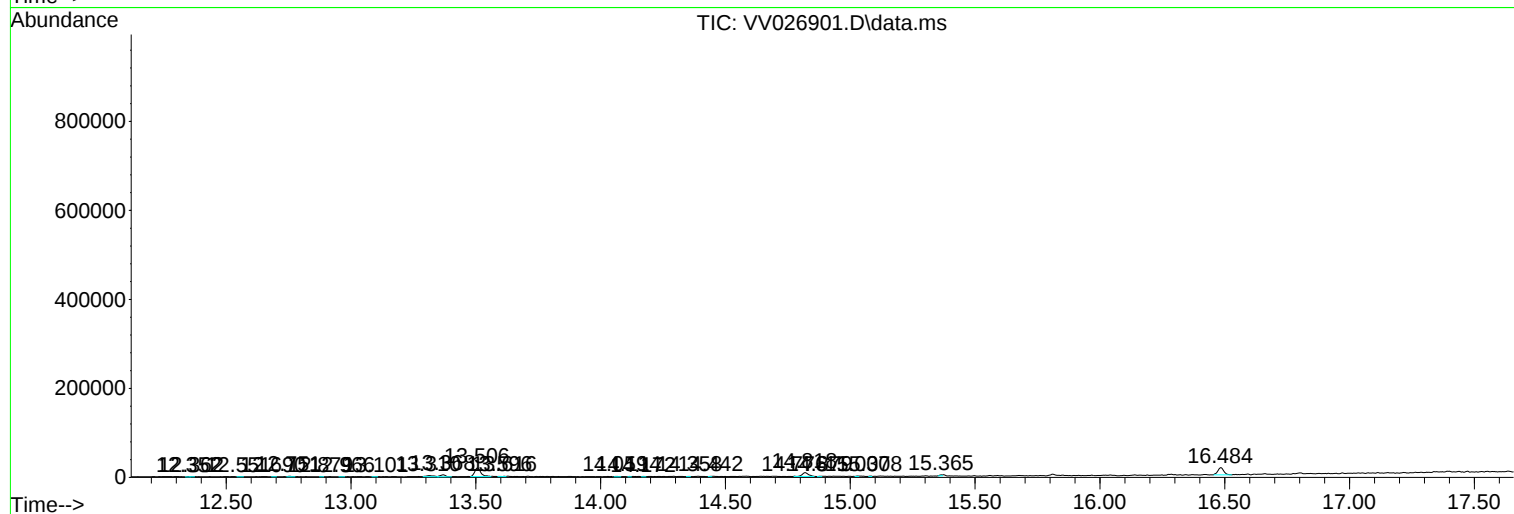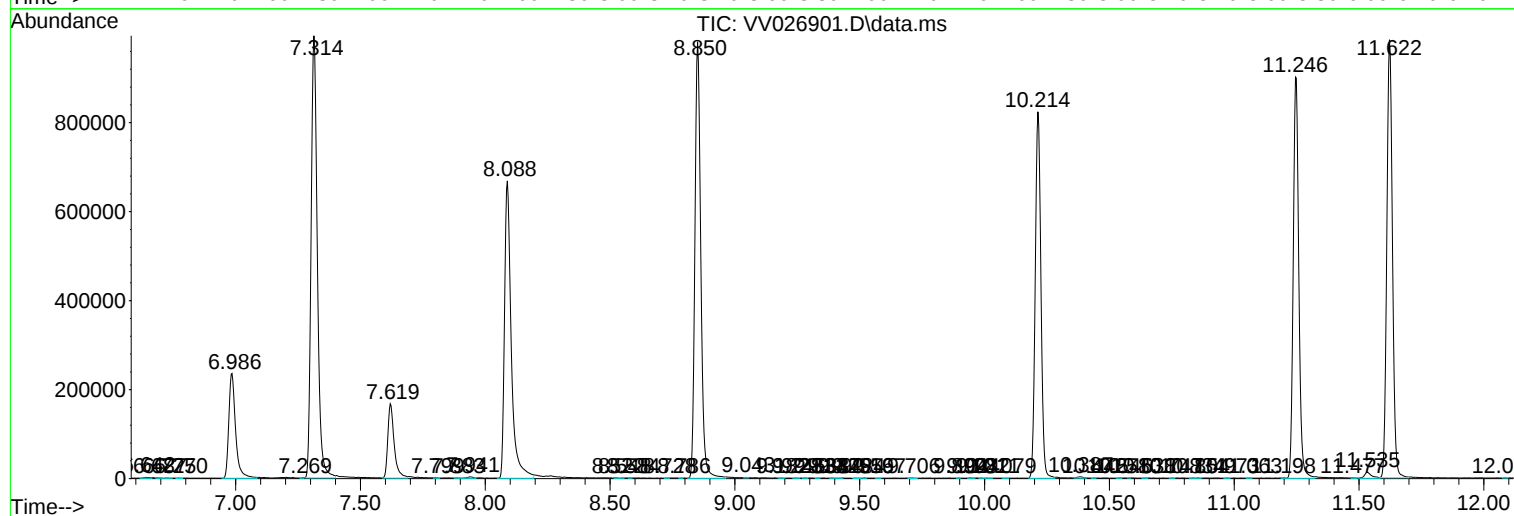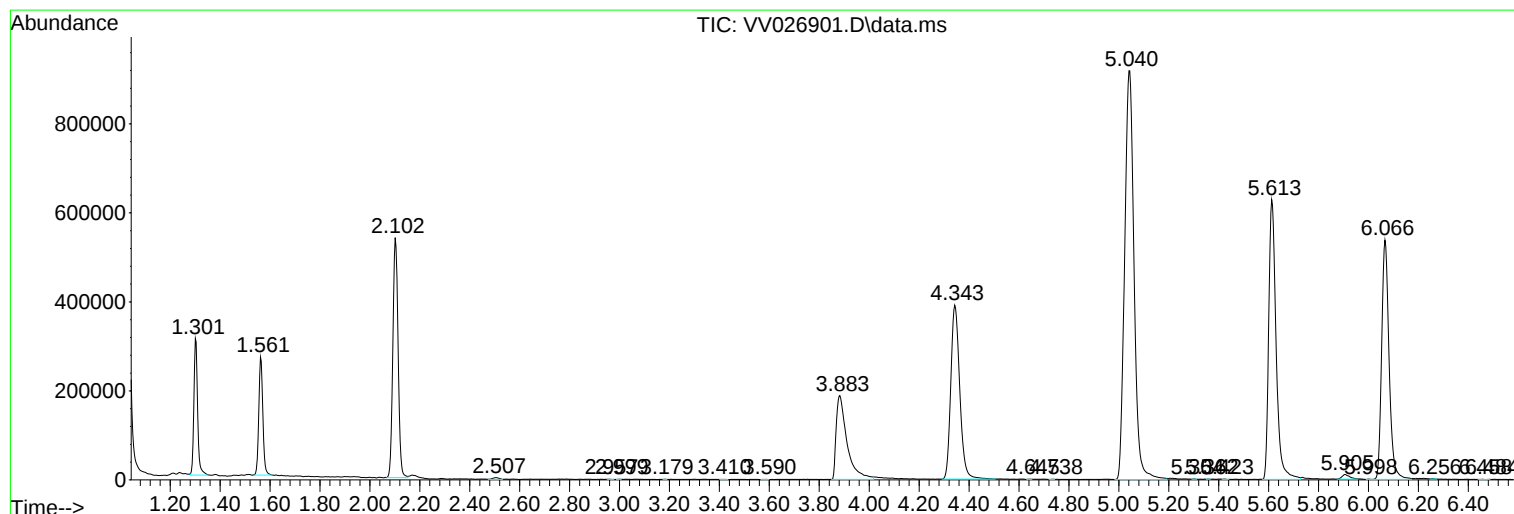

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026901.D
Acq On : 22 Jul 2022 20:53
Operator : SY/MD
Sample : N3841-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026901.D
Acq On : 22 Jul 2022 20:53
Operator : SY/MD
Sample : N3841-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc