

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026904.D
 Acq On : 22 Jul 2022 22:07
 Operator : SY/MD
 Sample : N3841-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

Signal : TIC: VV026904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	293373	302926	13.16%	1.798%
2	1.561	155	162	179	rVB	258827	287635	12.50%	1.707%
3	2.101	321	330	344	rBV	517356	726913	31.58%	4.314%
4	2.503	447	455	464	rBV3	4309	6609	0.29%	0.039%
5	2.590	480	482	484	rBV	536	156	0.01%	0.001%
6	2.767	526	537	556	rVB2	28182	60483	2.63%	0.359%
7	3.098	637	640	642	rVB2	229	120	0.01%	0.001%
8	3.124	642	648	650	rBV3	364	371	0.02%	0.002%
9	3.252	686	688	690	rBV	166	90	0.00%	0.001%
10	3.301	692	703	708	rBV4	933	1611	0.07%	0.010%
11	3.397	728	733	738	rBV3	294	362	0.02%	0.002%
12	3.432	742	744	746	rVB	326	146	0.01%	0.001%
13	3.519	768	771	773	rBV3	193	130	0.01%	0.001%
14	3.661	811	815	816	rBV2	164	119	0.01%	0.001%
15	3.738	835	839	840	rBV	288	190	0.01%	0.001%
16	3.760	844	846	852	rVB	277	141	0.01%	0.001%
17	3.793	852	856	857	rBV	119	75	0.00%	0.000%
18	3.809	859	861	866	rVB2	214	156	0.01%	0.001%
19	3.834	866	869	870	rBV	283	119	0.01%	0.001%
20	3.879	873	883	932	rBV	186909	555468	24.13%	3.296%
21	4.342	1011	1027	1056	rBV	380459	942797	40.96%	5.595%
22	4.863	1185	1189	1191	rBV2	178	152	0.01%	0.001%
23	4.876	1191	1193	1196	rVV	423	270	0.01%	0.002%
24	4.902	1199	1201	1204	rVB2	272	108	0.00%	0.001%
25	4.918	1204	1206	1209	rVB	232	86	0.00%	0.001%
26	4.940	1210	1213	1214	rBV	267	135	0.01%	0.001%
27	5.043	1227	1245	1287	rBV2	883539	2301948	100.00%	13.660%
28	5.400	1353	1356	1362	rBV4	689	724	0.03%	0.004%
29	5.436	1365	1367	1370	rBV2	405	268	0.01%	0.002%
30	5.481	1378	1381	1383	rBV3	407	266	0.01%	0.002%
31	5.551	1401	1403	1406	rBV	431	236	0.01%	0.001%
32	5.612	1410	1422	1459	rBV	588943	1226245	53.27%	7.277%
33	5.908	1504	1514	1528	rBV4	9059	19732	0.86%	0.117%
34	6.066	1549	1563	1597	rBV	517967	1075731	46.73%	6.383%
35	6.307	1635	1638	1640	rBV3	336	176	0.01%	0.001%
36	6.339	1646	1648	1649	rBV2	354	140	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026904.D
 Acq On : 22 Jul 2022 22:07
 Operator : SY/MD
 Sample : N3841-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

37	6.400	1666	1667	1668	rBV2	259	63	0.00%	0.000%
38	6.432	1675	1677	1682	rVB2	440	206	0.01%	0.001%
39	6.455	1682	1684	1686	rBV2	229	160	0.01%	0.001%
40	6.484	1690	1693	1698	rBV3	449	297	0.01%	0.002%
41	6.513	1700	1702	1705	rBV	272	164	0.01%	0.001%
42	6.564	1714	1718	1719	rBV	314	192	0.01%	0.001%
43	6.600	1727	1729	1731	rBV2	254	113	0.00%	0.001%
44	6.641	1734	1742	1746	rBV5	1365	1922	0.08%	0.011%
45	6.751	1774	1776	1778	rVB	240	90	0.00%	0.001%
46	6.760	1778	1779	1781	rBV	225	111	0.00%	0.001%
47	6.776	1782	1784	1788	rVB3	382	199	0.01%	0.001%
48	6.834	1799	1802	1807	rBV3	317	219	0.01%	0.001%
49	6.931	1830	1832	1834	rBV2	150	85	0.00%	0.001%
50	6.985	1837	1849	1874	rBV	225885	421387	18.31%	2.501%
51	7.272	1935	1938	1939	rBV2	468	239	0.01%	0.001%
52	7.313	1939	1951	1985	rVV	941668	1669565	72.53%	9.907%
53	7.619	2037	2046	2069	rBV	157241	279843	12.16%	1.661%
54	7.879	2125	2127	2131	rVB4	745	404	0.02%	0.002%
55	8.043	2175	2178	2181	rBV	224	189	0.01%	0.001%
56	8.088	2181	2192	2228	rBV	655460	1223345	53.14%	7.259%
57	8.571	2339	2342	2345	rBV2	522	357	0.02%	0.002%
58	8.673	2372	2374	2378	rVB2	436	255	0.01%	0.002%
59	8.693	2378	2380	2384	rVB2	285	192	0.01%	0.001%
60	8.718	2384	2388	2391	rBV2	410	272	0.01%	0.002%
61	8.738	2391	2394	2397	rVB2	517	321	0.01%	0.002%
62	8.754	2397	2399	2400	rBV	426	164	0.01%	0.001%
63	8.850	2417	2429	2456	rBV	924782	1527556	66.36%	9.065%
64	9.152	2517	2523	2530	rBV7	1091	1569	0.07%	0.009%
65	9.265	2555	2558	2563	rBV3	449	417	0.02%	0.002%
66	9.326	2574	2577	2578	rBV2	224	124	0.01%	0.001%
67	9.558	2644	2649	2653	rVB2	1683	1576	0.07%	0.009%
68	9.603	2661	2663	2669	rBV2	392	408	0.02%	0.002%
69	9.644	2673	2676	2679	rBV	265	188	0.01%	0.001%
70	9.741	2699	2706	2709	rBV2	445	574	0.02%	0.003%
71	9.779	2715	2718	2721	rBV2	294	215	0.01%	0.001%
72	9.799	2721	2724	2728	rBV2	543	396	0.02%	0.002%
73	9.837	2734	2736	2739	rBV	210	112	0.00%	0.001%
74	9.892	2748	2753	2757	rBV3	393	440	0.02%	0.003%
75	10.111	2819	2821	2825	rBV3	286	224	0.01%	0.001%
76	10.214	2841	2853	2874	rBV	809716	1267211	55.05%	7.520%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
 Data File : VV026904.D
 Acq On : 22 Jul 2022 22:07
 Operator : SY/MD
 Sample : N3841-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Title : VOC Analysis

77	10.435	2920	2922	2924	rBV	324	168	0.01%	0.001%
78	10.458	2928	2929	2930	rBV	307	68	0.00%	0.000%
79	10.519	2945	2948	2951	rBV2	420	305	0.01%	0.002%
80	10.554	2955	2959	2961	rBV3	472	368	0.02%	0.002%
81	10.635	2979	2984	2986	rBV	376	365	0.02%	0.002%
82	10.850	3047	3051	3055	rBV3	727	626	0.03%	0.004%
83	10.947	3079	3081	3084	rBV3	258	109	0.00%	0.001%
84	11.021	3100	3104	3107	rBV3	341	291	0.01%	0.002%
85	11.037	3107	3109	3110	rBV3	243	109	0.00%	0.001%
86	11.165	3144	3149	3151	rBV2	389	378	0.02%	0.002%
87	11.249	3163	3175	3202	rBV	842165	1316655	57.20%	7.813%
88	11.529	3251	3262	3276	rBV2	34922	57865	2.51%	0.343%
89	11.622	3279	3291	3316	rBV	950584	1489444	64.70%	8.838%
90	12.049	3418	3424	3432	rVB6	1870	2625	0.11%	0.016%
91	12.117	3437	3445	3454	rVB2	9671	15024	0.65%	0.089%
92	12.464	3550	3553	3554	rBV2	1816	984	0.04%	0.006%
93	12.728	3628	3635	3641	rBV4	4051	5843	0.25%	0.035%
94	12.885	3677	3684	3692	rVB3	7923	10472	0.45%	0.062%
95	13.184	3774	3777	3780	rBV2	571	433	0.02%	0.003%
96	13.303	3812	3814	3816	rBV2	1307	803	0.03%	0.005%
97	13.506	3868	3877	3897	rBV	16821	29986	1.30%	0.178%
98	13.593	3902	3904	3905	rBV	741	272	0.01%	0.002%
99	14.146	4073	4076	4079	rBV3	526	441	0.02%	0.003%
100	14.821	4279	4286	4287	rBV3	3711	4052	0.18%	0.024%




Sum of corrected areas: 16851884

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026904.D
Acq On : 22 Jul 2022 22:07
Operator : SY/MD
Sample : N3841-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

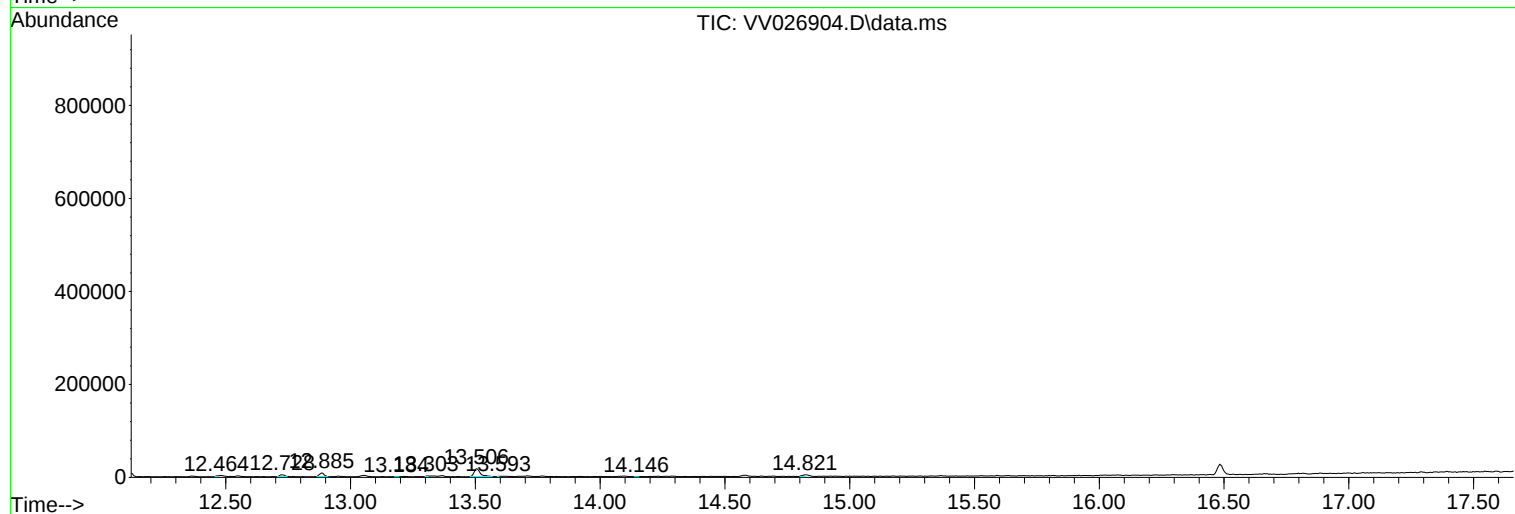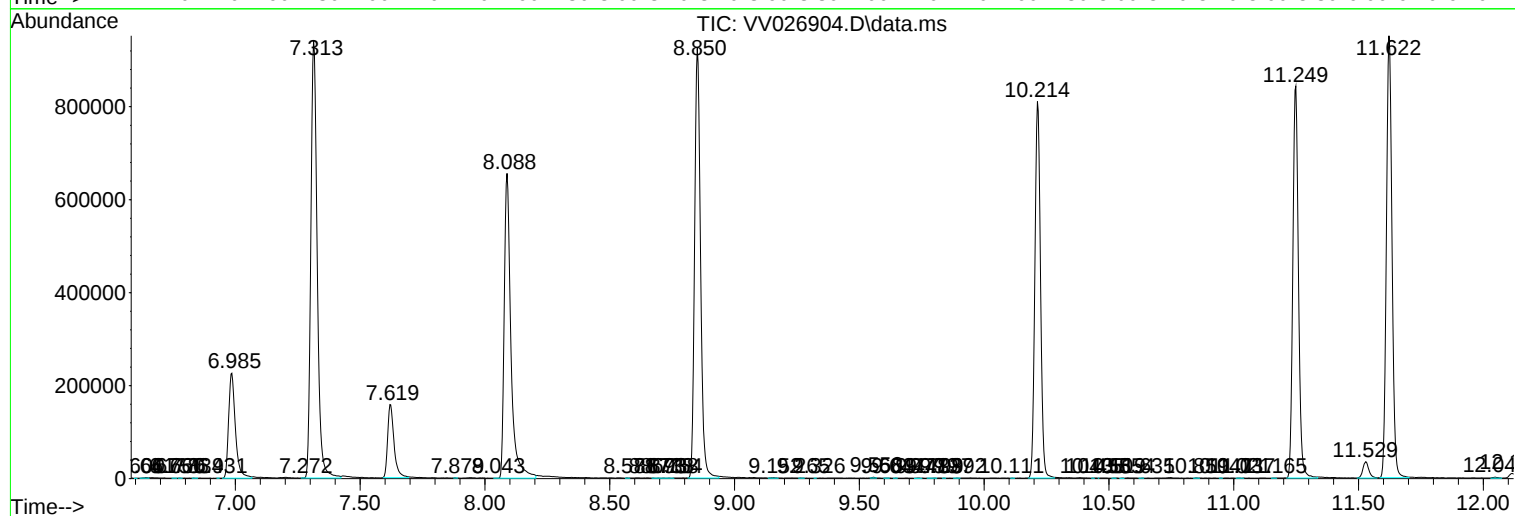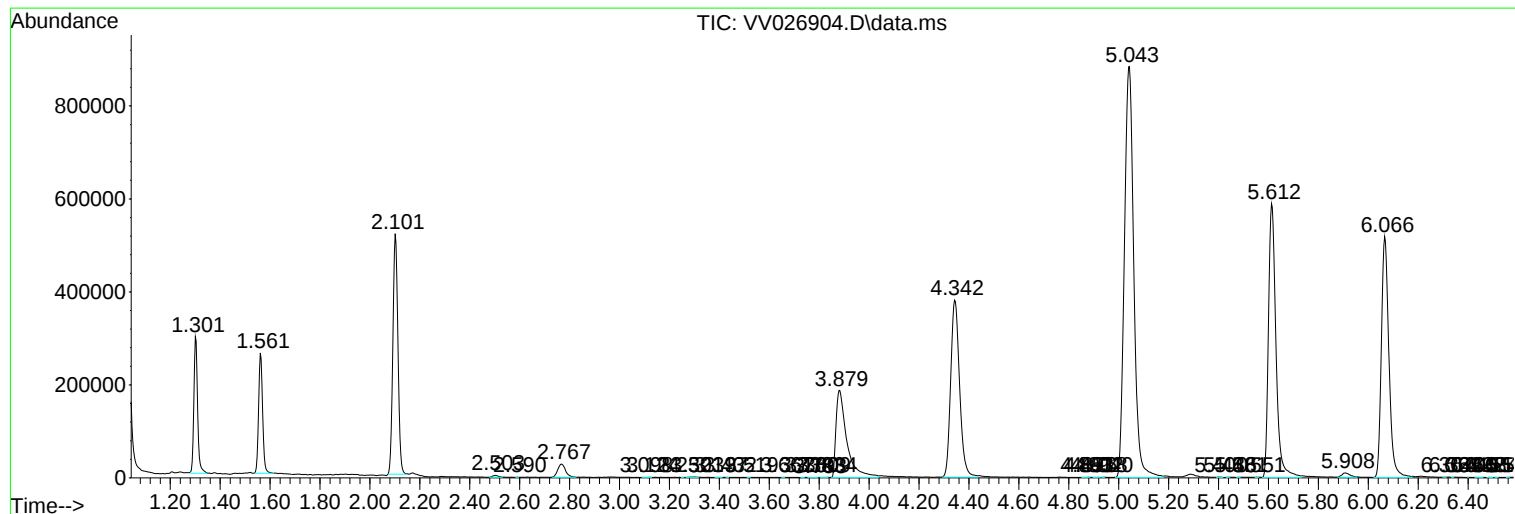

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026904.D
Acq On : 22 Jul 2022 22:07
Operator : SY/MD
Sample : N3841-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026904.D
Acq On : 22 Jul 2022 22:07
Operator : SY/MD
Sample : N3841-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc