
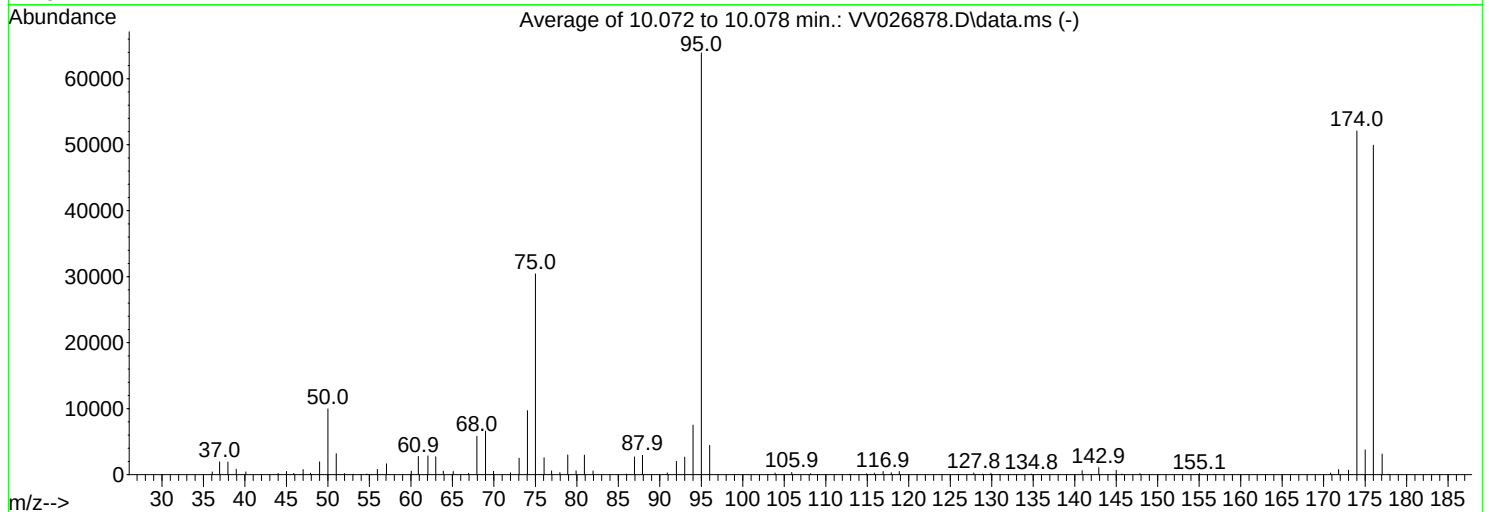


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072222\
Data File : VV026878.D
Acq On : 22 Jul 2022 09:56
Operator : SY/MD
Sample : BFB296
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB296

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Title : VOC Analysis
Last Update : Sat Jul 23 00:23:15 2022

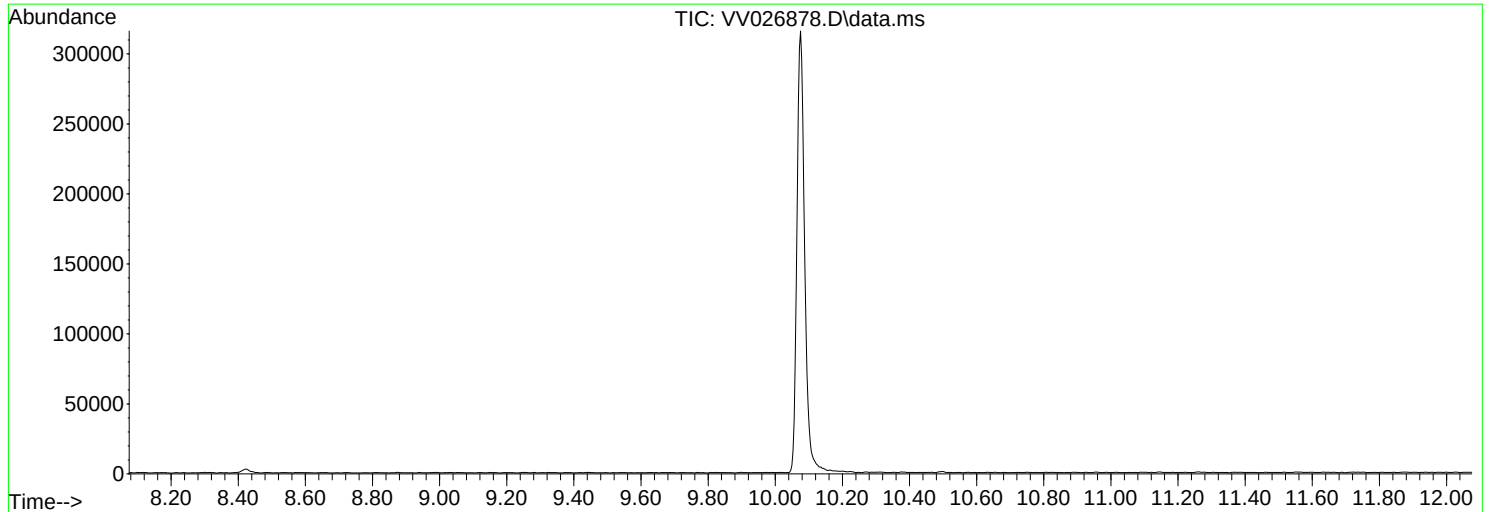

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9959	PASS
75	95	30	80	47.6	30429	PASS
95	95	100	100	100.0	63925	PASS
96	95	5	9	6.9	4430	PASS
173	174	0.00	2	1.3	690	PASS
174	95	50	120	81.5	52080	PASS
175	174	5	9	7.2	3768	PASS
176	174	95	105	95.9	49939	PASS
177	176	5	10	6.3	3135	PASS

m/z	Abundance
39.80	452.0
44.00	573.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.10	423.0
36.90	2014.0
37.90	1971.0
39.00	766.0
40.10	440.0
44.00	736.0
45.00	542.0
45.90	209.0
47.00	786.0
49.00	1999.0
50.00	10182.0
51.00	3169.0
52.00	218.0
53.10	134.0
54.70	107.0
55.20	102.0
56.00	793.0
57.00	1589.0
60.10	561.0
60.90	2514.0
62.10	2685.0
63.00	2863.0
63.90	591.0
65.10	488.0
66.90	153.0
68.00	5717.0
69.00	6772.0
70.00	446.0
72.00	266.0
73.10	2517.0
74.00	9700.0
75.00	30648.0
76.00	2437.0
76.90	606.0
77.90	335.0
78.90	3025.0
79.90	619.0
80.90	2956.0
82.00	482.0
86.90	2912.0
87.90	2720.0
90.90	257.0
92.00	2010.0
93.00	2626.0
94.00	7588.0
95.00	64664.0
96.00	4347.0
103.90	207.0
105.90	299.0
108.20	118.0
114.90	139.0
115.90	225.0
117.00	478.0
117.90	234.0
118.90	482.0
127.90	242.0
128.90	171.0
129.90	183.0
140.90	598.0
142.00	112.0
142.90	942.0
145.00	635.0
145.70	158.0
147.90	154.0
155.10	166.0
156.80	116.0
170.80	227.0
171.80	719.0
173.00	636.0
174.00	51272.0
175.00	3762.0
176.00	49072.0
177.00	3100.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	421.0
37.00	1999.0
37.90	1994.0
39.00	842.0
40.20	438.0
44.00	714.0
45.00	494.0
45.90	218.0
47.00	824.0
47.90	355.0
49.00	1968.0
50.00	10307.0
51.00	3296.0
52.00	165.0
53.10	109.0
54.70	119.0
55.90	830.0
57.00	1754.0
60.10	548.0
60.90	2904.0
62.00	2929.0
63.00	2807.0
63.90	537.0
65.10	496.0
67.00	207.0
67.90	6010.0
69.00	6967.0
69.90	521.0
72.00	298.0
73.00	2588.0
74.00	9862.0
75.00	31496.0
76.00	2711.0
77.00	573.0
77.90	332.0
78.90	3077.0
79.90	604.0
80.90	3089.0
81.90	584.0
86.00	135.0
86.90	2759.0
87.90	3065.0
90.90	261.0
92.00	2097.0
93.00	2749.0
94.00	7790.0
95.00	66008.0
96.00	4661.0
103.90	236.0
105.90	361.0
108.20	139.0
112.80	110.0
114.90	141.0
115.80	245.0
116.90	464.0
117.90	317.0
118.90	481.0
127.90	283.0
128.90	129.0
129.90	226.0
134.80	136.0
140.90	623.0
142.90	1106.0
145.00	705.0
145.70	117.0
147.80	195.0
155.00	175.0
156.80	107.0
170.80	265.0
171.80	848.0
173.00	739.0
174.00	54016.0
175.00	3903.0
176.00	51512.0
177.00	3165.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	402.0
37.00	1827.0
38.00	1782.0
38.90	839.0
40.00	380.0
44.00	774.0
45.00	426.0
45.90	180.0
47.00	727.0
47.90	331.0
49.00	1834.0
50.00	9388.0
51.00	3053.0
52.00	167.0
54.70	104.0
55.90	790.0
57.10	1617.0
60.00	525.0
60.90	2875.0
62.00	2891.0
63.00	2521.0
63.90	472.0
65.10	451.0
67.00	250.0
67.90	5710.0
69.00	6033.0
69.90	538.0
72.00	315.0
73.00	2388.0
74.10	9584.0
75.00	29144.0
76.10	2598.0
77.00	520.0
78.00	253.0
78.90	2869.0
79.90	537.0
80.90	2859.0
81.90	607.0
86.00	157.0
87.00	2387.0
87.90	3044.0
90.90	251.0
92.00	1929.0
93.00	2622.0
94.00	7161.0
95.00	61104.0
96.00	4281.0
103.90	252.0
105.90	361.0
108.10	151.0
112.90	129.0
114.90	135.0
115.80	248.0
116.80	508.0
117.90	307.0
118.80	486.0
127.80	271.0
129.90	283.0
130.90	129.0
134.80	151.0
136.80	117.0
140.90	605.0
142.90	1189.0
145.00	648.0
147.80	195.0
155.00	152.0
170.90	238.0
171.80	779.0
173.00	694.0
174.00	50952.0
175.00	3638.0
176.00	49232.0
177.10	3141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296