


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072318\
Data File : VV006694.D
Acq On : 23 Jul 2018 09:20
Operator : SY/MD
Sample : BFB70
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB70

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 01 01:43:21 2018

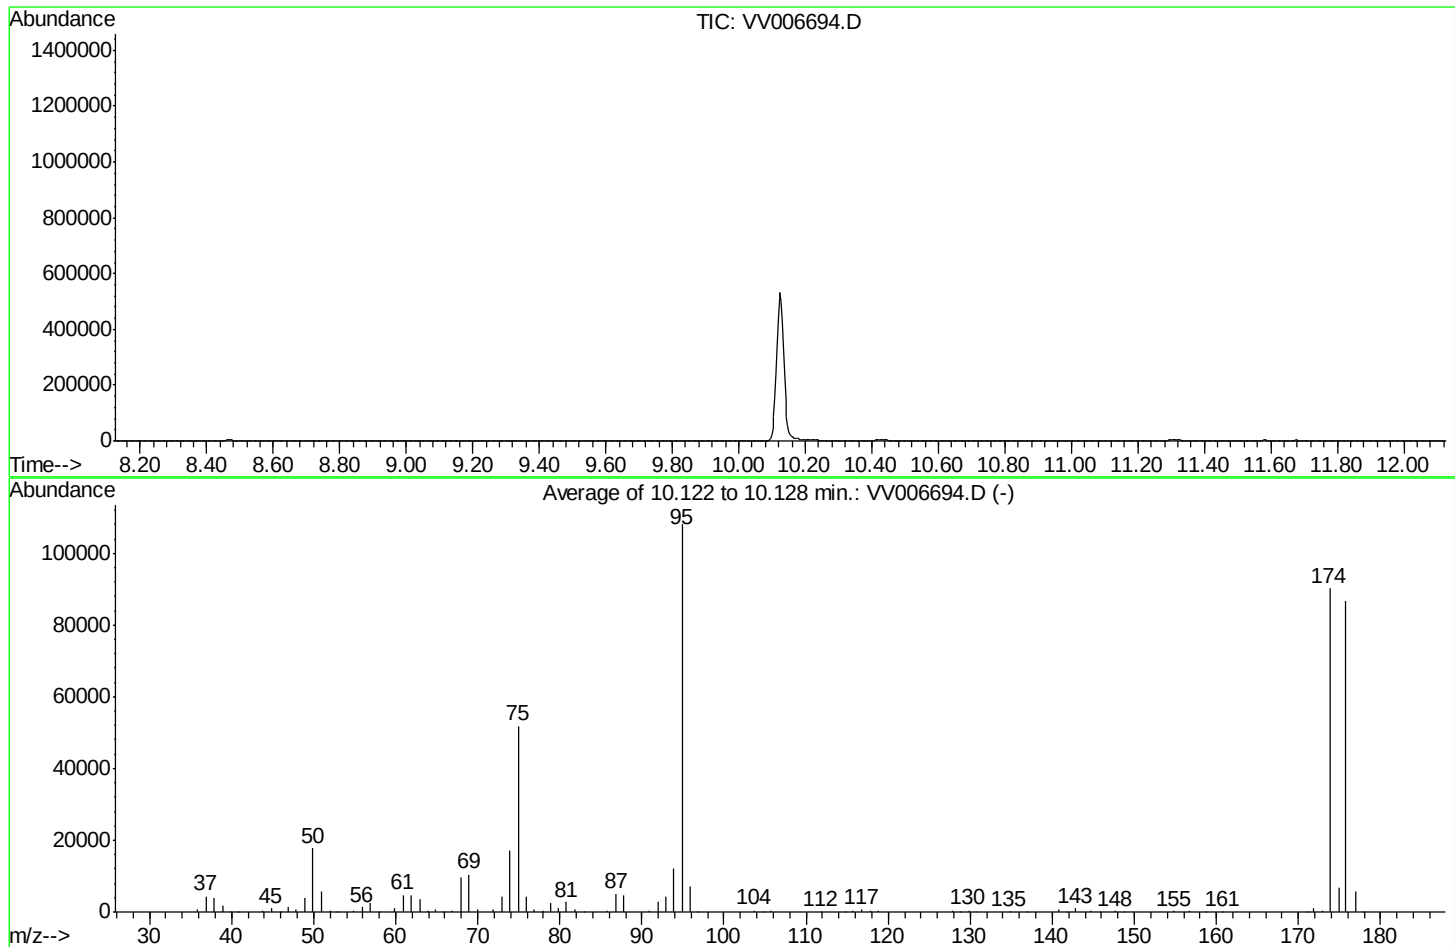

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	17765	PASS
75	95	30	80	47.9	51800	PASS
95	95	100	100	100.0	108045	PASS
96	95	5	9	6.8	7314	PASS
173	174	0.00	2	0.3	244	PASS
174	95	50	120	83.4	90144	PASS
175	174	5	9	7.4	6630	PASS
176	174	95	101	96.3	86837	PASS
177	176	5	9	6.5	5686	PASS

m/z	Abundance
35.80	585.0
37.80	202.0
39.80	196.0
43.80	555.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.90	1346.0
36.90	4260.0
37.90	4315.0
38.90	1830.0
39.90	203.0
43.90	1068.0
44.80	872.0
45.90	104.0
46.80	1530.0
47.80	554.0
48.90	3956.0
49.90	18136.0
50.90	5706.0
52.00	246.0
52.80	120.0
54.90	313.0
55.90	1341.0
56.90	2501.0
57.90	104.0
59.80	949.0
60.90	4751.0
61.90	4789.0
62.90	3557.0
63.90	541.0
64.90	795.0
65.80	114.0
66.80	276.0
67.90	10051.0
68.90	10465.0
70.00	855.0
71.90	506.0
72.90	4482.0
73.90	17296.0
74.90	52512.0
76.00	4474.0
76.90	692.0
78.00	511.0
78.80	2470.0
79.80	985.0
80.80	2653.0
81.80	705.0
83.00	104.0
85.80	223.0
86.90	5042.0
87.80	4769.0
90.90	347.0
91.90	2931.0
92.90	4318.0
93.90	12198.0
94.90	107800.0
96.00	7384.0
96.80	168.0
103.80	462.0
104.80	199.0
105.70	350.0
111.80	113.0
114.70	127.0
115.70	316.0
116.80	696.0
117.80	336.0
118.70	560.0
127.80	383.0
128.70	181.0
129.80	369.0
130.70	102.0
134.90	170.0
136.90	128.0
140.80	892.0
141.70	146.0
142.80	970.0
144.70	229.0
145.80	162.0
147.70	233.0
154.80	243.0
156.80	218.0
158.80	108.0
160.80	107.0
171.80	970.0
172.90	733.0
173.80	88096.0
174.90	6471.0
175.80	83968.0
176.90	5501.0
177.90	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.90	1290.0
36.90	4547.0
37.90	4382.0
38.90	1871.0
39.90	215.0
40.70	104.0
43.90	1091.0
44.80	951.0
45.90	126.0
46.90	1518.0
47.80	596.0
48.90	3913.0
49.90	18248.0
50.90	5867.0
52.00	219.0
52.80	129.0
54.90	342.0
55.90	1352.0
56.90	2587.0
57.90	106.0
59.80	960.0
60.90	4909.0
61.90	4843.0
62.90	3646.0
63.90	517.0
64.90	851.0
65.80	119.0
66.80	247.0
67.90	10111.0
68.90	10823.0
70.00	836.0
71.90	603.0
72.90	4577.0
73.90	17840.0
74.90	53576.0
75.90	4317.0
76.90	666.0
78.00	558.0
78.80	2585.0
79.90	1015.0
80.80	2849.0
81.80	643.0
85.70	238.0
86.90	5210.0
87.80	4903.0
90.80	344.0
91.90	3063.0
92.90	4560.0
93.90	12607.0
94.90	111720.0
95.90	7574.0
96.80	191.0
103.70	480.0
104.80	199.0
105.70	380.0
114.70	116.0
115.80	343.0
116.80	716.0
117.80	383.0
118.80	563.0
127.80	373.0
128.80	156.0
129.80	422.0
130.60	123.0
134.80	194.0
136.90	134.0
140.80	904.0
141.70	157.0
142.80	1028.0
144.80	234.0
145.80	175.0
147.70	265.0
154.80	237.0
156.80	243.0
158.80	122.0
160.80	120.0
171.00	119.0
171.80	1064.0
173.80	93176.0
174.90	6836.0
175.80	90096.0
176.90	5894.0
177.90	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.90	1163.0
36.90	4243.0
37.90	3954.0
38.90	1685.0
39.90	235.0
40.80	107.0
43.90	1022.0
44.80	905.0
45.90	131.0
46.90	1326.0
47.80	569.0
48.90	3511.0
49.90	16912.0
50.90	5431.0
52.00	174.0
52.80	123.0
54.90	302.0
55.90	1258.0
56.90	2467.0
57.90	104.0
59.80	853.0
60.90	4507.0
61.90	4423.0
62.90	3364.0
63.90	433.0
64.90	848.0
66.80	206.0
67.90	9162.0
68.90	10018.0
69.90	701.0
71.90	621.0
72.90	4238.0
73.90	16512.0
74.90	49312.0
75.90	3861.0
76.90	631.0
78.00	526.0
78.90	2515.0
79.90	922.0
80.80	2678.0
81.80	550.0
85.70	219.0
86.90	4906.0
87.80	4453.0
90.80	312.0
91.90	2876.0
92.90	4354.0
93.90	11795.0
94.90	104616.0
95.90	6984.0
96.90	187.0
103.70	419.0
104.80	171.0
105.70	357.0
115.80	341.0
116.80	635.0
117.80	386.0
118.80	519.0
127.80	323.0
128.80	145.0
129.80	393.0
130.70	121.0
134.90	191.0
136.90	133.0
140.80	837.0
141.70	140.0
142.90	978.0
144.80	199.0
145.90	159.0
147.70	246.0
148.70	108.0
154.90	236.0
156.70	244.0
158.80	109.0
160.80	107.0
171.00	118.0
171.80	1084.0
173.80	89160.0
174.90	6585.0
175.80	86448.0
176.90	5663.0
177.90	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70