

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072319\
 Data File : VV011974.D
 Acq On : 23 Jul 2019 19:34
 Operator : SY/MD
 Sample : K3823-18
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A52J6

Quant Time: Jul 24 07:28:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 24 05:52:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	136587	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	131716	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	64430	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35780	5.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.80%
7) Chloroethane-d5	1.59	69	28603	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	2.13	63	57340	4.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.20%
20) 2-Butanone-d5	3.94	46	114067	54.97	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.94%
24) Chloroform-d	4.40	84	91989	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.08	65	52770	5.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.00%
32) Benzene-d6	5.10	84	185131	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.12	67	54020	5.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.80%
41) Toluene-d8	7.36	98	168391	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
43) trans-1,3-Dichloropropene-	7.67	79	20526	4.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.20%
46) 2-Hexanone-d5	8.13	63	93456	54.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.10%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	39208	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	68938	5.56	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	5364	4.795 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072319\
Data File : VV011974.D
Acq On : 23 Jul 2019 19:34
Operator : SY/MD
Sample : K3823-18
Misc : 25ML/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52J6

Quant Time: Jul 24 07:28:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 24 05:52:52 2019
Response via : Initial Calibration

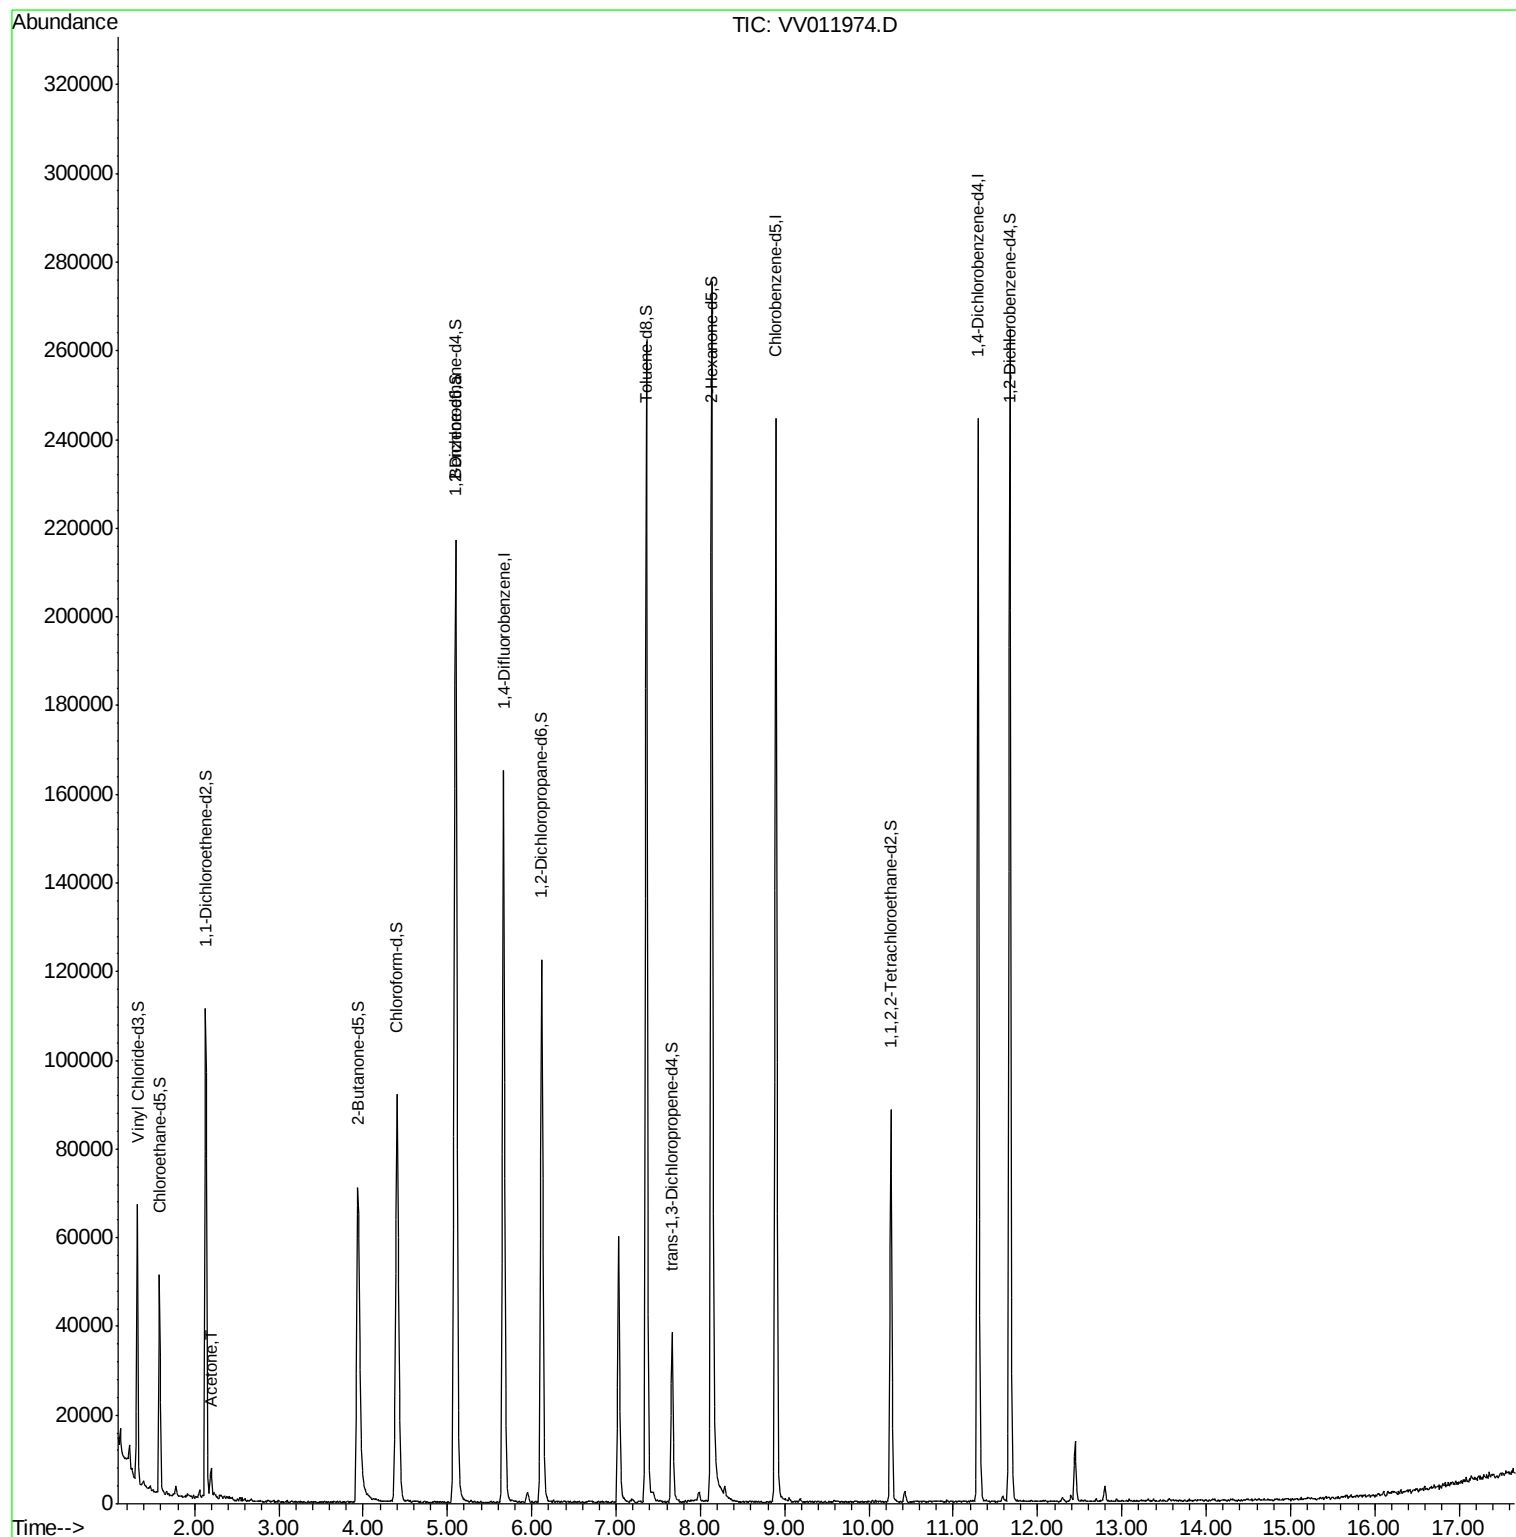

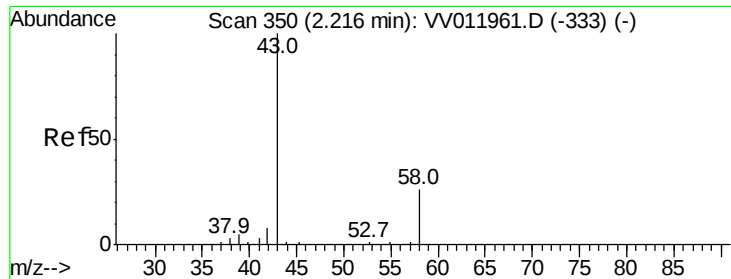

#13

Acetone

Concen: 4.795 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.02 min

Lab File: VV011974.D

Acq: 23 Jul 2019 19:34

Instrument :
MSVOA_V
ClientSampleId :
A52J6

Tot Ion: 43 Resp: 5364

Ion Ratio Lower Upper

43 100

58 28.5 0.0 51.8

