

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072319\
 Data File : VV011995.D
 Acq On : 24 Jul 2019 04:57
 Operator : SY/MD
 Sample : K3960-03
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB9A8

Quant Time: Jul 24 08:57:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 24 07:47:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	152124	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	148041	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	74089	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35765	4.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.40%
7) Chloroethane-d5	1.59	69	29163	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.14	63	56990	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	3.93	46	109579	47.41	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.82%
24) Chloroform-d	4.40	84	92677	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.08	65	51530	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.10	84	190678	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
36) 1,2-Dichloropropane-d6	6.12	67	53555	4.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.60%
41) Toluene-d8	7.36	98	173949	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
43) trans-1,3-Dichloropropene-	7.66	79	19992	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
46) 2-Hexanone-d5	8.13	63	86660	45.01	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.02%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37661	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	71647	5.02	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.40%

Target Compounds


					Ovalue
3) Chloromethane	1.25	50	3173	0.348	ug/L 99
13) Acetone	2.19	43	2079	1.669	ug/L 85
42) Toluene	7.43	91	148719	3.182	ug/L 98
51) Chlorobenzene	8.93	112	3807	0.124	ug/L 99
52) Ethylbenzene	9.05	91	42315	0.793	ug/L 99
53) m,p-xylene	9.18	106	73440	3.616	ug/L 99
54) o-xylene	9.59	106	27105	1.408	ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072319\
Data File : VV011995.D
Acq On : 24 Jul 2019 04:57
Operator : SY/MD
Sample : K3960-03
Misc : 25ML/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB9A8

Quant Time: Jul 24 08:57:16 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 24 07:47:25 2019
Response via : Initial Calibration

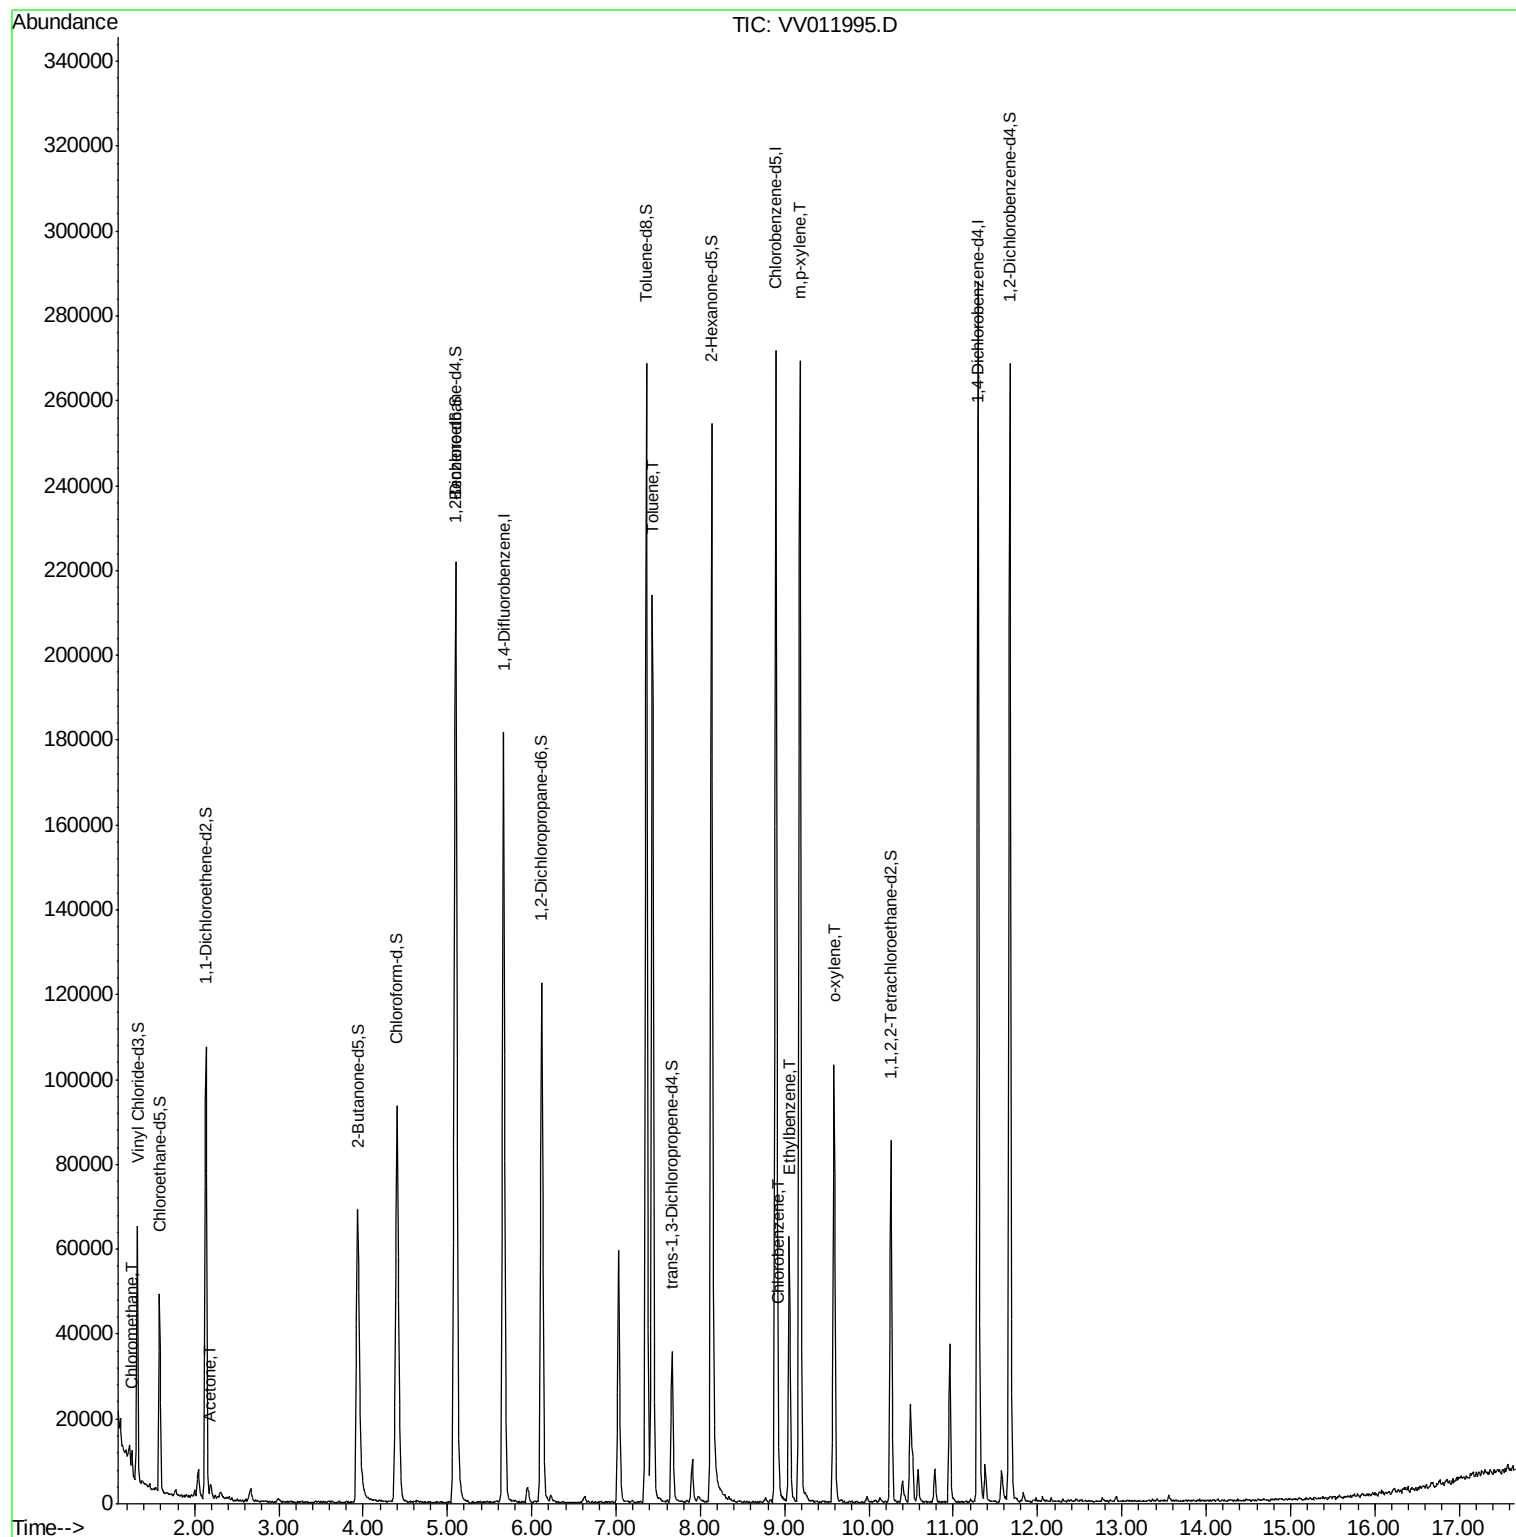

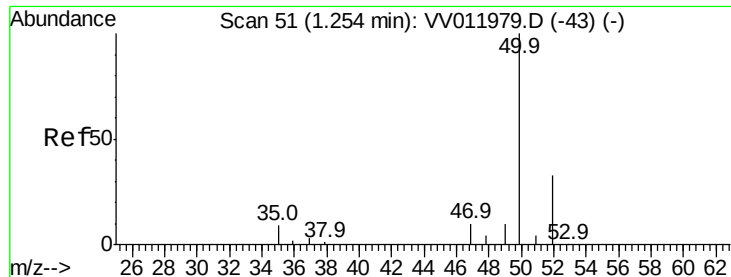

#3

Chloromethane

Concen: 0.348 ug/L

RT: 1.25 min Scan# 51

Delta R.T. -0.00 min

Lab File: VV011995.D

Acq: 24 Jul 2019 04:57

Instrument :

MSVOA_V

ClientSampleId :


DB9A8

Tot Ion: 50 Resp: 3173

Ion Ratio Lower Upper




50 100

52 31.4 21.6 40.2

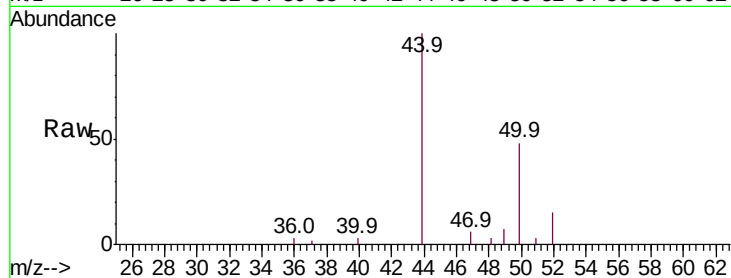

Abundance Ion 50.05 (49.75 to 50.75): VV0

Ion 52.05 (51.75 to 52.75): VV0

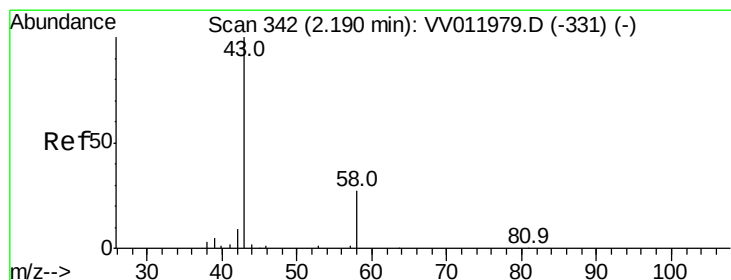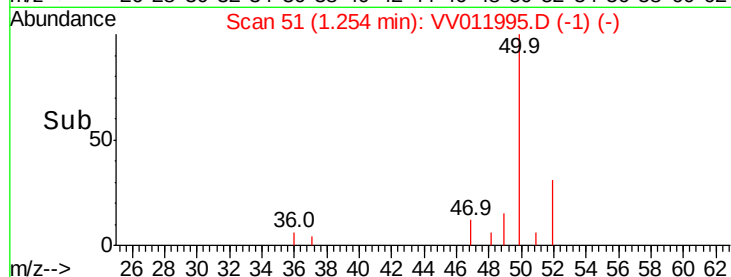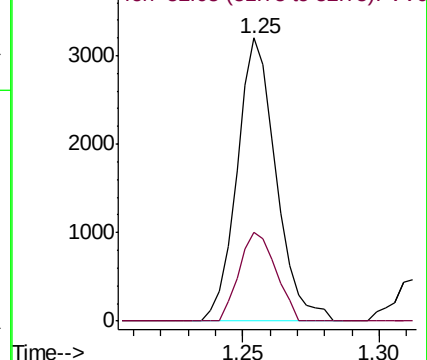

#13

Acetone

Concen: 1.669 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.00 min

Lab File: VV011995.D


Acq: 24 Jul 2019 04:57

Tgt Ion: 43 Resp: 2079

Ion Ratio Lower Upper



43 100


58 18.2 0.0 51.8

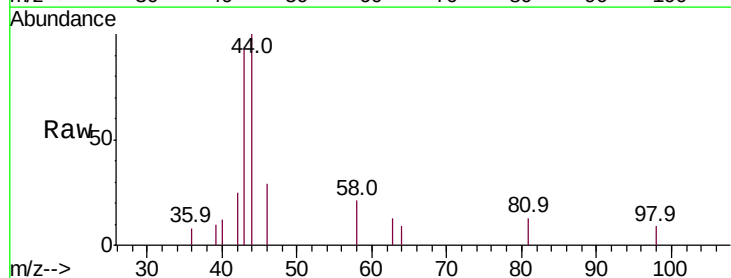

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

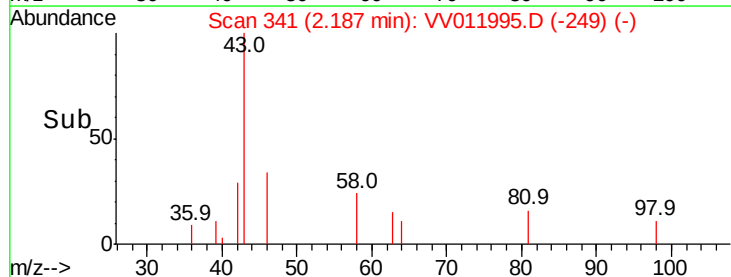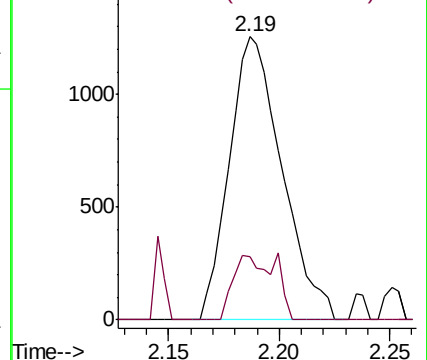

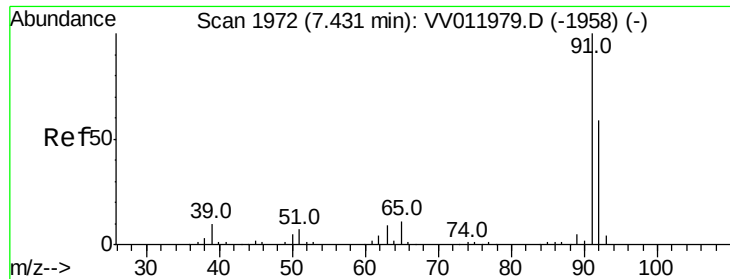

#42

Toluene

Concen: 3.182 ug/L

RT: 7.43 min Scan# 1972

Delta R.T. -0.00 min

Lab File: VV011995.D

Acq: 24 Jul 2019 04:57

Instrument :

MSVOA_V

ClientSampleId :


DB9A8

Tot Ion: 91 Resp: 148719

Ion Ratio Lower Upper




91 100

92 58.6 41.9 77.9

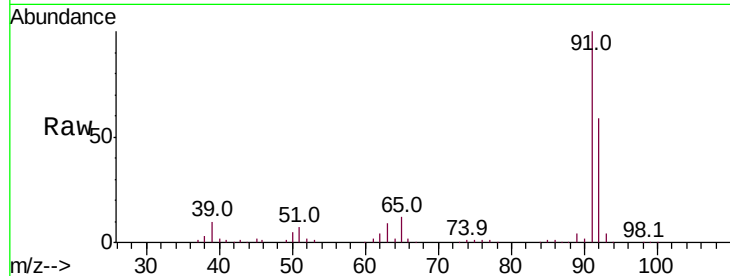

Abundance Ion 91.15 (90.85 to 91.85): VV011979.D (-1958) (-)

Ion 92.15 (91.85 to 92.85): VV011979.D (-1958) (-)

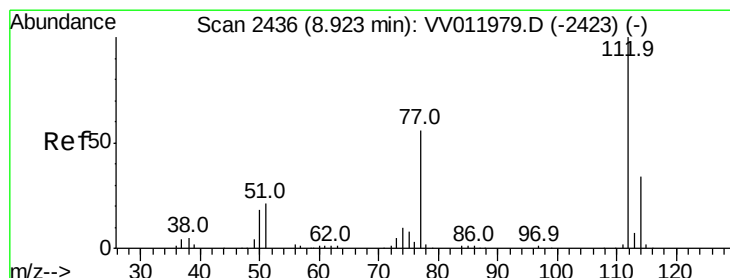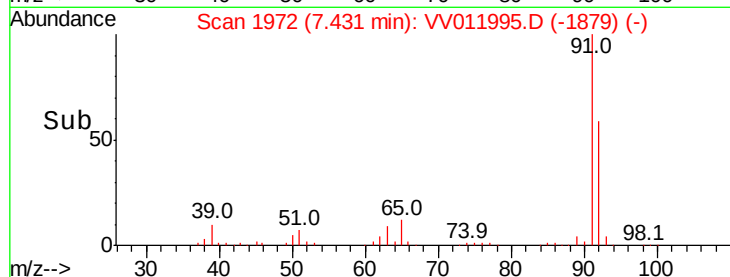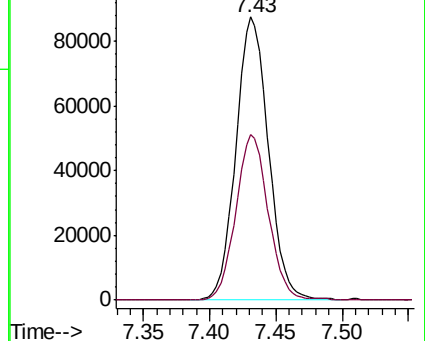

#51

Chlorobenzene

Concen: 0.124 ug/L

RT: 8.93 min Scan# 2438

Delta R.T. 0.01 min

Lab File: VV011995.D

Acq: 24 Jul 2019 04:57


Tgt Ion: 112 Resp: 3807

Ion Ratio Lower Upper

112 100

114 32.8 23.0 42.8



77 58.9 46.4 69.6

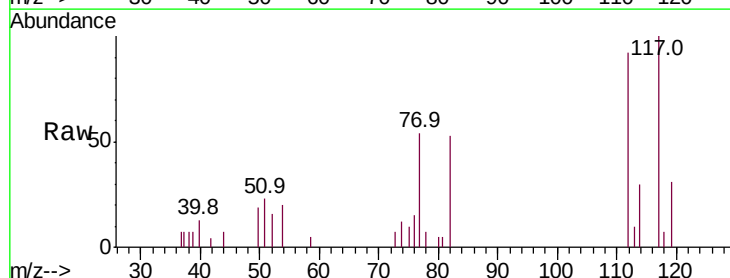


Abundance Ion 112.10 (111.80 to 112.80): VV011979.D (-2423) (-)

Ion 114.05 (113.75 to 114.75): VV011979.D (-2423) (-)

Ion 77.10 (76.80 to 77.80): VV011979.D (-2423) (-)

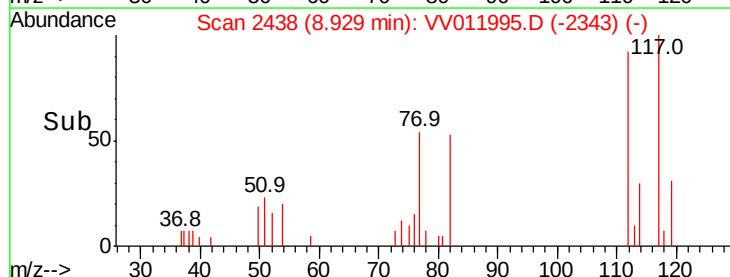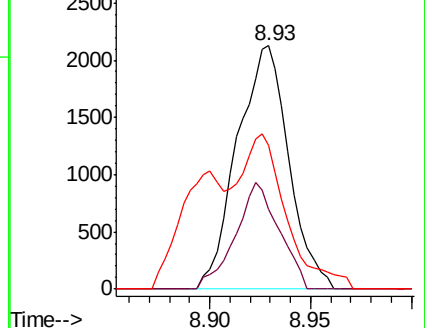

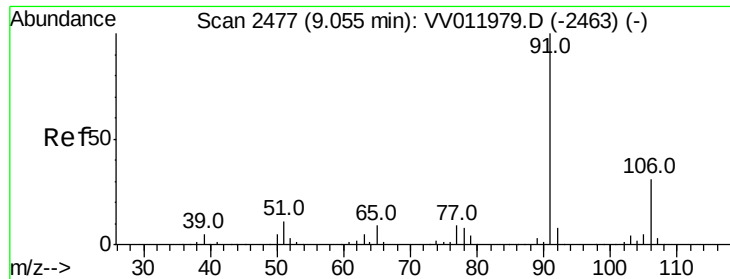

#52

Ethylbenzene

Concen: 0.793 ug/L

RT: 9.05 min Scan# 2477

Delta R.T. -0.00 min

Lab File: VV011995.D

Acq: 24 Jul 2019 04:57

Instrument :

MSVOA_V

ClientSampleId :


DB9A8

Tot Ion: 91 Resp: 42315




Ion Ratio Lower Upper

91 100

106 31.1 21.6 40.0

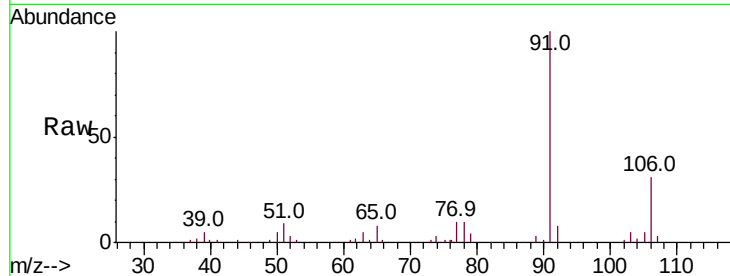

Abundance Ion 91.15 (90.85 to 91.85): VV011995.D (-2463) (-)

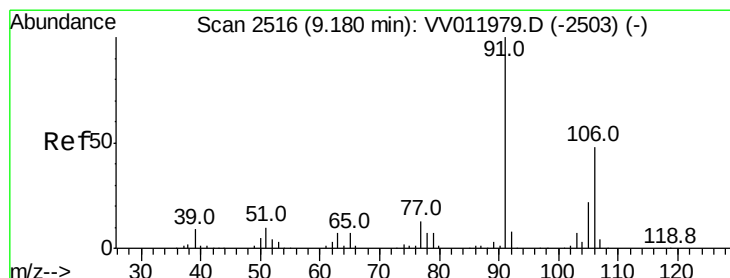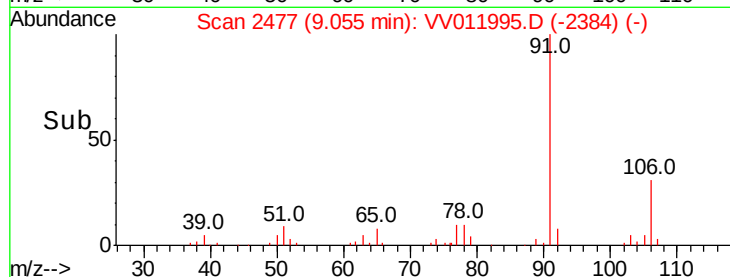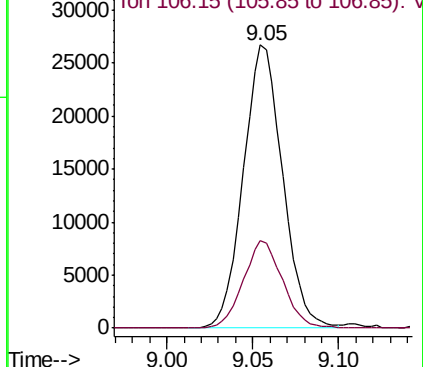

#53

m,p-xylene

Concen: 3.616 ug/L

RT: 9.18 min Scan# 2516

Delta R.T. -0.00 min

Lab File: VV011995.D


Acq: 24 Jul 2019 04:57

Tgt Ion: 106 Resp: 73440



Ion Ratio Lower Upper


106 100

91 204.7 142.7 265.1

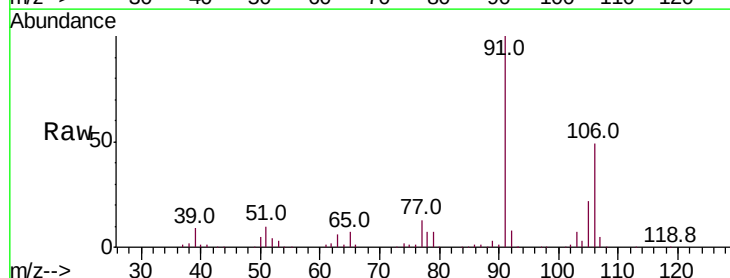

Abundance Ion 106.15 (105.85 to 106.85): VV011995.D (-2503) (-)

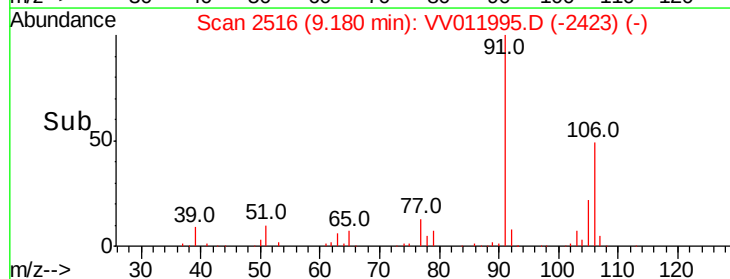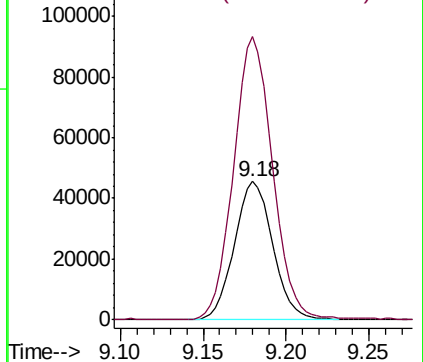

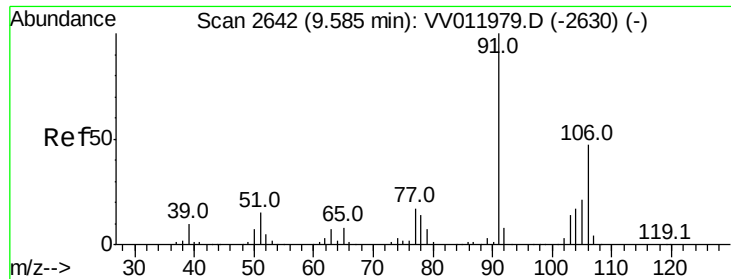

#54
o-xylene
Concen: 1.408 ug/L
RT: 9.59 min Scan# 2643
Delta R.T. 0.00 min
Lab File: VV011995.D
Acq: 24 Jul 2019 04:57

Instrument :
MSVOA_V
ClientSampleId :
DB9A8

Tot Ion:106 Resp: 27105
Ion Ratio Lower Upper
106 100
91 213.7 151.0 280.4

