

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072319\
 Data File : VV011976.D
 Acq On : 23 Jul 2019 20:25
 Operator : SY/MD
 Sample : K3823-21
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A52K2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	89	rVB2	116467	127135	2.01%	0.977%
2	2.142	313	327	338	rBV3	248697	417067	6.59%	3.205%
3	3.232	647	666	691	rBV	557456	1160276	18.32%	8.917%
4	3.961	873	893	915	rBV2	274068	782498	12.35%	6.014%
5	4.402	1013	1030	1060	rBV2	89863	236869	3.74%	1.820%
6	4.659	1087	1110	1149	rBV	2579004	6333530	100.00%	48.677%
7	5.096	1227	1246	1269	rBV2	226035	540506	8.53%	4.154%
8	5.666	1407	1423	1444	rBV	161714	318656	5.03%	2.449%
9	5.961	1502	1515	1531	rBV2	86379	168880	2.67%	1.298%
10	6.119	1548	1564	1591	rBV	124550	253130	4.00%	1.945%
11	7.029	1836	1847	1870	rBV	62952	112456	1.78%	0.864%
12	7.360	1936	1950	1965	rBV	271208	463849	7.32%	3.565%
13	7.666	2034	2045	2061	rBV	38231	65724	1.04%	0.505%
14	8.019	2144	2155	2171	rVB2	75193	128701	2.03%	0.989%
15	8.132	2177	2190	2232	rBV	255007	470612	7.43%	3.617%
16	8.894	2416	2427	2447	rBV	238754	390922	6.17%	3.004%
17	10.260	2840	2852	2863	rBV	86762	134613	2.13%	1.035%
18	11.292	3159	3173	3195	rBV	239873	391119	6.18%	3.006%
19	11.582	3252	3263	3276	rBV3	42198	67755	1.07%	0.521%
20	11.672	3278	3291	3310	rBV	271352	447070	7.06%	3.436%




Sum of corrected areas: 13011368

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072319\
Data File : VV011976.D
Acq On : 23 Jul 2019 20:25
Operator : SY/MD
Sample : K3823-21
Misc : 25ML/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52K2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

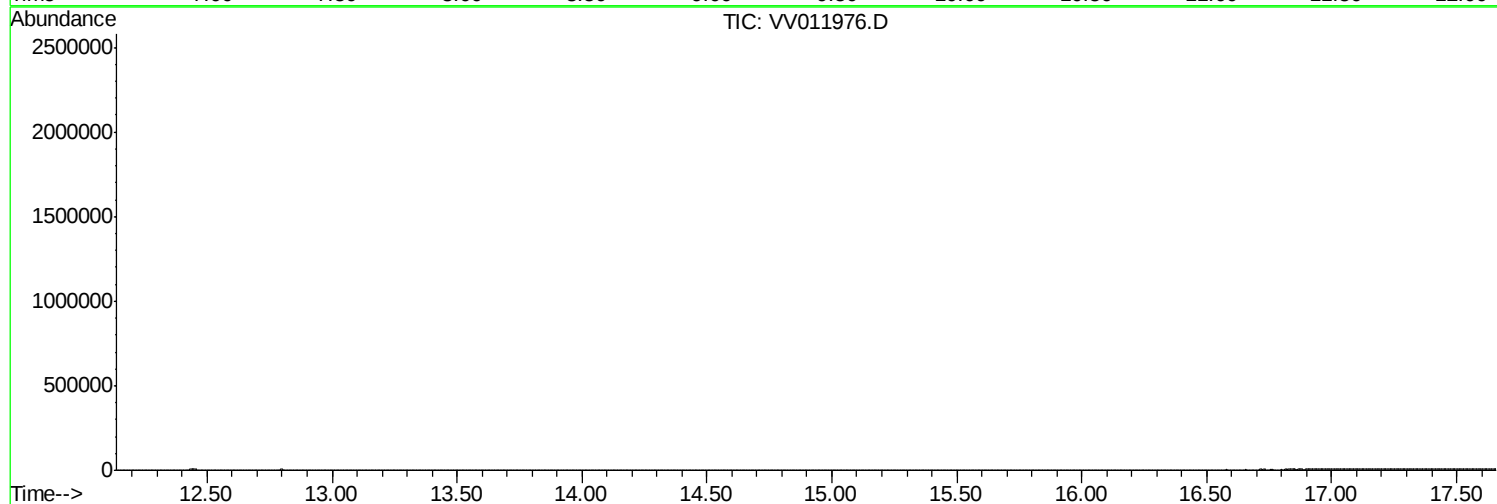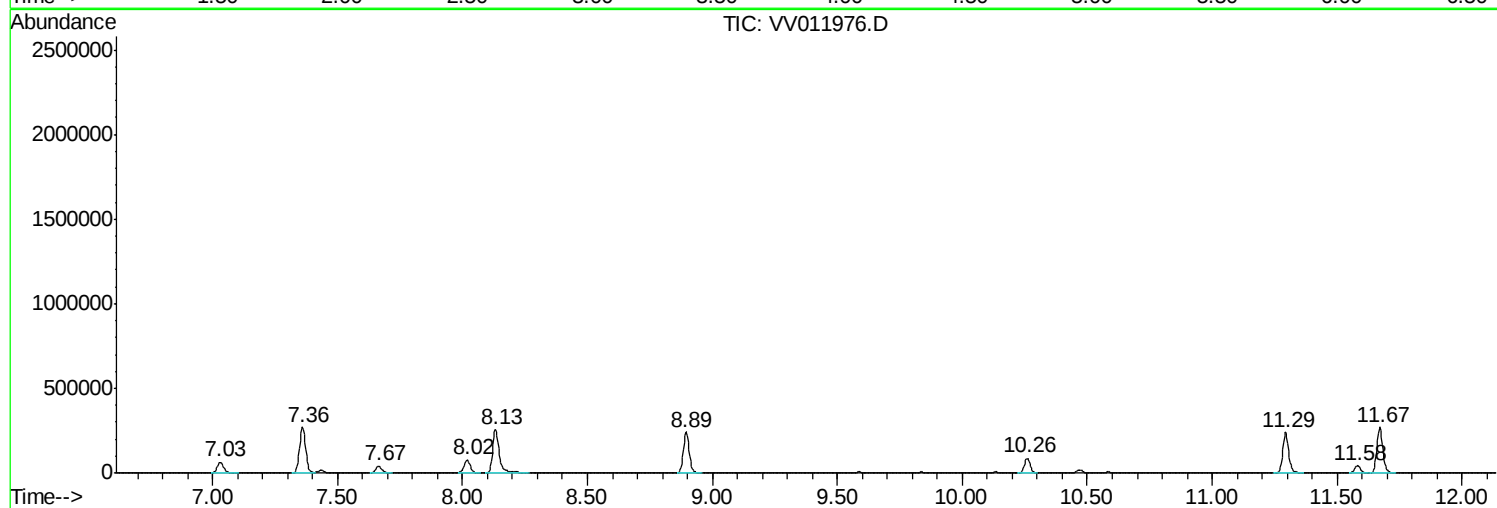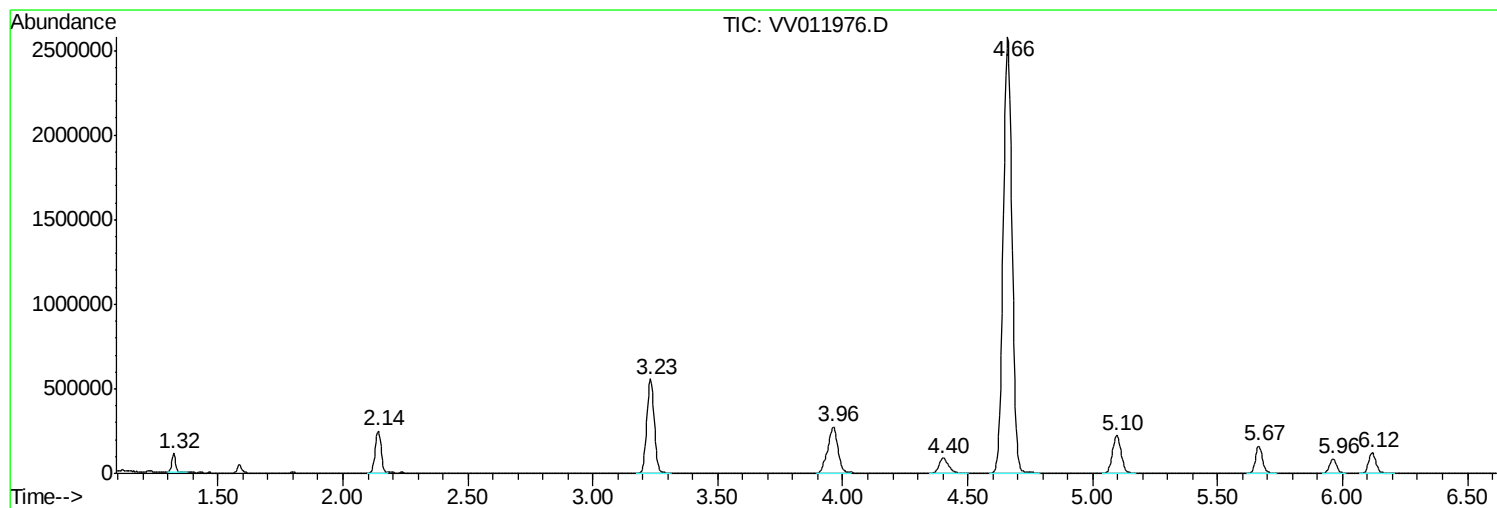

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072319\
Data File : VV011976.D
Acq On : 23 Jul 2019 20:25
Operator : SY/MD
Sample : K3823-21
Misc : 25ML/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52K2










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.58	0.87 ug/L	67755	1,4-Dichlorobenzene-d4	11.30

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopropane, 1,1-dichloro-2-chl...	172	C5H7Cl3	015997-19-0	32
2		4-Pyridinecarboxaldehyde N-oxide	123	C6H5NO2	007216-42-4	27
3		Methyl 3,3-dichloropropenoate	154	C4H4Cl2O2	002257-46-7	25
4		2-Fluorophenylmethylcarbinol	140	C8H9FO	000445-26-1	16
5		Benzoyl chloride, 2-fluoro-	158	C7H4ClFO	000393-52-2	16

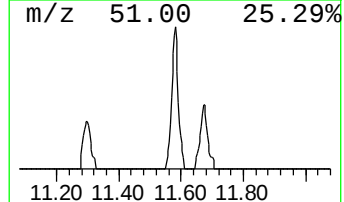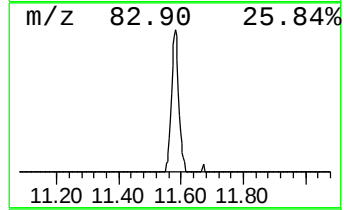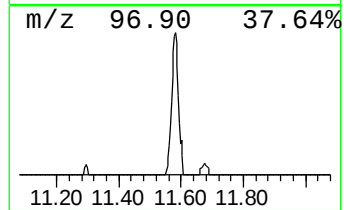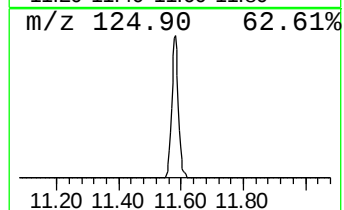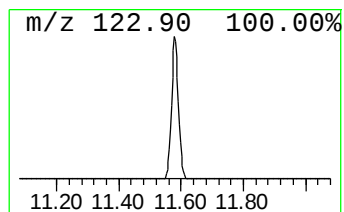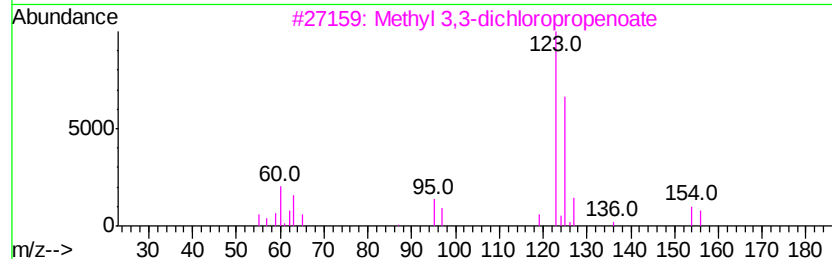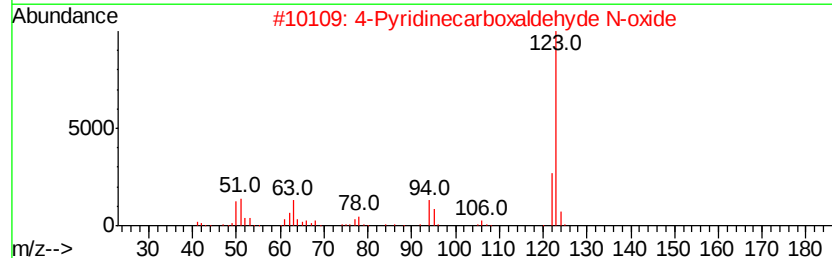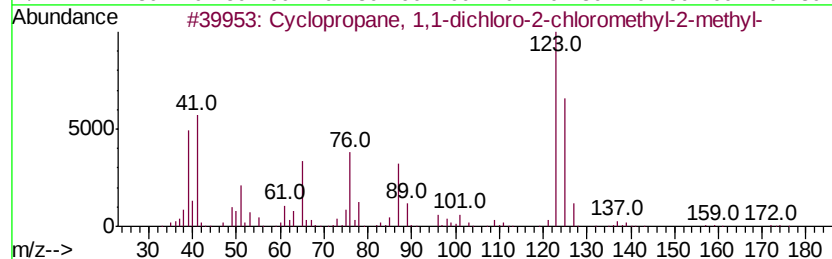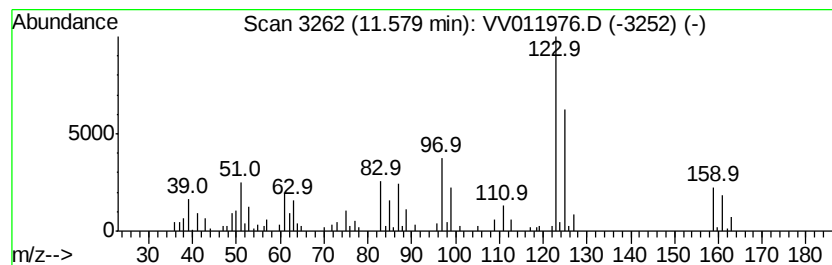

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV072319\
Data File : VV011976.D
Acq On : 23 Jul 2019 20:25
Operator : SY/MD
Sample : K3823-21
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52K2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	11.58	0.9	ug/L	67755	3	11.30	391119	5.0