


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072319\
 Data File : VV011960.D
 Acq On : 23 Jul 2019 11:56
 Operator : SY/MD
 Sample: BFB99
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 25 04:12:02 2019

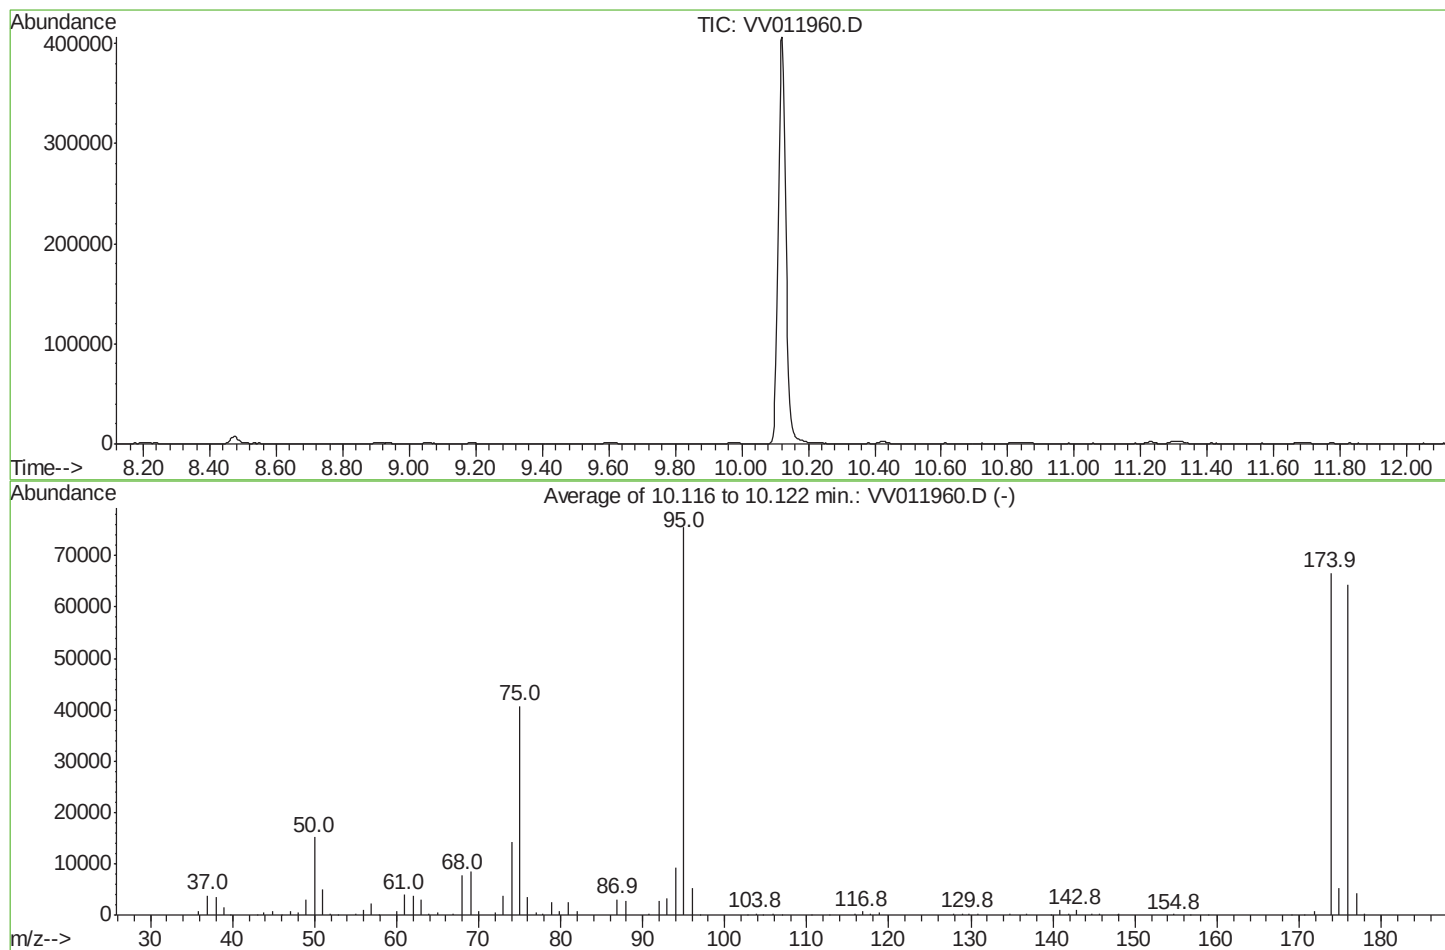

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	15169	PASS
75	95	30	80	54.0	40760	PASS
95	95	100	100	100.0	75533	PASS
96	95	5	9	6.9	5211	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.3	66680	PASS
175	174	5	9	8.0	5310	PASS
176	174	95	101	96.7	64450	PASS
177	176	5	9	6.5	4162	PASS

Scan 2795 (10.077 min): VV011960.D
BFB99

m/z	Abundance
39.80	212.0
43.80	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.90	736.0
37.00	3543.0
38.00	3472.0
38.90	1347.0
39.80	273.0
43.90	717.0
44.90	697.0
47.10	897.0
47.90	484.0
49.00	3005.0
50.00	14195.0
51.00	4493.0
51.90	210.0
52.90	144.0
54.90	168.0
56.00	1029.0
56.90	1826.0
57.90	111.0
60.00	628.0
61.00	3464.0
62.00	3698.0
63.00	2765.0
64.00	315.0
64.90	470.0
66.80	206.0
68.00	7605.0
69.00	7731.0
70.00	626.0
72.00	452.0
73.00	3560.0
74.00	13176.0
75.00	37664.0
76.00	3389.0
77.00	537.0
77.90	277.0
78.90	2379.0
79.80	682.0
80.80	2389.0
81.90	644.0
86.90	2940.0
87.90	2594.0
90.80	292.0
92.00	2588.0
93.00	3015.0
94.00	8802.0
95.00	70616.0
96.00	5052.0
96.90	108.0
103.80	303.0
104.70	100.0
105.90	268.0
112.80	120.0
115.80	361.0
116.80	602.0
117.70	343.0
118.80	466.0
127.90	284.0
129.00	124.0
129.80	271.0
130.90	121.0
134.80	218.0
136.80	134.0
140.80	859.0
141.80	143.0
142.80	926.0
144.80	161.0
145.70	123.0
147.80	168.0
154.70	204.0
170.70	118.0
171.90	629.0
173.90	60032.0
174.90	4804.0
175.90	58272.0
176.90	3808.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.90	865.0
37.00	3935.0
38.00	3676.0
38.90	1533.0
39.90	290.0
43.90	715.0
44.90	766.0
47.10	896.0
48.00	533.0
49.00	3268.0
50.00	15798.0
50.90	5048.0
51.90	224.0
52.90	145.0
54.90	194.0
55.90	1106.0
56.90	2160.0
57.90	120.0
59.90	651.0
60.90	4006.0
62.00	3976.0
63.00	2996.0
63.90	366.0
64.90	509.0
66.80	233.0
68.00	7952.0
69.00	8848.0
70.00	703.0
72.00	477.0
73.00	3783.0
74.00	14560.0
75.00	42216.0
76.00	3560.0
76.90	579.0
77.90	288.0
78.90	2608.0
79.80	779.0
80.90	2644.0
82.00	676.0
86.90	3225.0
88.00	3022.0
90.80	328.0
92.00	2835.0
93.00	3366.0
94.00	9545.0
95.00	77992.0
96.00	5483.0
97.00	133.0
103.80	330.0
105.90	332.0
106.90	110.0
110.50	109.0
112.80	132.0
115.80	397.0
116.80	700.0
117.70	362.0
118.80	545.0
127.90	289.0
129.00	157.0
129.70	319.0
130.90	159.0
134.80	253.0
136.90	157.0
140.90	926.0
141.80	153.0
142.80	1058.0
144.80	178.0
145.70	148.0
148.00	224.0
154.70	235.0
156.70	104.0
171.90	730.0
173.90	69024.0
174.90	5492.0
175.90	66592.0
177.00	4278.0
178.00	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.90	906.0
36.90	3860.0
38.00	3462.0
38.90	1522.0
39.90	295.0
43.00	105.0
43.90	673.0
44.90	843.0
46.00	124.0
47.00	801.0
47.90	547.0
49.00	3082.0
50.00	15516.0
50.90	5122.0
51.90	242.0
55.00	212.0
55.90	971.0
56.90	2411.0
59.90	666.0
60.90	4159.0
62.00	3771.0
63.00	3031.0
63.90	368.0
65.00	544.0
66.80	216.0
68.00	7724.0
69.00	8862.0
70.00	677.0
71.90	486.0
73.00	3672.0
74.00	14648.0
75.00	42400.0
76.00	3346.0
76.90	567.0
77.80	245.0
78.90	2525.0
79.80	836.0
80.90	2651.0
82.00	648.0
86.90	3071.0
88.00	2934.0
90.80	314.0
92.00	2769.0
92.90	3512.0
94.00	9506.0
95.00	77992.0
96.00	5100.0
97.00	163.0
102.70	107.0
103.80	347.0
106.00	336.0
107.00	103.0
110.50	115.0
112.80	121.0
115.80	366.0
116.80	685.0
117.80	328.0
118.80	586.0
127.80	287.0
128.90	165.0
129.70	329.0
130.90	190.0
134.80	240.0
136.90	165.0
139.70	130.0
140.90	939.0
141.90	159.0
142.80	1086.0
144.80	174.0
145.70	144.0
148.00	244.0
154.80	235.0
156.70	120.0
159.00	115.0
169.10	117.0
171.90	727.0
173.90	70984.0
174.90	5634.0
175.90	68488.0
177.00	4401.0
177.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99