

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072320\
 Data File : VV017619.D
 Acq On : 23 Jul 2020 22:15
 Operator : SY/MD
 Sample : L3398-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4C23

Quant Time: Jul 24 03:03:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 24 02:33:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	161201	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	161768	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	75083	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	41510	5.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.80%
7) Chloroethane-d5	1.58	69	33186	5.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.60%
11) 1,1-Dichloroethene-d2	2.12	63	66916	3.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.60%
20) 2-Butanone-d5	3.93	46	94227	51.17	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.34%
24) Chloroform-d	4.38	84	100014	5.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.40%
26) 1,2-Dichloroethane-d4	5.06	65	53228	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.80%
32) Benzene-d6	5.07	84	180295	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.09	67	49421	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.34	98	165177	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
45) trans-1,3-Dichloropropene-	7.65	79	20501	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
48) 2-Hexanone-d5	8.11	63	61331	44.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.10%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	34283	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	67829	5.97	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	21026	14.586 ug/L #	43
42) Toluene	7.41	91	8908	0.178 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072320\
Data File : VV017619.D
Acq On : 23 Jul 2020 22:15
Operator : SY/MD
Sample : L3398-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4C23

Quant Time: Jul 24 03:03:03 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 24 02:33:05 2020
Response via : Initial Calibration

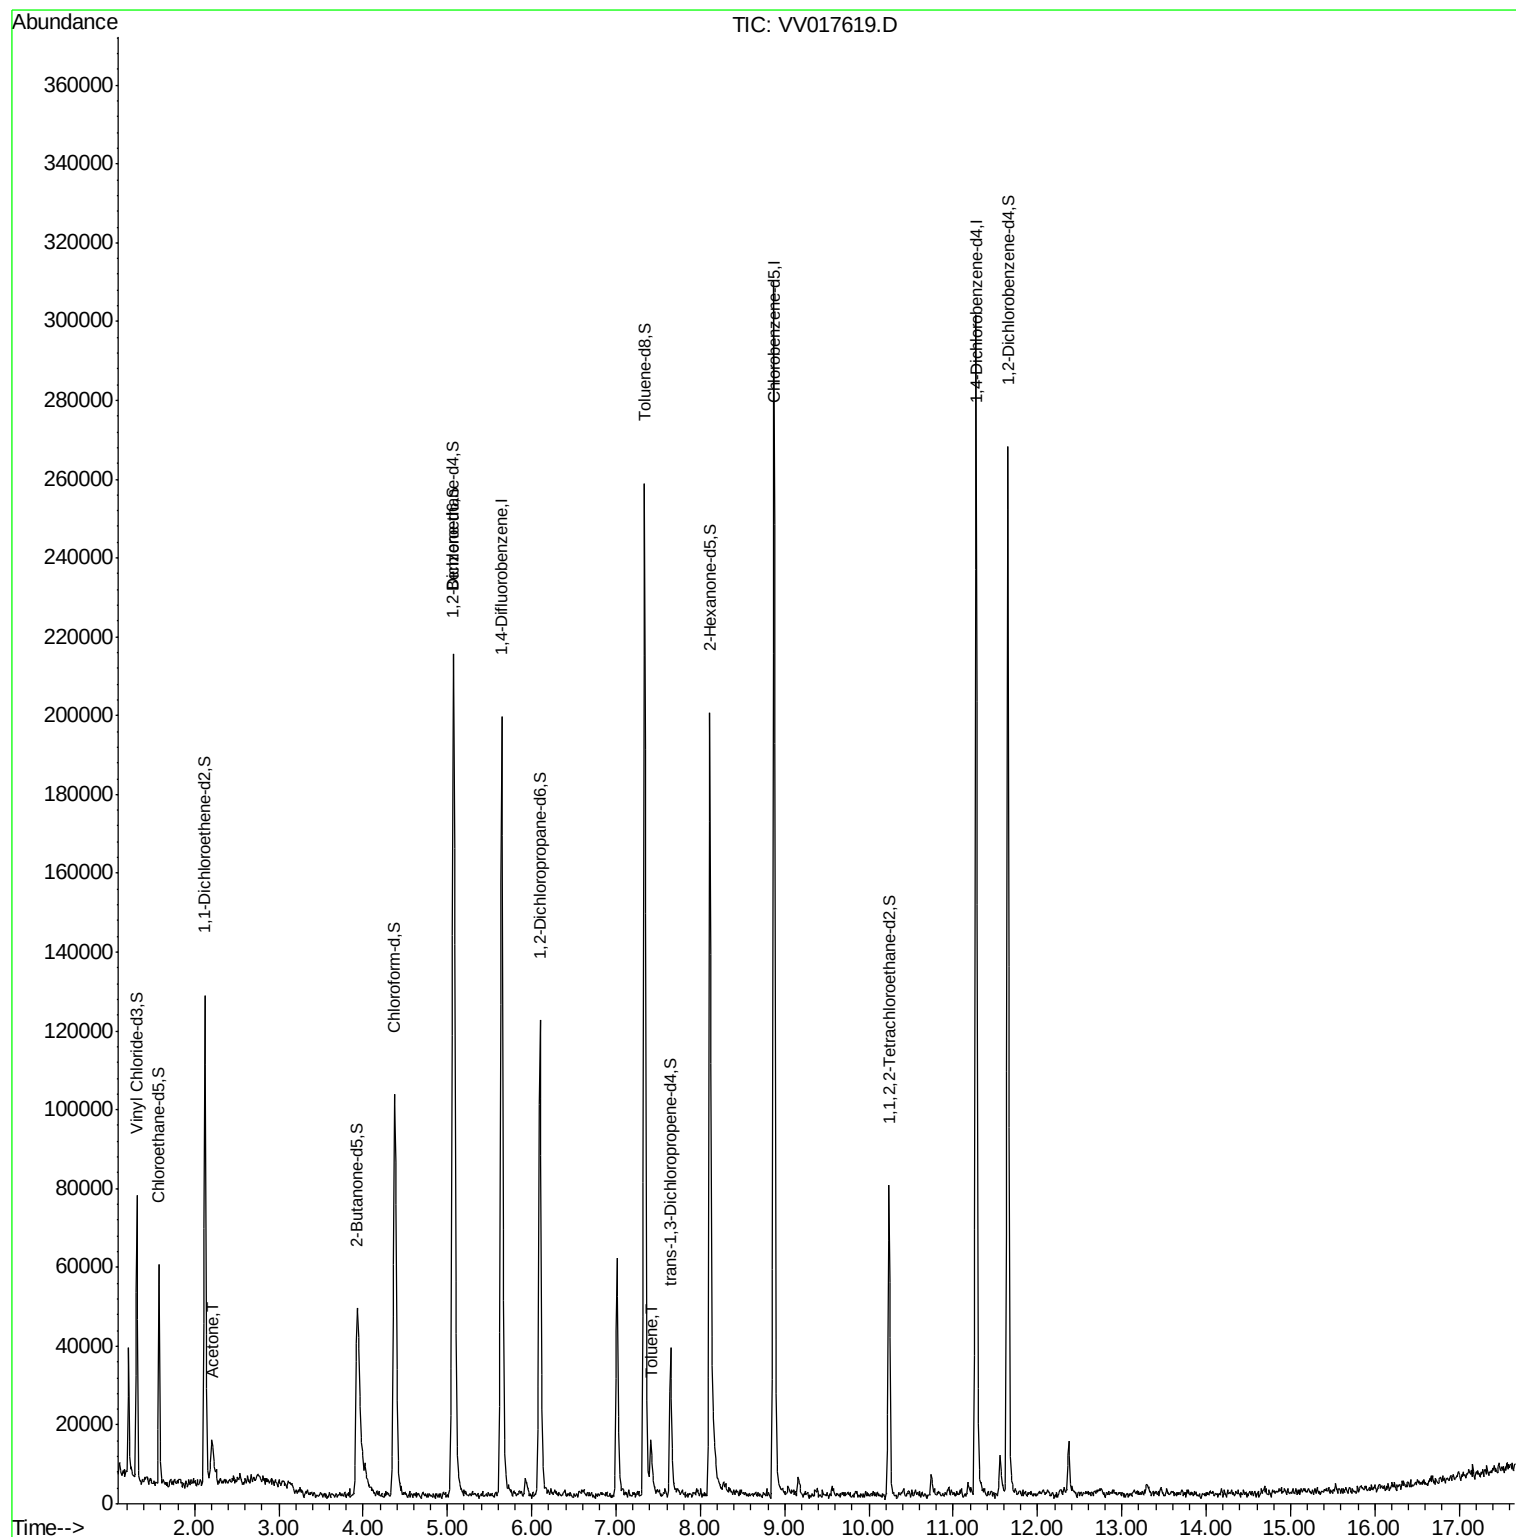

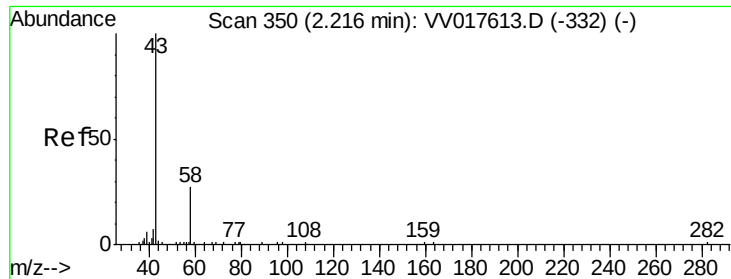

#13

Acetone

Concen: 14.586 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.01 min

Lab File: VV017619.D

Acq: 23 Jul 2020 22:15

Instrument :

MSVOA_V

ClientSampleId :





F4C23

Tot Ion: 43 Resp: 21026

Ion Ratio Lower Upper

43 100

58 30.1 0.0 18.6#

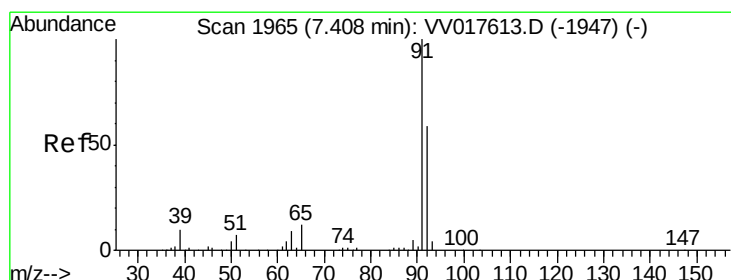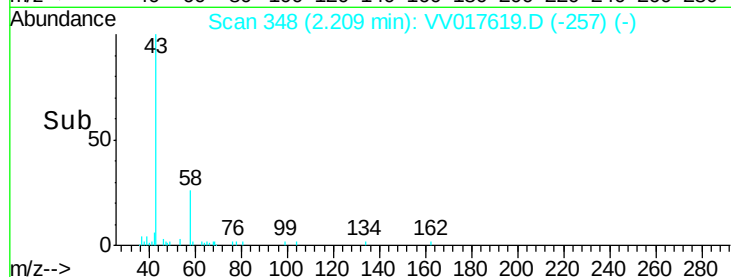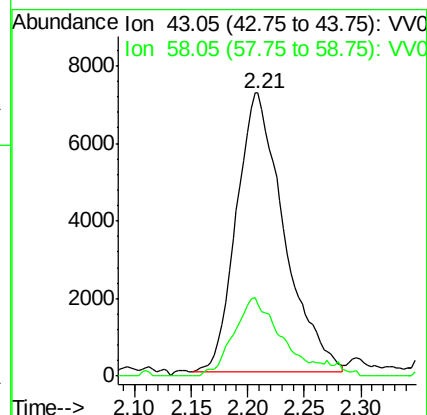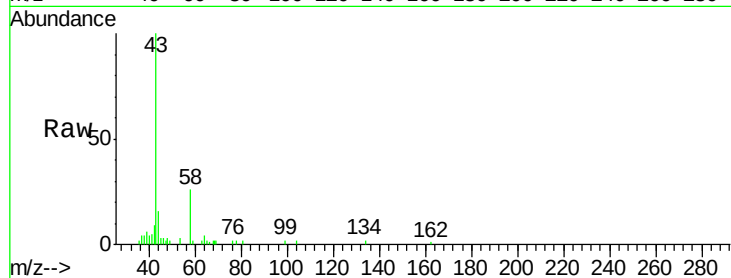

#42

Toluene

Concen: 0.178 ug/L

RT: 7.41 min Scan# 1966

Delta R.T. 0.00 min

Lab File: VV017619.D

Acq: 23 Jul 2020 22:15

Tgt Ion: 91 Resp: 8908

Ion Ratio Lower Upper

91 100

92 52.4 40.8 75.8

