

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072320\
 Data File : VV017639.D
 Acq On : 24 Jul 2020 09:51
 Operator : SY/MD
 Sample : L3398-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 24 12:52:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 24 12:19:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	160821	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	158720	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	74022	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	37127	4.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.80%
7) Chloroethane-d5	1.58	69	29422	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.20%
11) 1,1-Dichloroethene-d2	2.12	63	62231	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	3.96	46	84197	45.83	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.66%
24) Chloroform-d	4.37	84	95218	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	5.06	65	51283	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	5.07	84	165573	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
36) 1,2-Dichloropropane-d6	6.09	67	45183	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	7.34	98	148686	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
45) trans-1,3-Dichloropropene-	7.65	79	19580	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
48) 2-Hexanone-d5	8.12	63	57232	41.90	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.80%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	31558	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	61851	5.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.60%


Target Compounds					Ovalue
16) Methylene chloride	2.52	84	1389	0.144 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072320\
Data File : VV017639.D
Acq On : 24 Jul 2020 09:51
Operator : SY/MD
Sample : L3398-09
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 24 12:52:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 24 12:19:07 2020
Response via : Initial Calibration

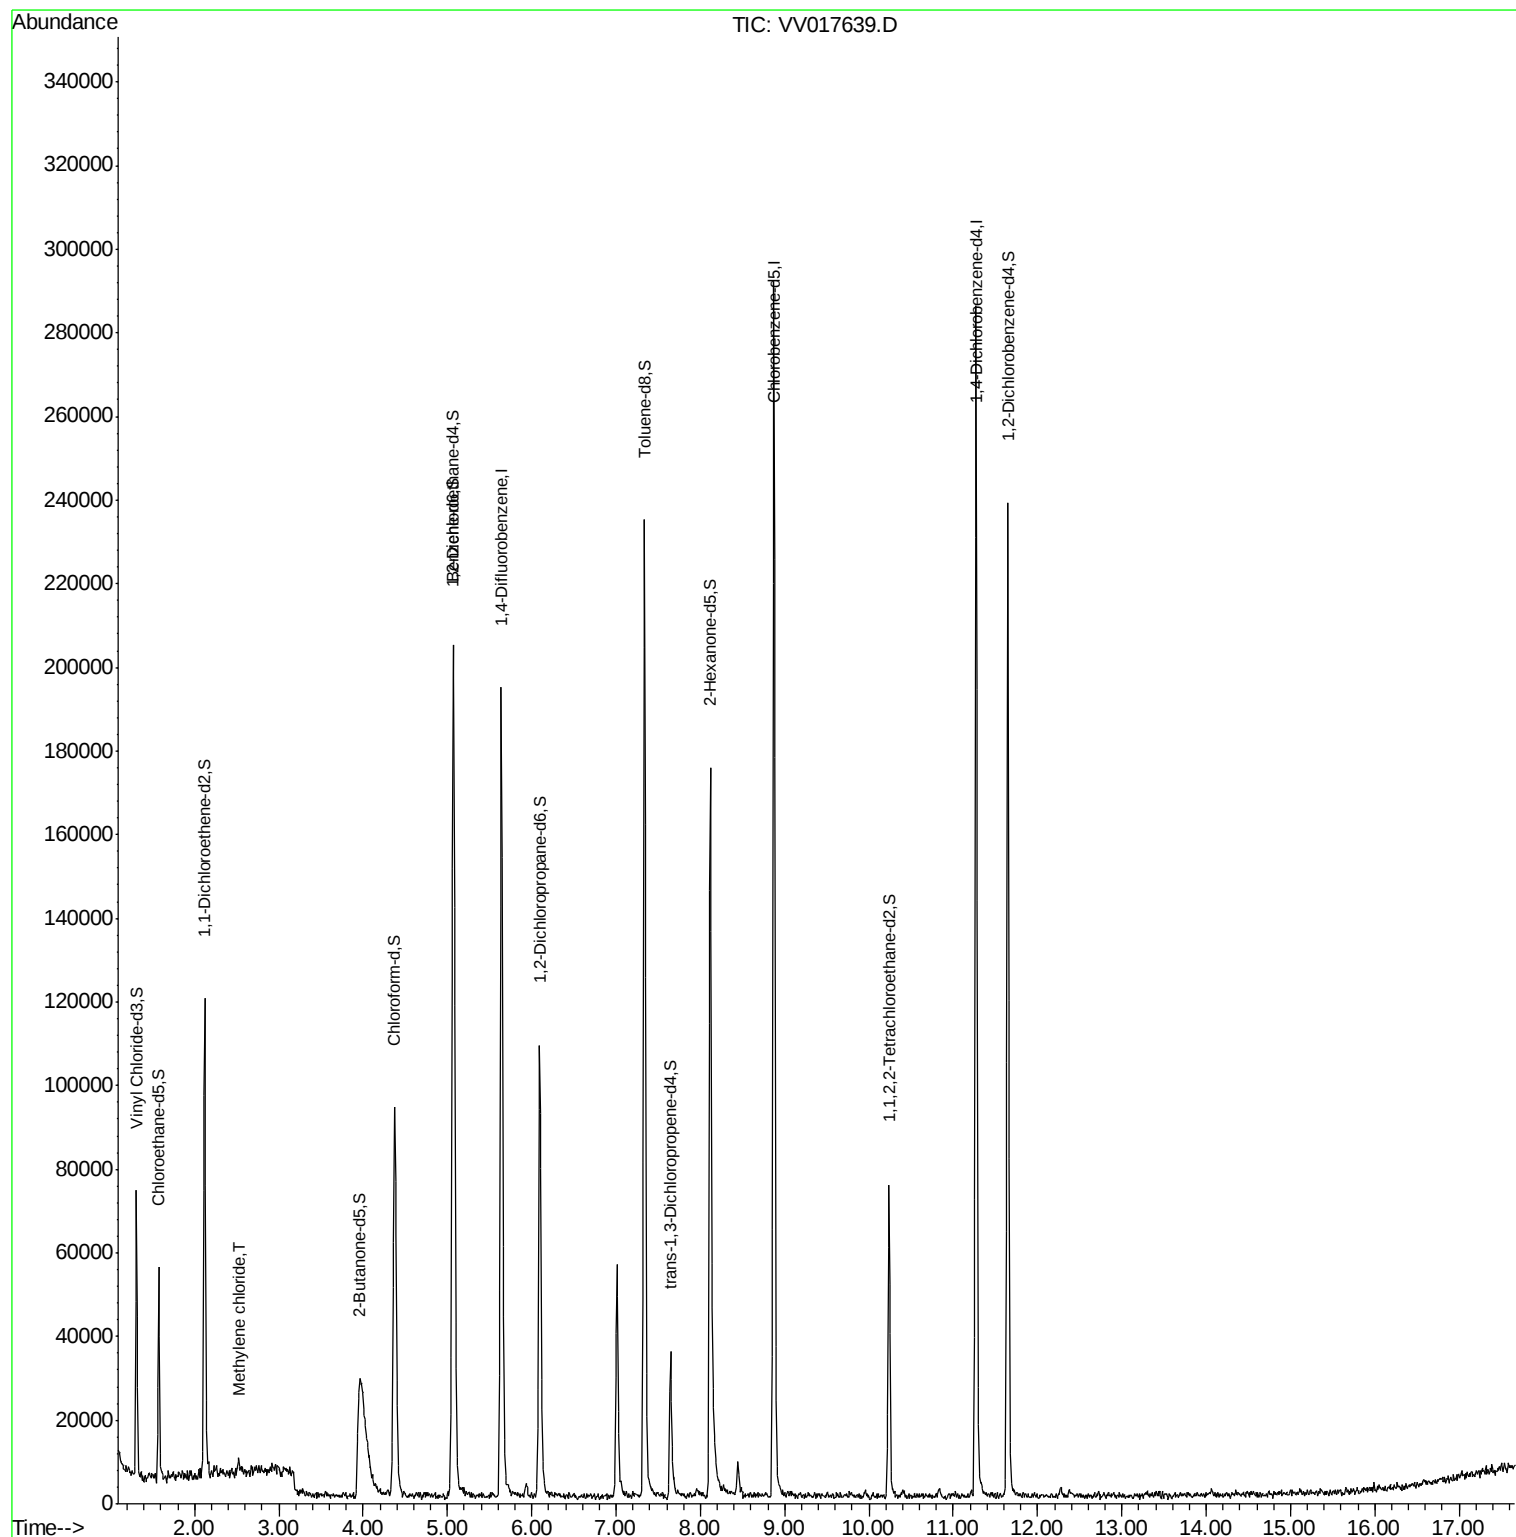

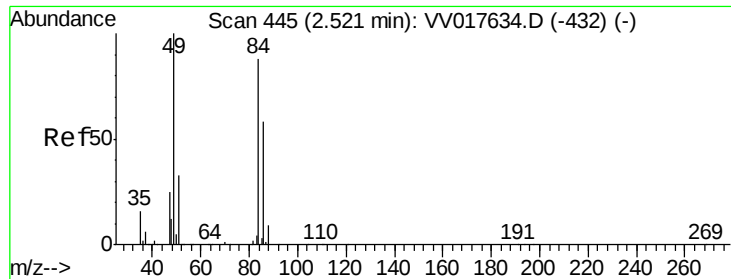

#16
 Methvlene chloride
 Concen: 0.144 ug/L
 RT: 2.52 min Scan# 446
 Delta R.T. 0.00 min
 Lab File: VV017639.D
 Acq: 24 Jul 2020 09:51

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 1389
 Ion Ratio Lower Upper
 84 100
 86 68.5 46.5 86.3
 49 136.9 79.2 147.2

