


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072320\
 Data File : VV017596.D
 Acq On : 23 Jul 2020 09:14
 Operator : SY/MD
 Sample : BFB51
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB51

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jul 24 12:19:07 2020

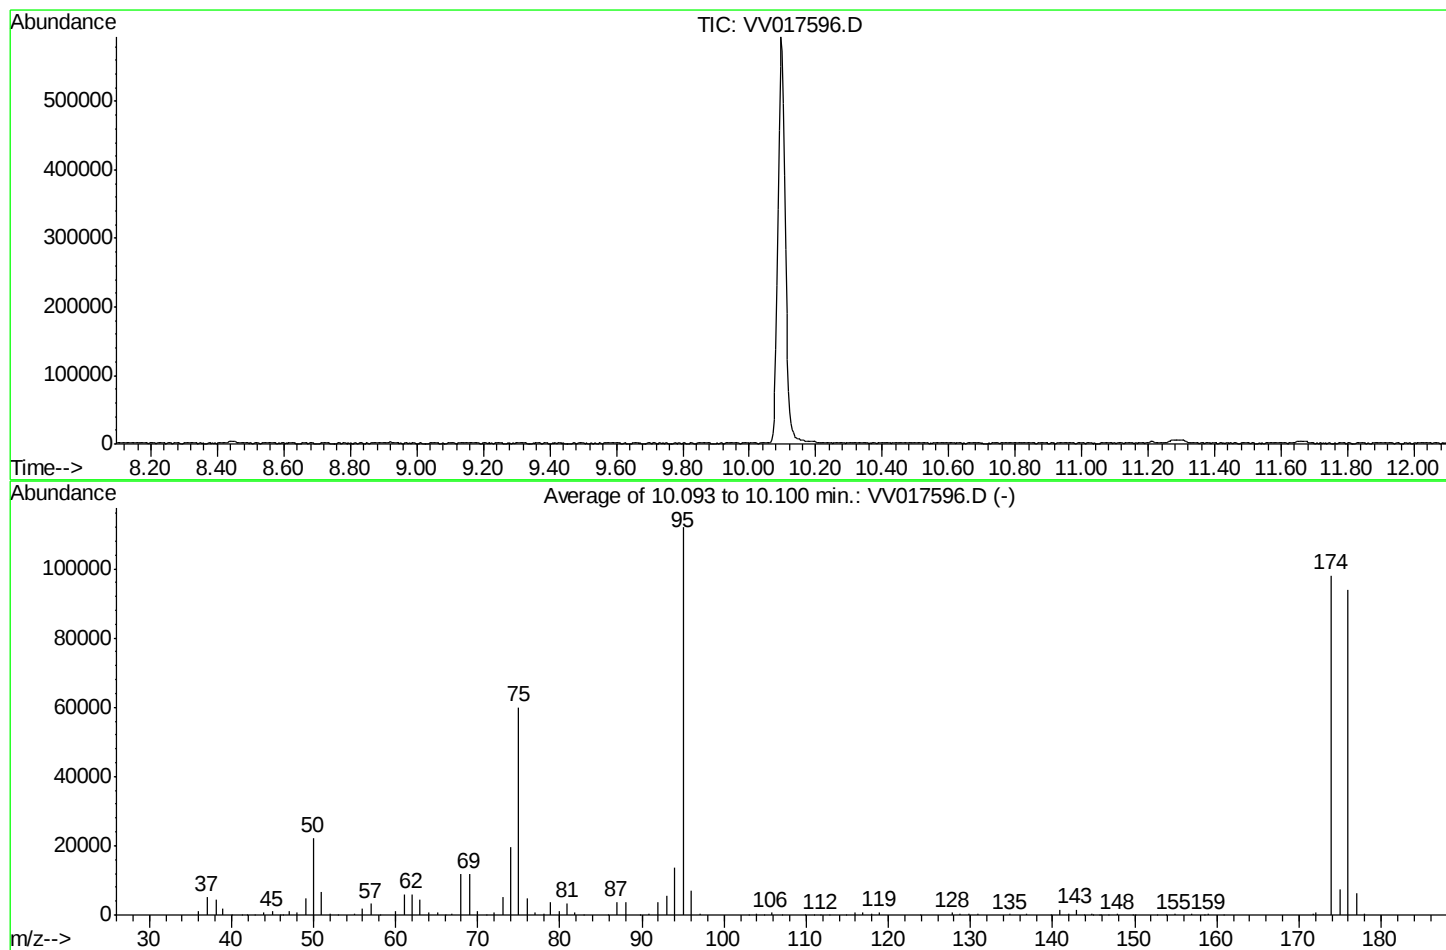

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	22318	PASS
75	95	30	80	53.6	59992	PASS
95	95	100	100	100.0	111962	PASS
96	95	5	9	6.4	7181	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.7	98136	PASS
175	174	5	9	7.5	7344	PASS
176	174	95	101	95.5	93754	PASS
177	176	5	9	6.6	6226	PASS

m/z	Abundance
36.00	1189.0
37.10	5453.0
38.10	4707.0
39.00	1913.0
40.00	291.0
41.30	104.0
44.00	1031.0
45.00	993.0
45.90	165.0
46.30	200.0
47.00	1018.0
48.00	552.0
49.00	4346.0
50.00	22272.0
51.00	6643.0
51.90	326.0
52.90	161.0
55.00	365.0
56.00	1614.0
57.00	3322.0
58.20	169.0
60.00	1061.0
61.00	5799.0
62.00	5796.0
63.00	4233.0
63.90	647.0
65.10	917.0
66.00	111.0
66.90	455.0
68.00	11273.0
69.00	11725.0
70.00	1000.0
72.00	712.0
73.00	5211.0
74.00	19080.0
75.00	58704.0
76.00	4730.0
76.90	736.0
77.90	416.0
78.90	3489.0
79.90	1236.0
80.90	3559.0
81.80	846.0
82.90	108.0
85.80	147.0
86.90	3458.0
88.00	3639.0
90.90	501.0
92.00	3418.0
93.00	5384.0
94.00	13264.0
95.00	107688.0
96.00	6968.0
97.10	324.0
103.10	118.0
103.90	489.0
104.90	210.0
105.80	600.0
107.00	205.0
109.80	128.0
111.80	140.0
112.80	134.0
115.90	561.0
116.90	769.0
118.00	501.0
118.90	820.0
123.90	130.0
127.80	601.0
128.70	148.0
129.80	421.0
130.90	240.0
134.80	268.0
136.80	250.0
139.70	120.0
140.90	1616.0
141.90	235.0
142.90	1533.0
144.70	361.0
145.70	172.0
145.90	153.0
146.80	121.0
148.00	373.0
149.70	170.0
152.70	141.0
153.70	139.0
154.90	313.0
157.00	222.0
159.00	260.0
160.80	132.0
171.80	879.0
172.10	899.0
174.00	92680.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

174.90	6910.0
175.90	87904.0
177.00	5855.0
178.00	244.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
36.00	1240.0
37.10	5725.0
38.10	4784.0
39.00	1987.0
39.90	363.0
44.00	992.0
45.00	1052.0
46.30	213.0
47.00	996.0
47.90	674.0
49.00	4826.0
50.00	23272.0
51.00	7180.0
52.00	421.0
52.90	194.0
55.10	353.0
56.00	1868.0
57.00	3296.0
58.10	171.0
60.00	1107.0
61.00	6080.0
62.00	6375.0
63.00	4468.0
64.00	699.0
65.10	921.0
66.90	495.0
68.00	12386.0
69.00	12363.0
70.00	968.0
72.00	794.0
73.00	5217.0
74.00	20472.0
75.00	62264.0
76.00	5034.0
76.90	903.0
78.00	457.0
78.90	3667.0
79.90	1186.0
80.90	3600.0
81.80	977.0
85.80	189.0
86.90	3949.0
88.00	3686.0
89.80	110.0
90.90	530.0
92.00	3873.0
93.00	5867.0
94.00	13984.0
95.00	115936.0
96.00	7413.0
97.10	331.0
103.10	123.0
103.90	584.0
104.90	197.0
105.80	610.0
107.00	206.0
109.90	138.0
110.90	105.0
111.80	156.0
112.80	127.0
114.90	120.0
115.90	620.0
116.90	929.0
118.00	507.0
118.90	941.0
123.90	114.0
127.90	628.0
128.80	205.0
129.80	479.0
130.90	207.0
134.80	293.0
136.80	264.0
139.80	132.0
140.90	1603.0
141.90	276.0
142.80	1716.0
143.90	124.0
144.70	310.0
145.60	167.0
146.80	115.0
148.00	384.0
149.70	158.0
152.70	153.0
153.80	134.0
154.90	305.0
157.00	205.0
159.00	220.0
160.90	200.0
172.10	937.0
173.90	101816.0
175.00	7644.0
175.90	97544.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

177.006459.0

178.00216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
36.00	1101.0
37.00	5280.0
38.10	4369.0
39.00	1783.0
39.90	403.0
41.90	116.0
42.80	125.0
44.00	874.0
45.00	1003.0
46.30	185.0
47.00	971.0
47.90	701.0
49.00	4814.0
50.00	21744.0
51.00	6709.0
52.00	465.0
52.90	172.0
55.00	315.0
56.00	1861.0
57.00	2897.0
58.10	223.0
60.00	1058.0
61.00	5699.0
62.00	6149.0
63.00	4103.0
64.00	695.0
65.10	840.0
66.90	455.0
68.00	12139.0
69.00	11936.0
70.00	878.0
71.10	108.0
72.00	735.0
73.00	5031.0
74.00	19432.0
75.00	59008.0
76.00	4642.0
77.00	967.0
78.10	412.0
78.90	3542.0
79.90	1024.0
80.90	3360.0
81.80	859.0
85.80	221.0
86.90	4090.0
88.00	3550.0
89.80	145.0
90.90	473.0
92.00	3582.0
93.00	5560.0
94.00	13383.0
95.00	112264.0
96.00	7162.0
97.10	311.0
102.90	110.0
103.90	608.0
104.90	155.0
105.80	578.0
107.00	160.0
109.90	123.0
110.90	123.0
111.70	144.0
112.90	122.0
114.90	158.0
115.90	548.0
116.90	965.0
118.00	463.0
118.90	908.0
127.90	601.0
128.80	273.0
129.80	485.0
130.80	164.0
134.80	279.0
136.80	237.0
139.80	117.0
140.90	1463.0
141.90	245.0
142.80	1650.0
143.90	129.0
144.90	287.0
145.80	151.0
147.90	317.0
149.70	144.0
150.10	104.0
152.80	147.0
153.90	158.0
154.90	301.0
157.00	174.0
158.50	157.0
159.00	190.0
160.80	222.0
172.00	959.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

173.90	99912.0
175.00	7480.0
175.90	95816.0
177.00	6364.0
177.90	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

Scan 2788 (10.055 min): VV017596.D
BFB51

m/z	Abundance
35.60	108.0
37.00	125.0
38.70	134.0
40.10	237.0
43.90	278.0
46.20	101.0
50.00	111.0
55.00	111.0
100.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51