

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026913.D
 Acq On : 23 Jul 2022 10:35
 Operator : SY/MD
 Sample : VV0723WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Quant Time: Jul 25 02:07:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	541335	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	557937	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	232916	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	216049	47.586	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.180%
7) Chloroethane-d5	1.564	69	187602	51.076	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.160%
11) 1,1-Dichloroethene-d2	2.101	63	297211	36.386	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.780%
21) 2-Butanone-d5	3.883	46	314148	102.652	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.650%
24) Chloroform-d	4.342	84	447046	50.031	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.060%
26) 1,2-Dichloroethane-d4	5.024	65	266945	52.227	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.460%
32) Benzene-d6	5.043	84	871503	51.675	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.340%
36) 1,2-Dichloropropane-d6	6.066	67	286014	52.624	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.240%
41) Toluene-d8	7.313	98	708507	48.013	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.020%
43) trans-1,3-Dichloroprop...	7.619	79	92664	40.689	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.380%
47) 2-Hexanone-d5	8.088	63	233370	98.613	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.610%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	406340	49.214	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.420%
66) 1,2-Dichlorobenzene-d4	11.622	152	267618	61.245	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	122.480%#
Target Compounds						
61) 1,2,3-Trichloropropane	11.246	75	26378	5.644	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026913.D
Acq On : 23 Jul 2022 10:35
Operator : SY/MD
Sample : VV0723WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Time: Jul 25 02:07:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

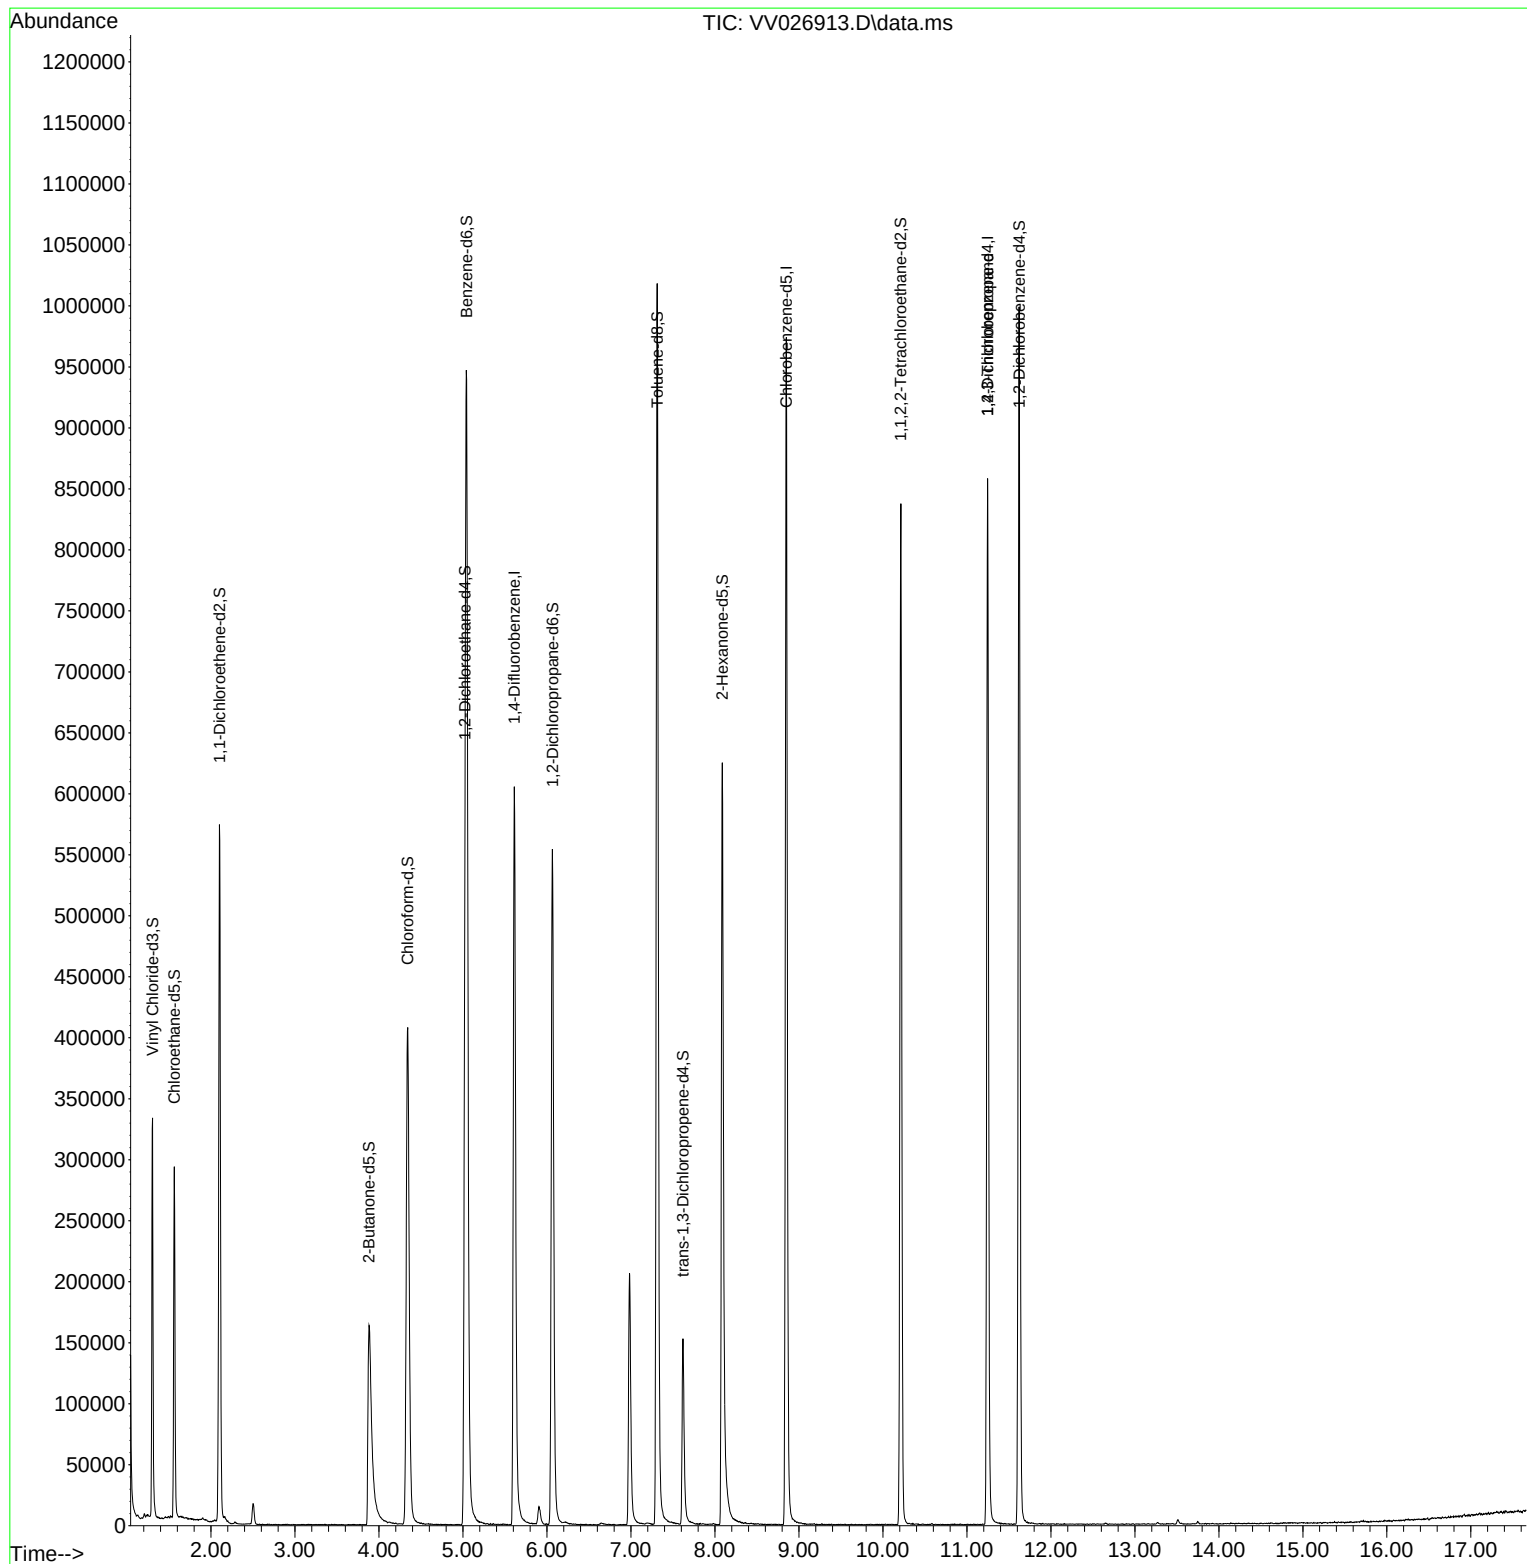

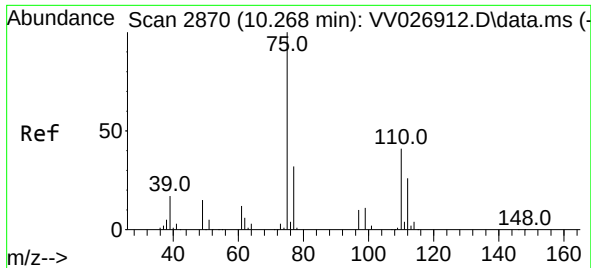

#61

1,2,3-Trichloropropane

Concen: 5.644 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.977 min

Lab File: VV026913.D


Acq: 23 Jul 2022 10:35

Instrument :

MSVOA_V

ClientSampleId :

VBLK225

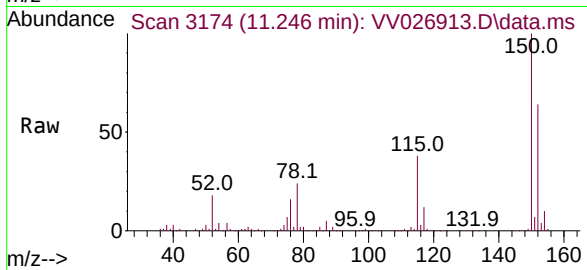

Tgt Ion: 75 Resp: 26378

Ion Ratio Lower Upper

75 100

77 29.9 25.6 38.4

110 2.5 31.7 47.5#

