

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026915.D
 Acq On : 23 Jul 2022 12:20
 Operator : SY/MD
 Sample : N3743-06ME
 Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5C93ME

Quant Time: Jul 25 02:07:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	701441	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	688759	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	297292	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	125730	21.372	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	42.740%#		
7) Chloroethane-d5	1.558	69	49445	10.389	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	20.780%#		
11) 1,1-Dichloroethene-d2	2.076	63	183695	17.356	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	34.720%#		
21) 2-Butanone-d5	3.905	46	200586	50.584	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery =	50.580%		
24) Chloroform-d	4.336	84	285232	24.635	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	49.280%#		
26) 1,2-Dichloroethane-d4	5.021	65	178955	27.021	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	54.040%#		
32) Benzene-d6	5.037	84	571657	27.457	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	54.920%#		
36) 1,2-Dichloropropane-d6	6.063	67	188761	28.134	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	56.260%#		
41) Toluene-d8	7.310	98	460866	25.299	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	50.600%#		
43) trans-1,3-Dichloroprop...	7.622	79	72457	25.773	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	51.540%#		
47) 2-Hexanone-d5	8.098	63	140071	47.947	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	47.950%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	258105	25.323	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	50.640%#		
66) 1,2-Dichlorobenzene-d4	11.625	152	178462	31.997	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	64.000%#		
Target Compounds					Qvalue	
22) 2-Butanone	4.002	43	32403	8.533	ug/L	78
61) 1,2,3-Trichloropropane	11.249	75	35207	5.902	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026915.D
Acq On : 23 Jul 2022 12:20
Operator : SY/MD
Sample : N3743-06ME
Misc : 5.55g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5C93ME

Quant Time: Jul 25 02:07:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration




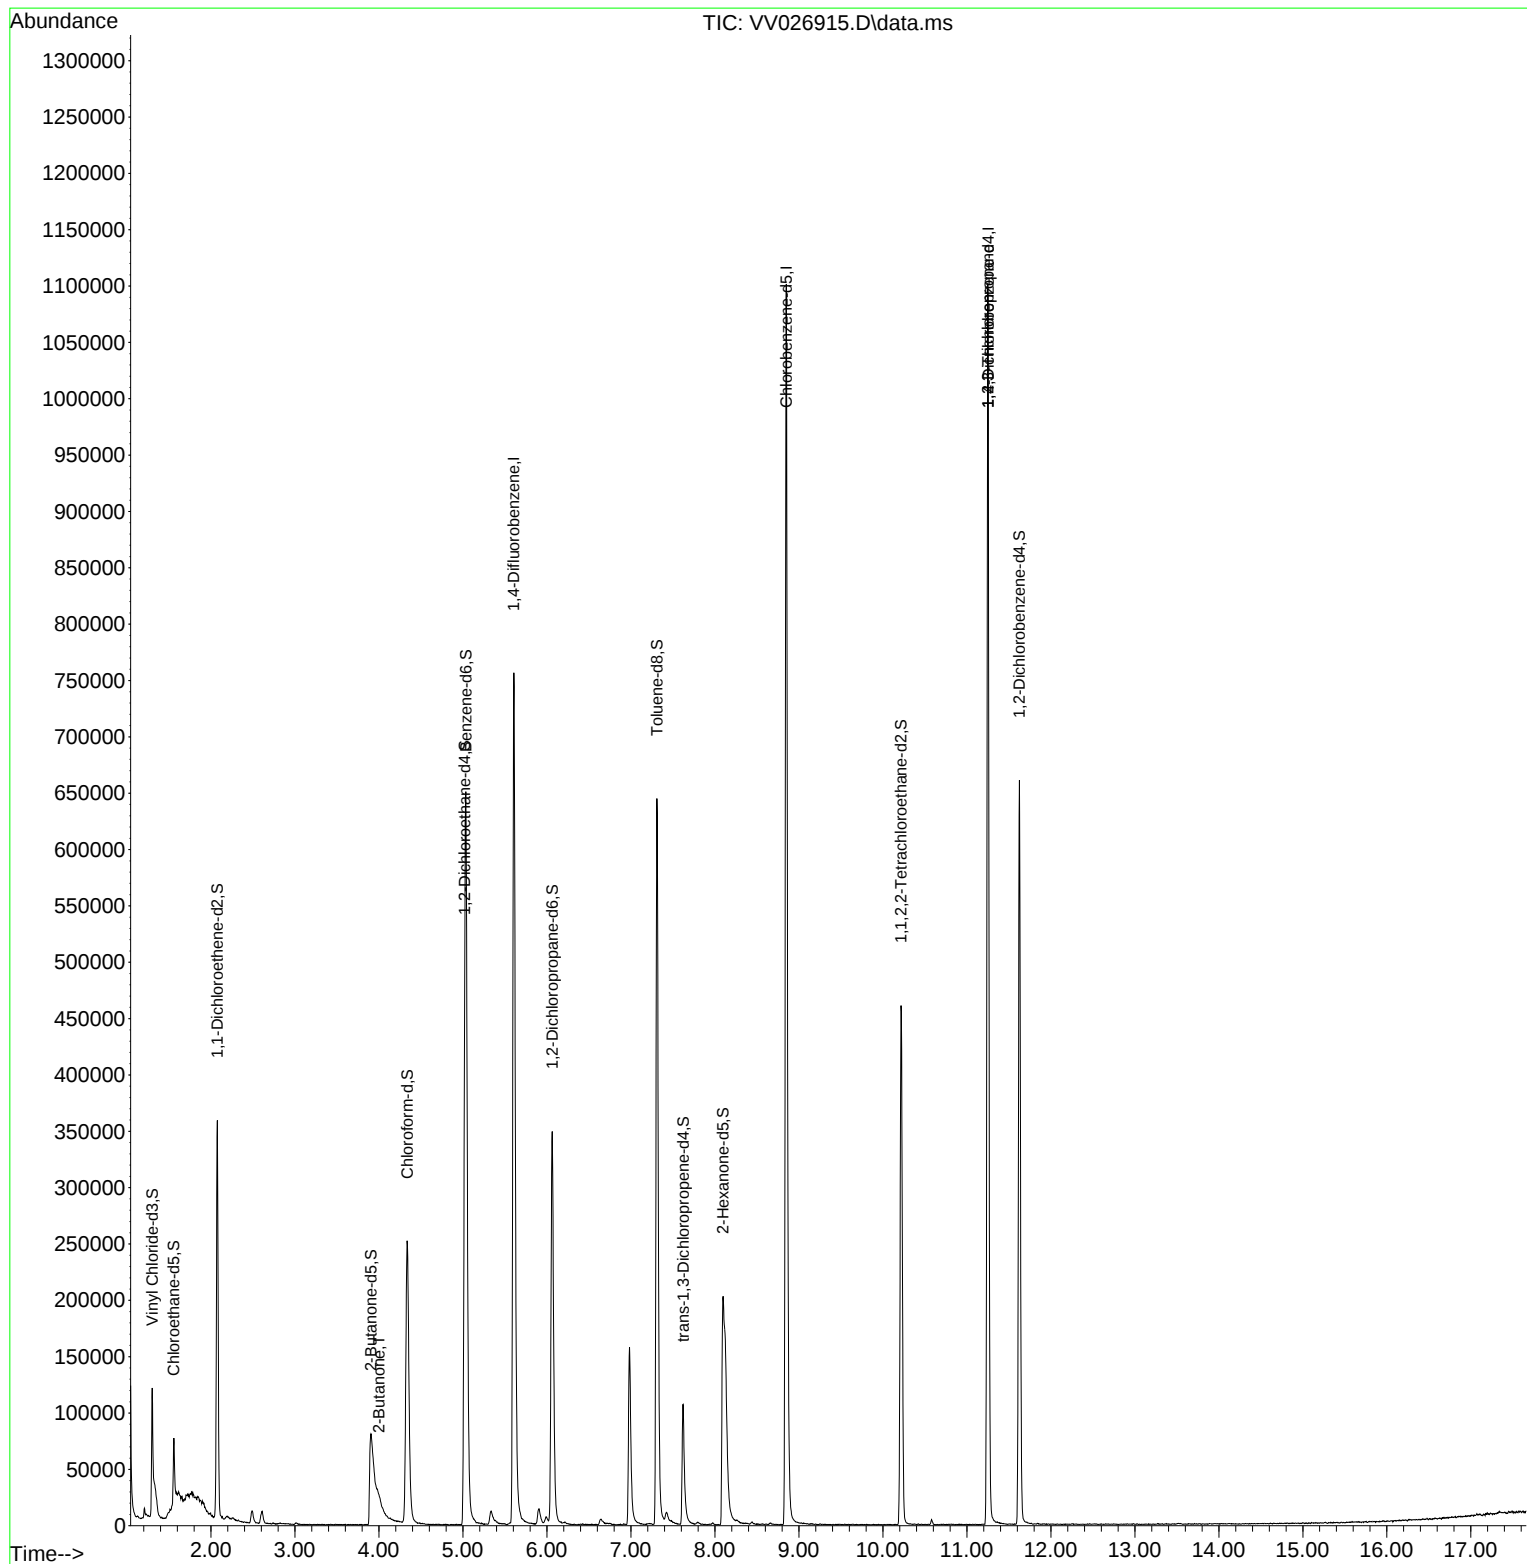


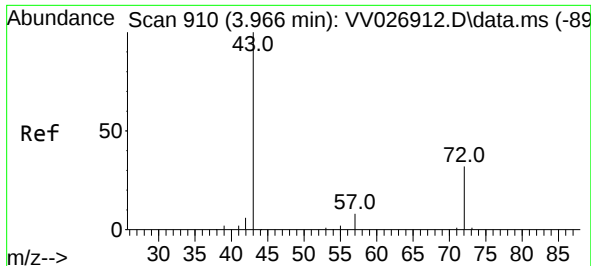

#22
2-Butanone
Concen: 8.533 ug/L
RT: 4.002 min Scan# 910
Delta R.T. 0.035 min
Lab File: VV026915.D
Acq: 23 Jul 2022 12:20

Instrument :
MSVOA_V
ClientSampleId :
F5C93ME

Tgt Ion: 43 Resp: 32403
Ion Ratio Lower Upper
43 100
72 17.7 14.9 44.5

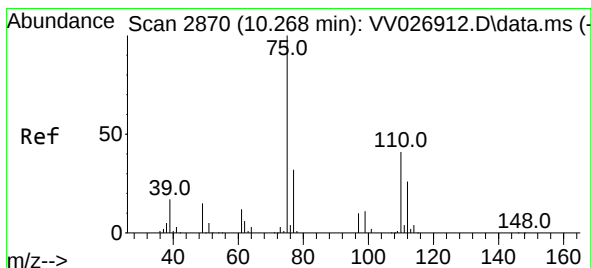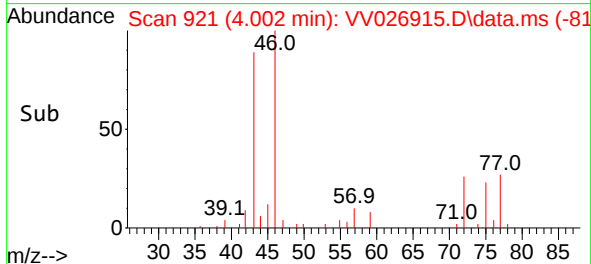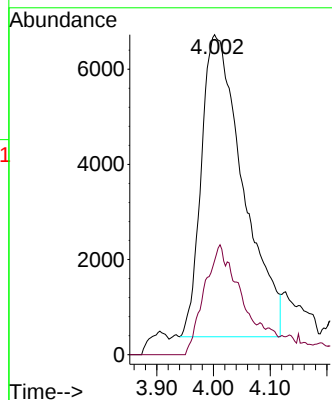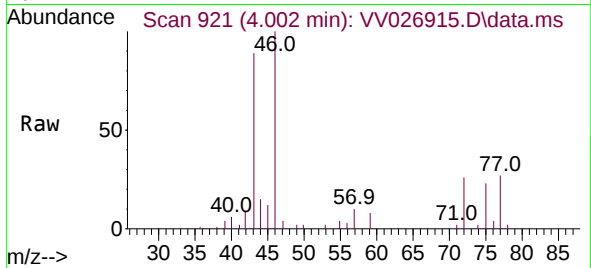

#61
1,2,3-Trichloropropane
Concen: 5.902 ug/L
RT: 11.249 min Scan# 3175
Delta R.T. 0.981 min
Lab File: VV026915.D
Acq: 23 Jul 2022 12:20

Tgt Ion: 75 Resp: 35207
Ion Ratio Lower Upper
75 100
77 31.0 25.6 38.4
110 2.7 31.7 47.5#

