

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026923.D
 Acq On : 23 Jul 2022 15:37
 Operator : SY/MD
 Sample : N3741-08ME
 Misc : 5.51g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B33ME


Quant Time: Jul 25 02:09:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	1553302	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	1466632	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	713423	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	36298	2.786	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	5.580%#
7) Chloroethane-d5	1.558	69	16375	1.554	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	3.100%#
11) 1,1-Dichloroethene-d2	2.085	63	48466	2.068	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	4.140%#
21) 2-Butanone-d5	3.915	46	47545	5.414	ug/L	0.04
Spiked Amount	100.000	Range	40 - 130	Recovery	=	5.410%#
24) Chloroform-d	4.342	84	73867	2.881	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	5.760%#
26) 1,2-Dichloroethane-d4	5.031	65	46233	3.152	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	6.300%#
32) Benzene-d6	5.043	84	139058	3.137	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	6.280%#
36) 1,2-Dichloropropane-d6	6.066	67	46352	3.244	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	6.480%#
41) Toluene-d8	7.317	98	100636	2.594	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	5.180%#
43) trans-1,3-Dichloroprop...	7.628	79	16046	2.680	ug/L	0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	5.360%#
47) 2-Hexanone-d5	8.101	63	26937	4.330	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	4.330%#
56) 1,1,2,2-Tetrachloroeth...	10.217	84	62117	2.862	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	5.720%#
66) 1,2-Dichlorobenzene-d4	11.625	152	43113	3.221	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	6.440%#
Target Compounds						Qvalue
15) Methyl Acetate	2.436	43	20808	1.530	ug/L	98
61) 1,2,3-Trichloropropane	11.246	75	80509	5.624	ug/L #	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jul 25 02:09:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration







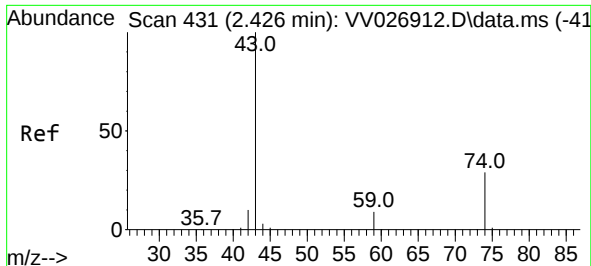

#15
Methyl Acetate
Concen: 1.530 ug/L
RT: 2.436 min Scan# 41
Delta R.T. 0.010 min
Lab File: VV026923.D
Acq: 23 Jul 2022 15:37

Instrument :
MSVOA_V
ClientSampleId :
H0B33ME

Tgt Ion: 43 Resp: 20808
Ion Ratio Lower Upper
43 100
74 26.4 22.1 33.1

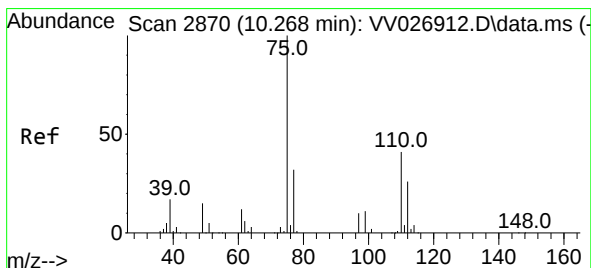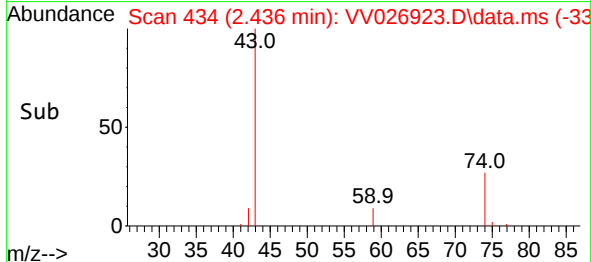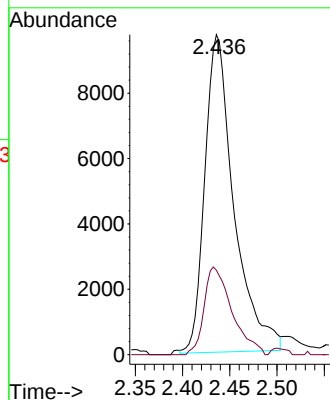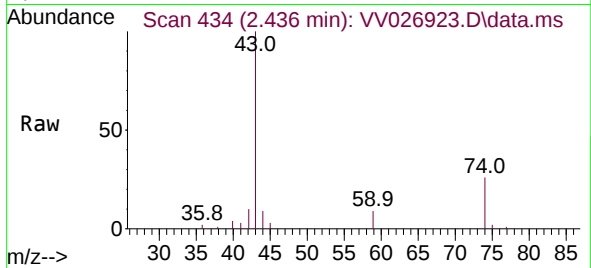

#61
1,2,3-Trichloropropane
Concen: 5.624 ug/L
RT: 11.246 min Scan# 3174
Delta R.T. 0.977 min
Lab File: VV026923.D
Acq: 23 Jul 2022 15:37

Tgt Ion: 75 Resp: 80509
Ion Ratio Lower Upper
75 100
77 31.5 25.6 38.4
110 2.9 31.7 47.5#

