

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026924.D
 Acq On : 23 Jul 2022 16:01
 Operator : SY/MD
 Sample : N3745-02ME
 Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

Quant Time: Jul 25 02:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	722061	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	705088	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	310402	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	201095	33.206	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	66.420%
7) Chloroethane-d5	1.558	69	76365	15.587	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	31.180%#
11) 1,1-Dichloroethene-d2	2.076	63	296184	27.185	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.360%#
21) 2-Butanone-d5	3.896	46	391994	96.030	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.030%
24) Chloroform-d	4.339	84	494132	41.459	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.920%
26) 1,2-Dichloroethane-d4	5.021	65	301515	44.226	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.460%
32) Benzene-d6	5.037	84	988095	46.360	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.720%
36) 1,2-Dichloropropane-d6	6.063	67	326972	47.605	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.200%
41) Toluene-d8	7.310	98	819011	43.919	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.840%
43) trans-1,3-Dichloroprop...	7.619	79	123331	42.853	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.700%
47) 2-Hexanone-d5	8.095	63	292305	97.739	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.740%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	462880	44.362	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.720%
66) 1,2-Dichlorobenzene-d4	11.625	152	307547	52.813	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.620%
Target Compounds						Qvalue
22) 2-Butanone	3.999	43	27941	7.148	ug/L	73
39) cis-1,3-Dichloropropene	6.982	75	6845	0.836	ug/L #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026924.D
Acq On : 23 Jul 2022 16:01
Operator : SY/MD
Sample : N3745-02ME
Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D06ME

Quant Time: Jul 25 02:09:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration




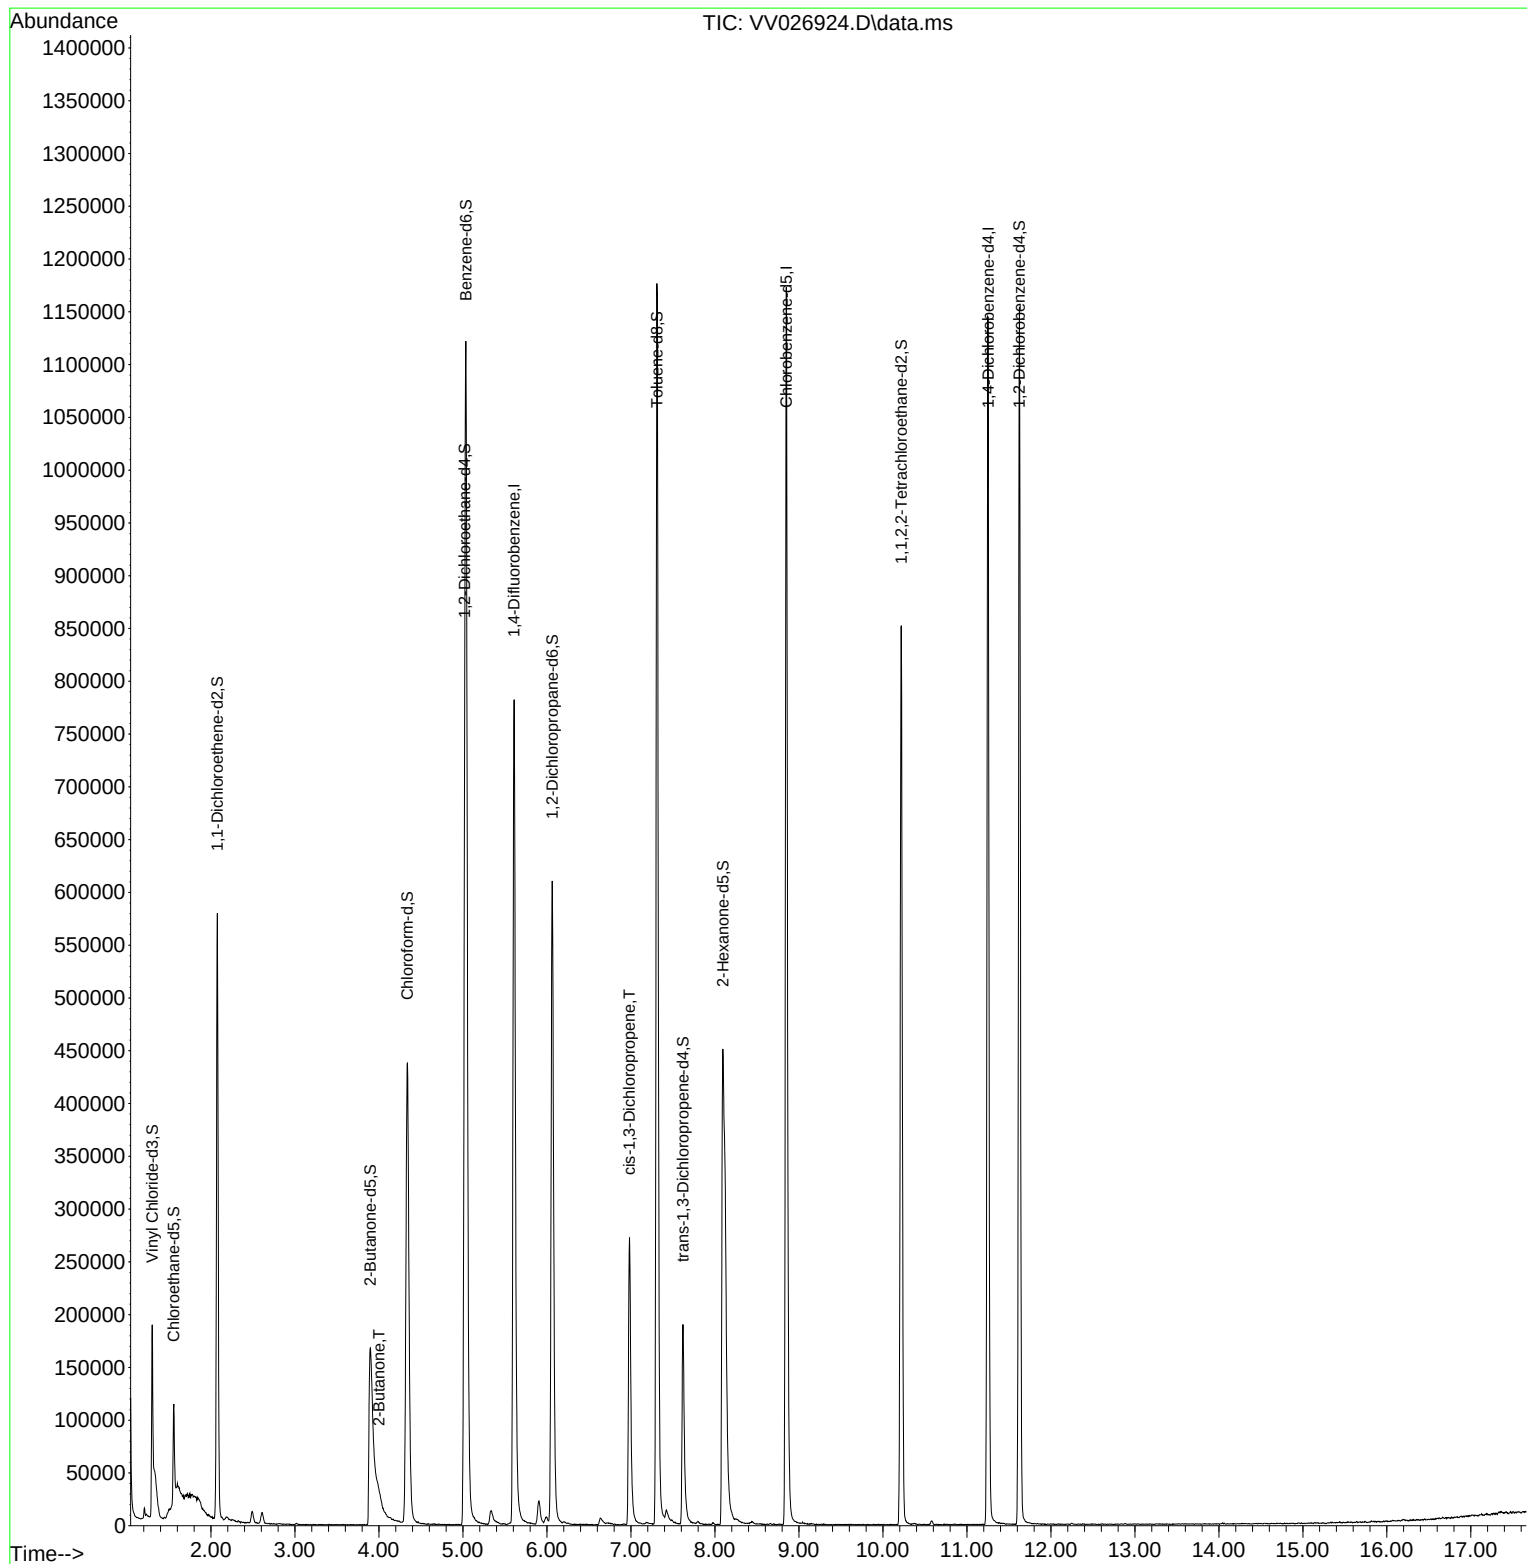


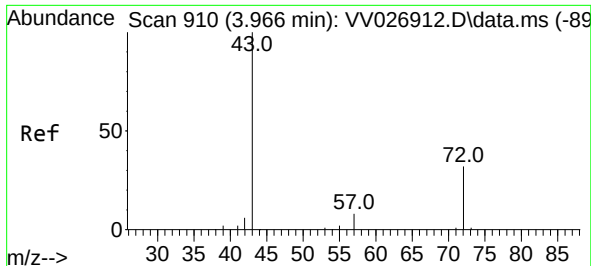

#22
2-Butanone
Concen: 7.148 ug/L
RT: 3.999 min Scan# 910
Delta R.T. 0.032 min
Lab File: VV026924.D
Acq: 23 Jul 2022 16:01

Instrument :
MSVOA_V
ClientSampleId :
F5D06ME

Tgt Ion: 43 Resp: 27941
Ion Ratio Lower Upper
43 100
72 15.3 14.9 44.5

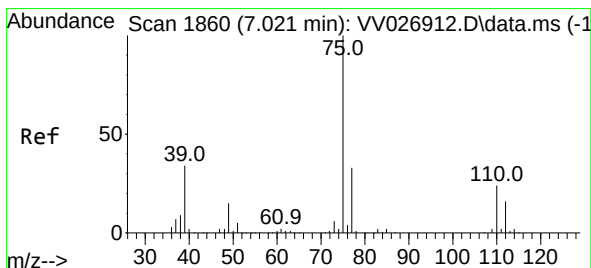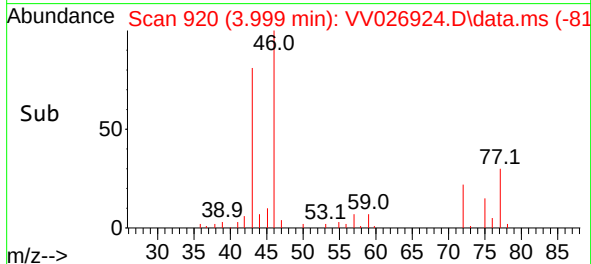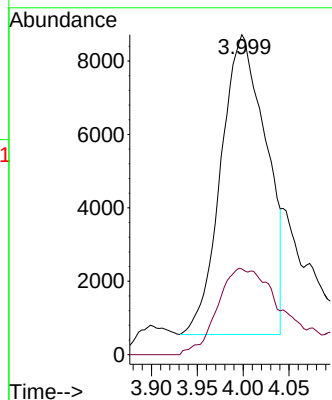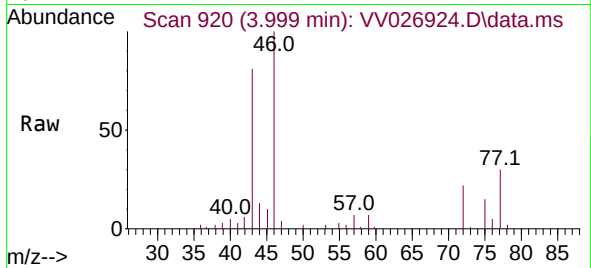

#39
cis-1,3-Dichloropropene
Concen: 0.836 ug/L
RT: 6.982 min Scan# 1848
Delta R.T. -0.038 min
Lab File: VV026924.D
Acq: 23 Jul 2022 16:01

Tgt Ion: 75 Resp: 6845
Ion Ratio Lower Upper
75 100
77 47.0 22.4 41.6#

