

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072322\
 Data File : VW026927.D
 Acq On : 23 Jul 2022 17:15
 Operator : SY/MD
 Sample : N3766-09ME
 Misc : 3.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COZD6ME

Quant Time: Jul 25 02:09:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	678609	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	662367	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	293931	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	137581	24.173	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	48.340%#
7) Chloroethane-d5	1.558	69	75662	16.432	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	32.860%#
11) 1,1-Dichloroethene-d2	2.079	63	280633	27.407	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.820%#
21) 2-Butanone-d5	3.895	46	382839	99.792	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.790%
24) Chloroform-d	4.339	84	463375	41.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.740%
26) 1,2-Dichloroethane-d4	5.024	65	292341	45.626	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.260%
32) Benzene-d6	5.037	84	929765	46.437	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.880%
36) 1,2-Dichloropropane-d6	6.063	67	308963	47.884	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.760%
41) Toluene-d8	7.313	98	765445	43.694	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.380%
43) trans-1,3-Dichloroprop...	7.619	79	113593	42.015	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.040%
47) 2-Hexanone-d5	8.095	63	278191	99.020	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	438307	44.716	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.440%
66) 1,2-Dichlorobenzene-d4	11.625	152	288969	52.403	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.800%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.436	43	10454	1.759	ug/L	92
48) 2-Hexanone	8.095	43	30508	5.941	ug/L #	68
61) 1,2,3-Trichloropropane	11.252	75	34447	5.840	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026927.D
Acq On : 23 Jul 2022 17:15
Operator : SY/MD
Sample : N3766-09ME
Misc : 3.30g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZD6ME

Quant Time: Jul 25 02:09:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration




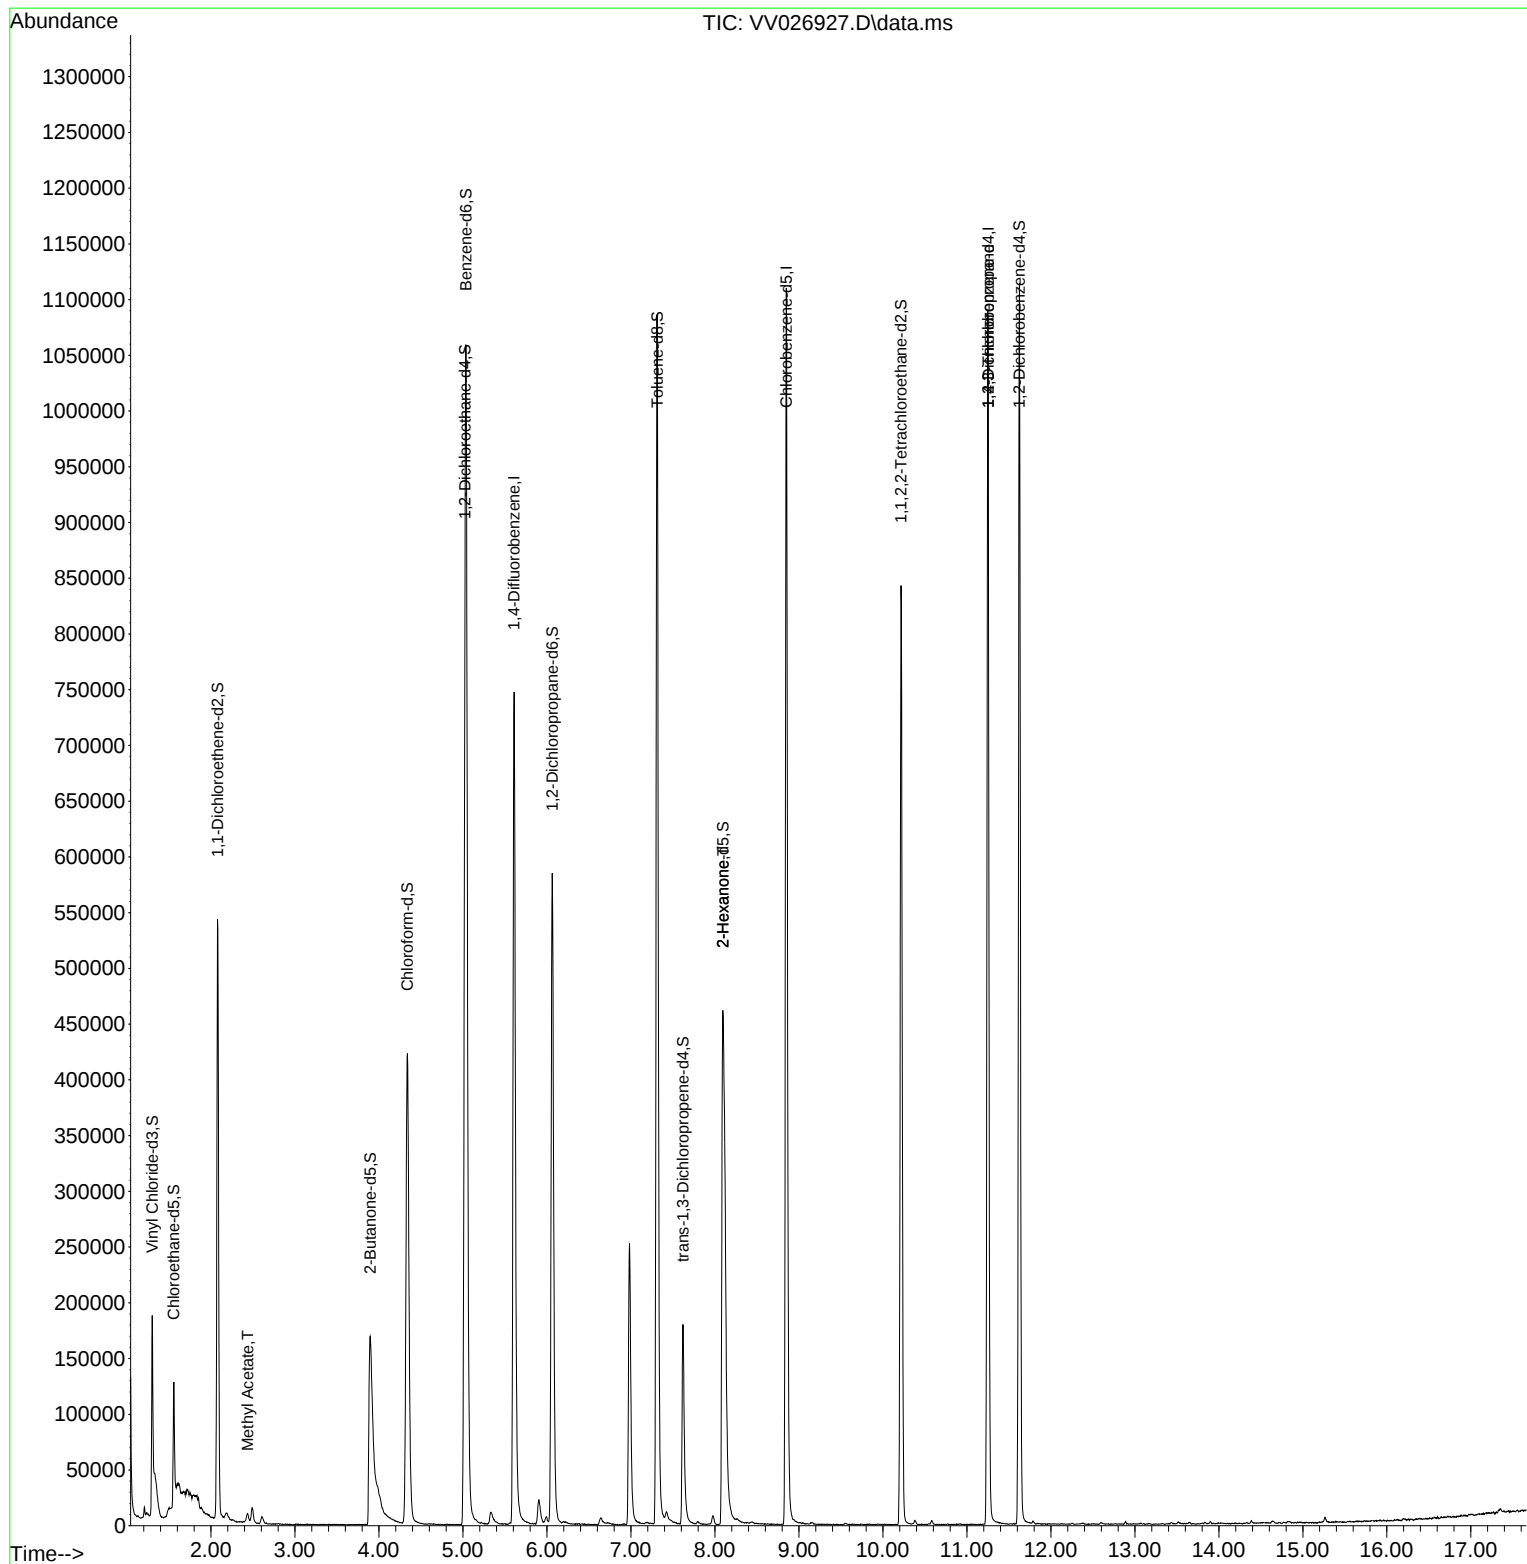


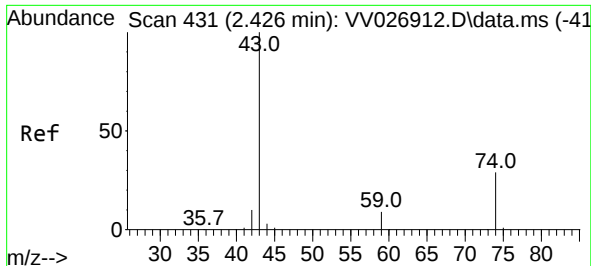

#15
Methyl Acetate
Concen: 1.759 ug/L
RT: 2.436 min Scan# 41
Delta R.T. 0.010 min
Lab File: VV026927.D
Acq: 23 Jul 2022 17:15




Instrument :
MSVOA_V
ClientSampleId :
COZD6ME


Tgt Ion: 43 Resp: 10454
Ion Ratio Lower Upper
43 100
74 31.8 22.1 33.1

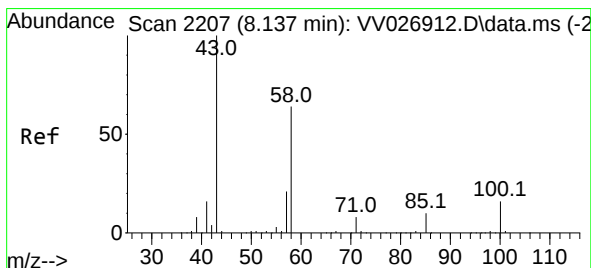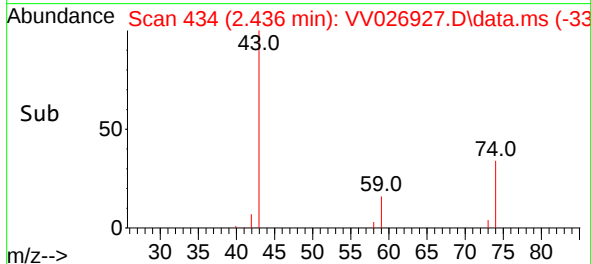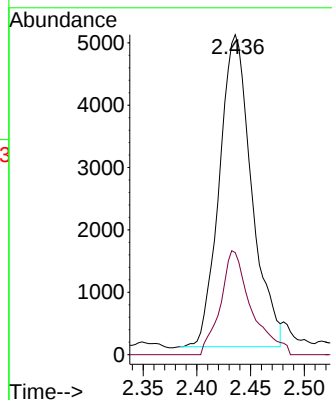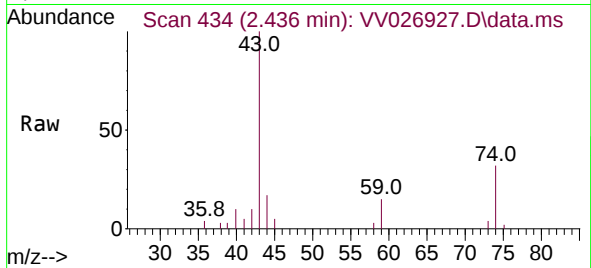

#48
2-Hexanone
Concen: 5.941 ug/L
RT: 8.095 min Scan# 2194
Delta R.T. -0.042 min
Lab File: VV026927.D
Acq: 23 Jul 2022 17:15

Tgt Ion: 43 Resp: 30508
Ion Ratio Lower Upper
43 100
58 37.7 48.8 73.2#
57 38.3 16.6 24.8#
100 2.1 11.6 17.4#

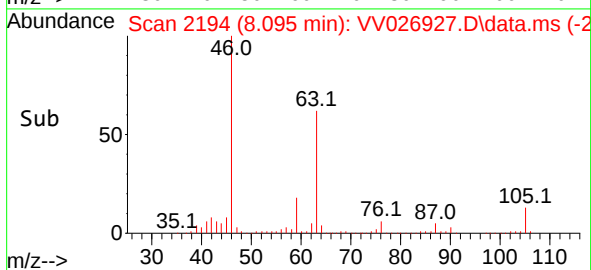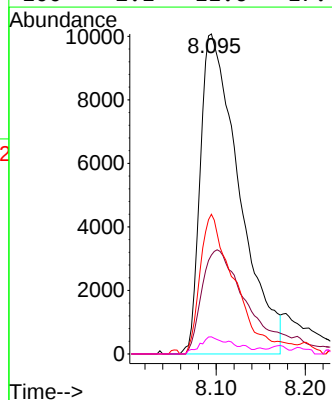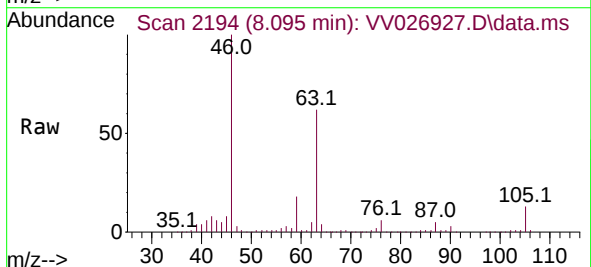

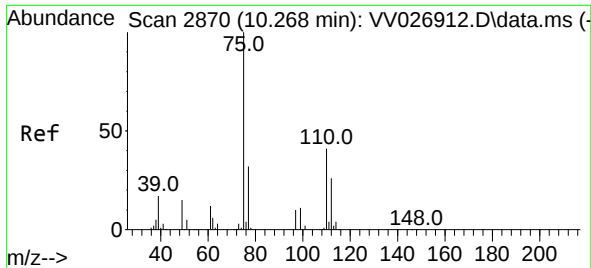

#61

1,2,3-Trichloropropane

Concen: 5.840 ug/L

RT: 11.252 min Scan# 31

Delta R.T. 0.984 min

Lab File: VV026927.D


Acq: 23 Jul 2022 17:15

Instrument :

MSVOA_V

ClientSampleId :

C0ZD6ME

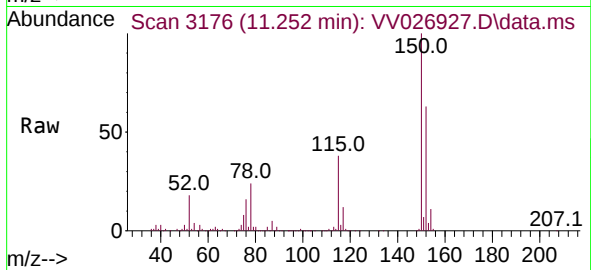

Tgt Ion: 75 Resp: 34447

Ion Ratio Lower Upper

75 100

77 31.9 25.6 38.4

110 2.4 31.7 47.5#

