




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026917.D
 Acq On : 23 Jul 2022 13:09
 Operator : SY/MD
 Sample : N3743-16ME
 Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

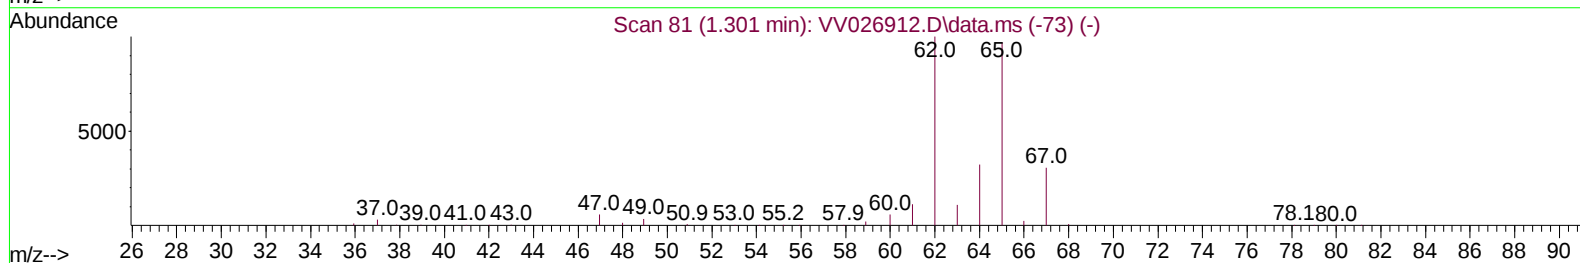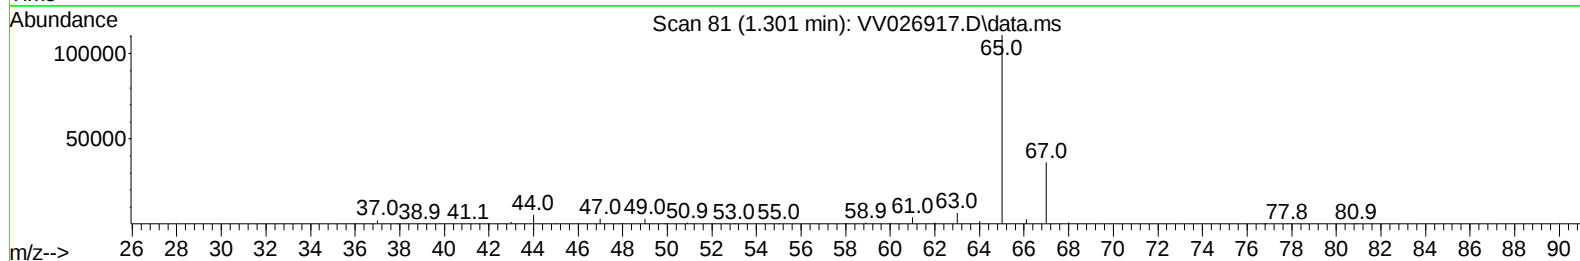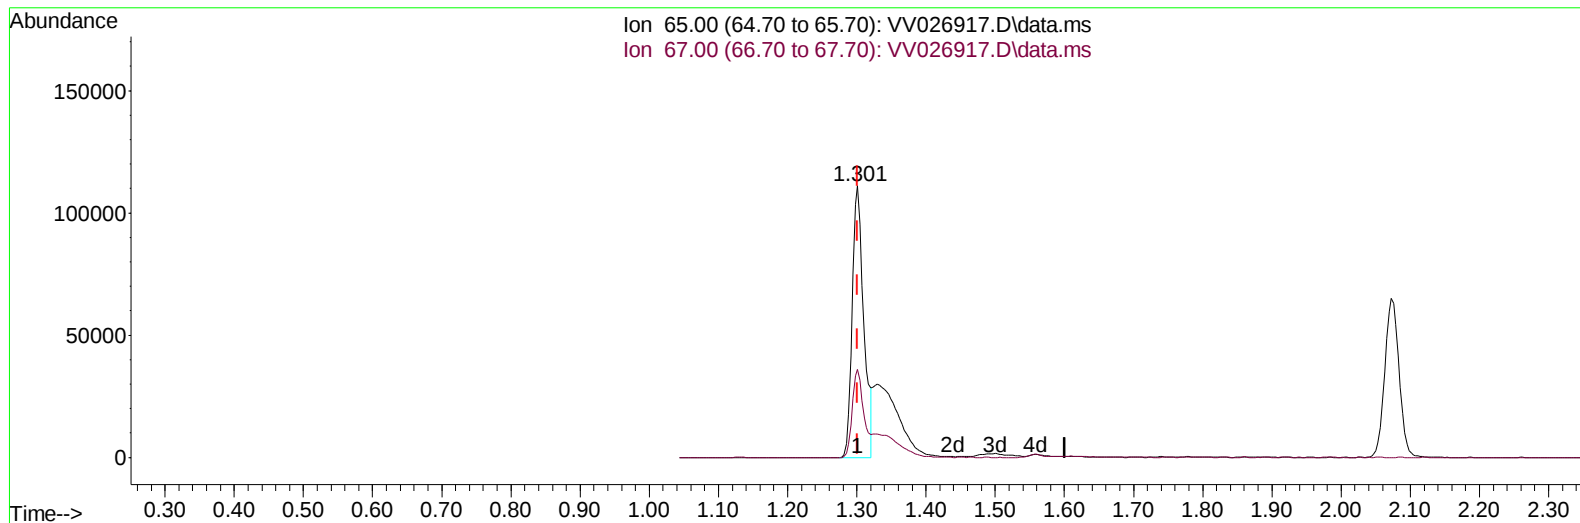

TIC: VV026917.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.301min (+ 0.000) 17.88 ug/L

response 128260

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.50	32.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026917.D
Acq On : 23 Jul 2022 13:09
Operator : SY/MD
Sample : N3743-16ME
Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

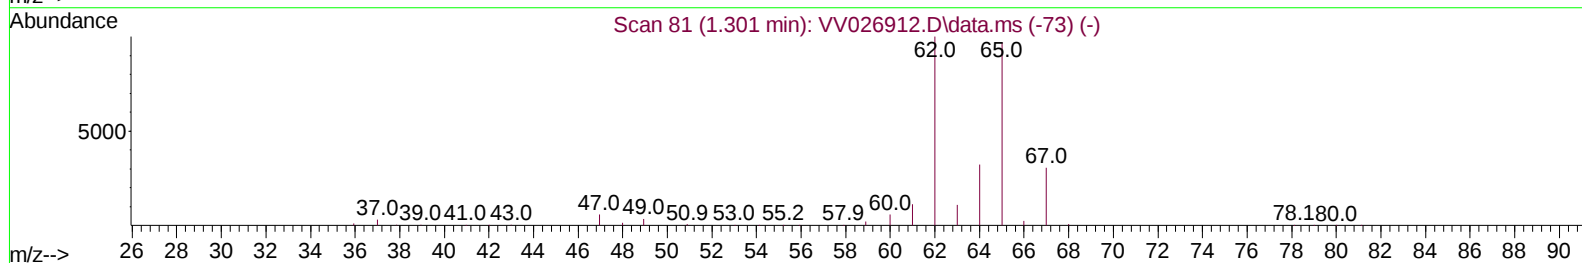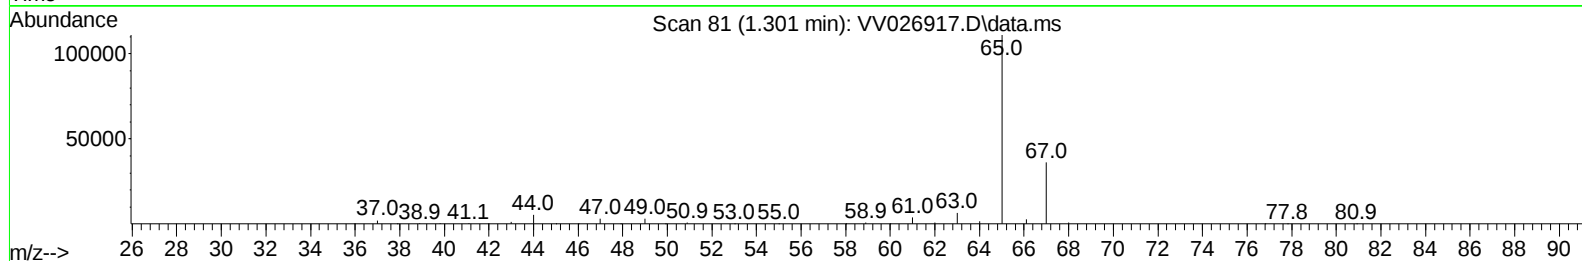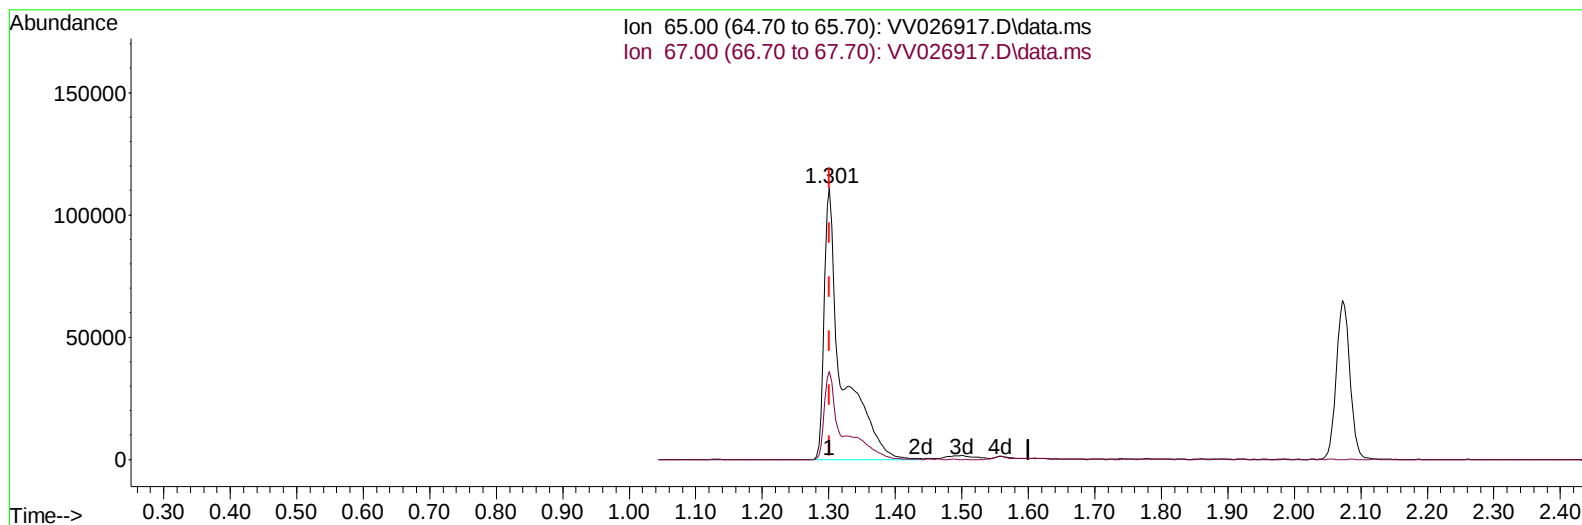

TIC: VV026917.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.301min (+ 0.000) 28.75 ug/L m

response 206180

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.50	20.31#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026917.D
 Acq On : 23 Jul 2022 13:09
 Operator : SY/MD
 Sample : N3743-16ME
 Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

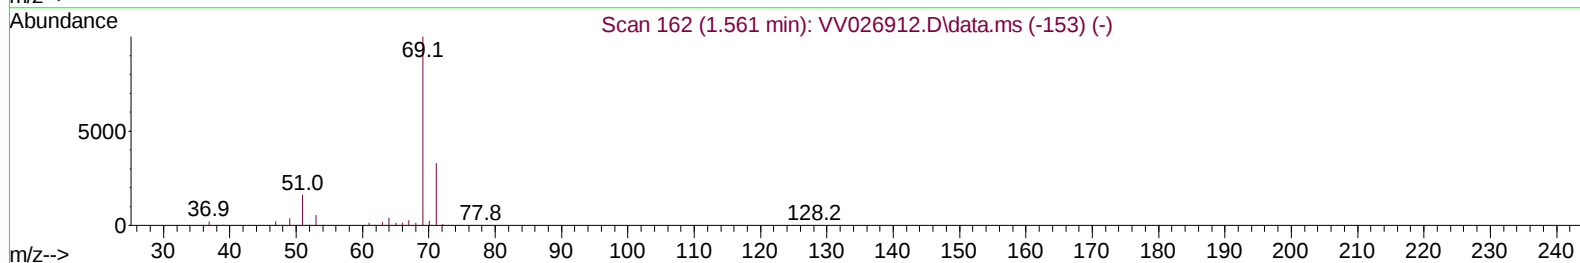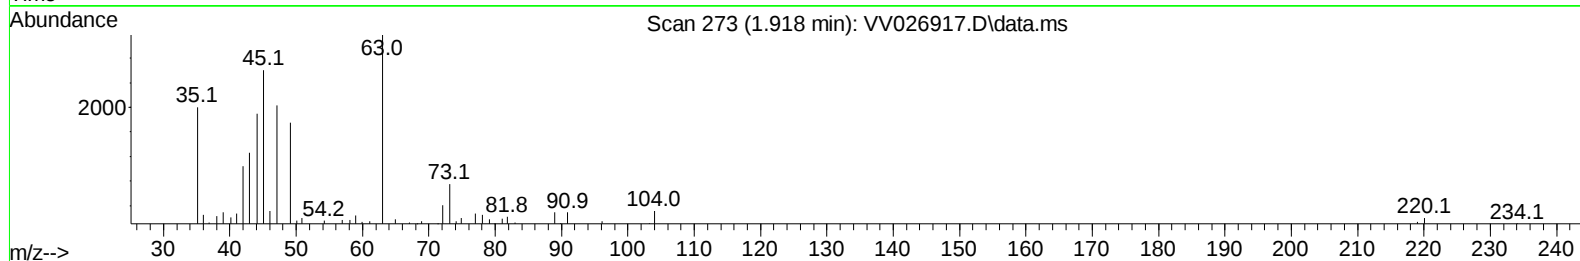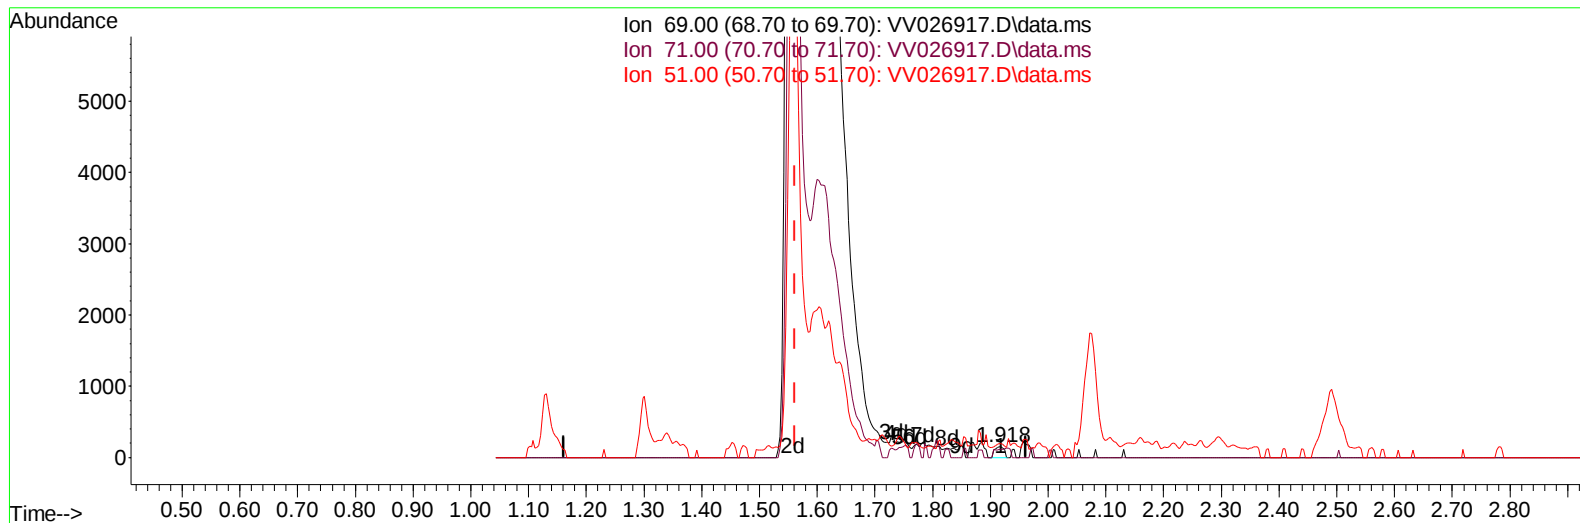

TIC: VV026917.D\data.ms

(7) Chloroethane-d5 (S)

1.918min (+ 0.357) 0.03 ug/L

response 175

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	23.43
51.00	23.00	25.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026917.D
 Acq On : 23 Jul 2022 13:09
 Operator : SY/MD
 Sample : N3743-16ME
 Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

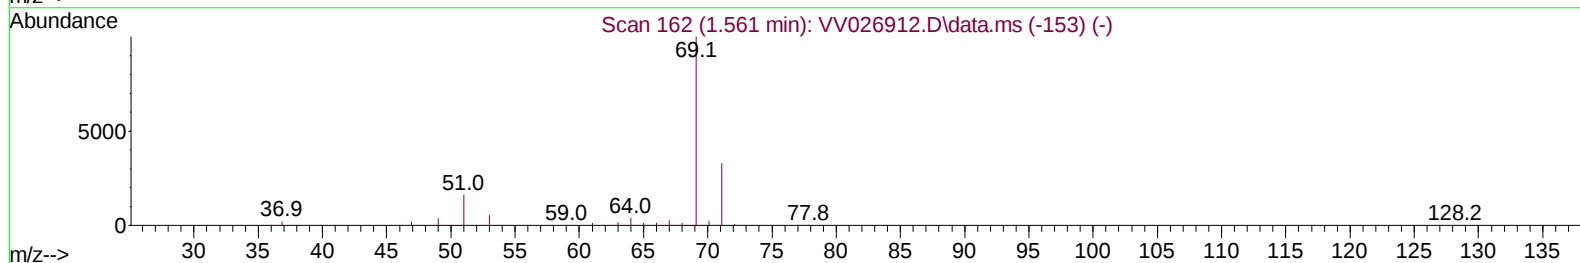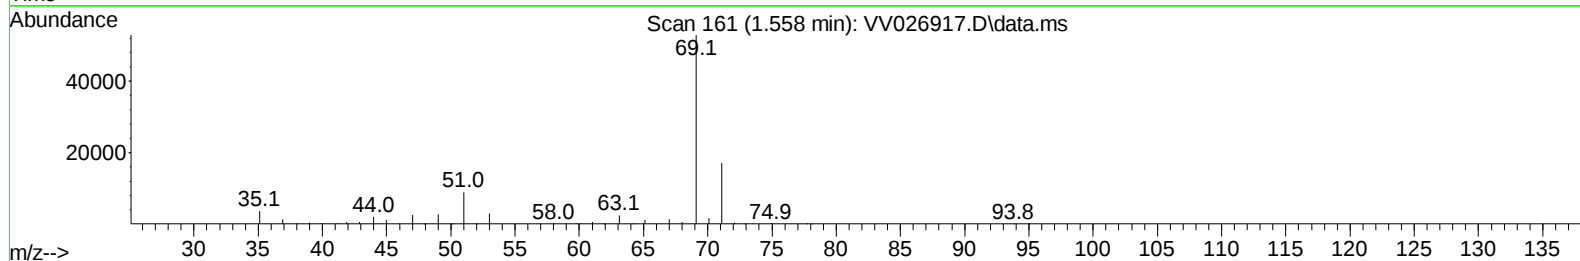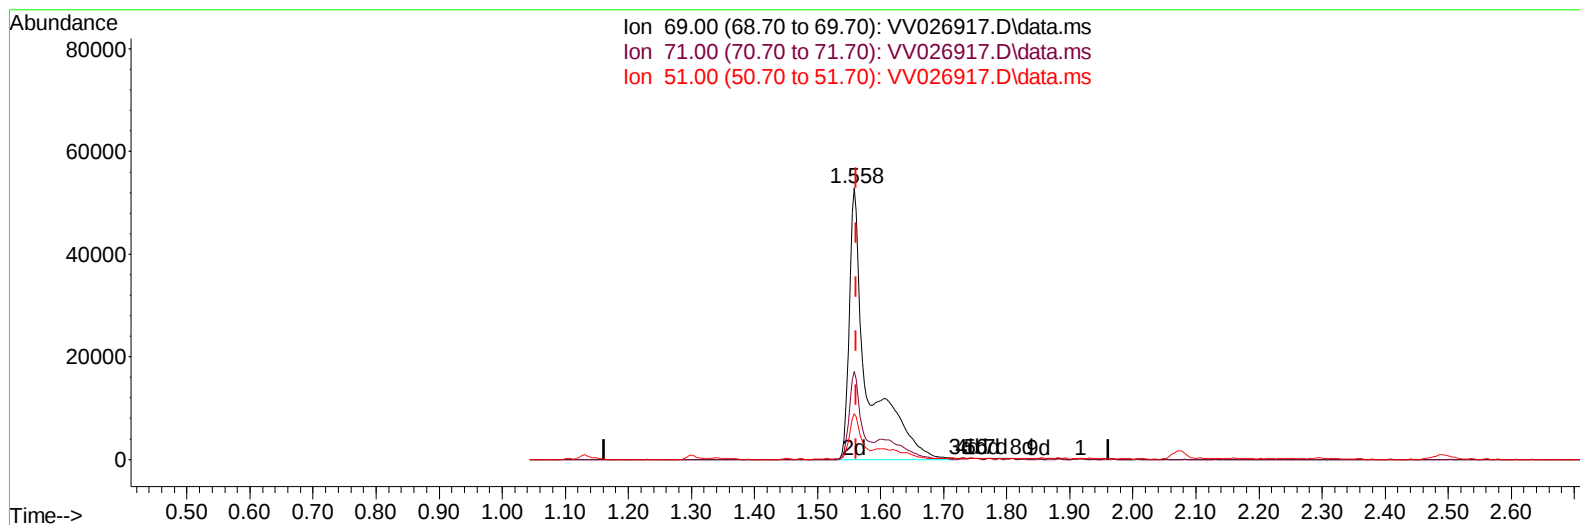

TIC: VV026917.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 18.83 ug/L m

response 109279

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	0.04#
51.00	23.00	0.04#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026917.D
 Acq On : 23 Jul 2022 13:09
 Operator : SY/MD
 Sample : N3743-16ME
 Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

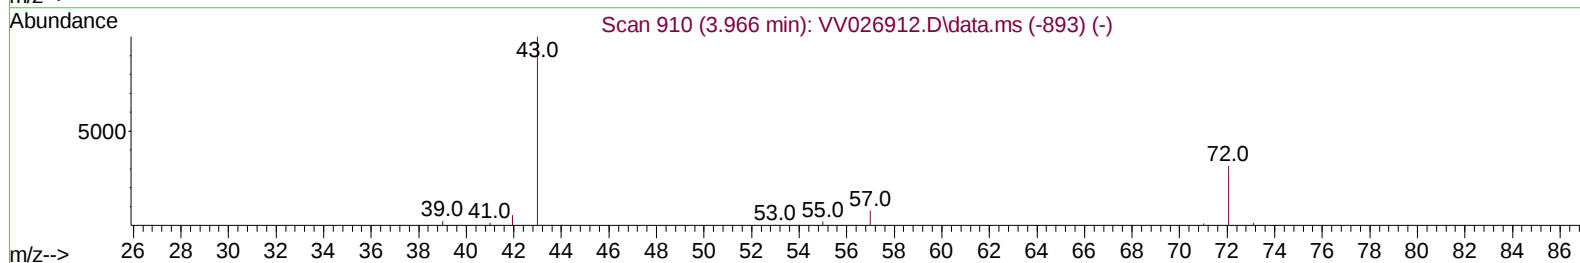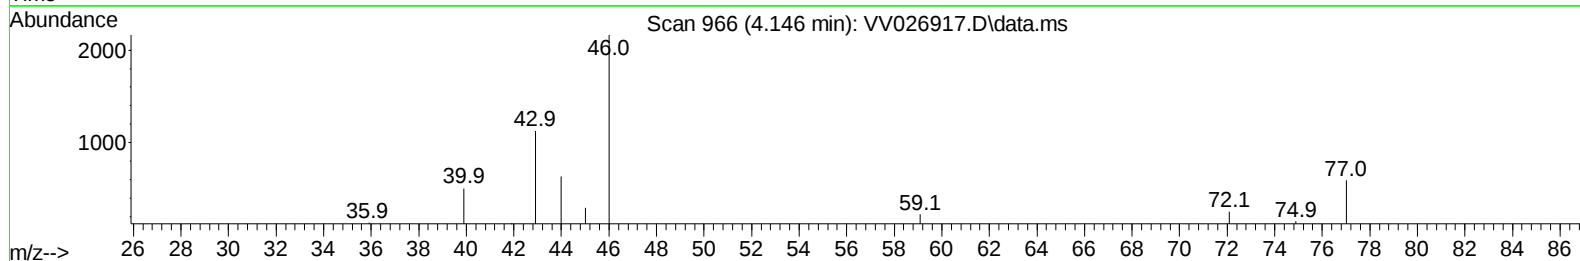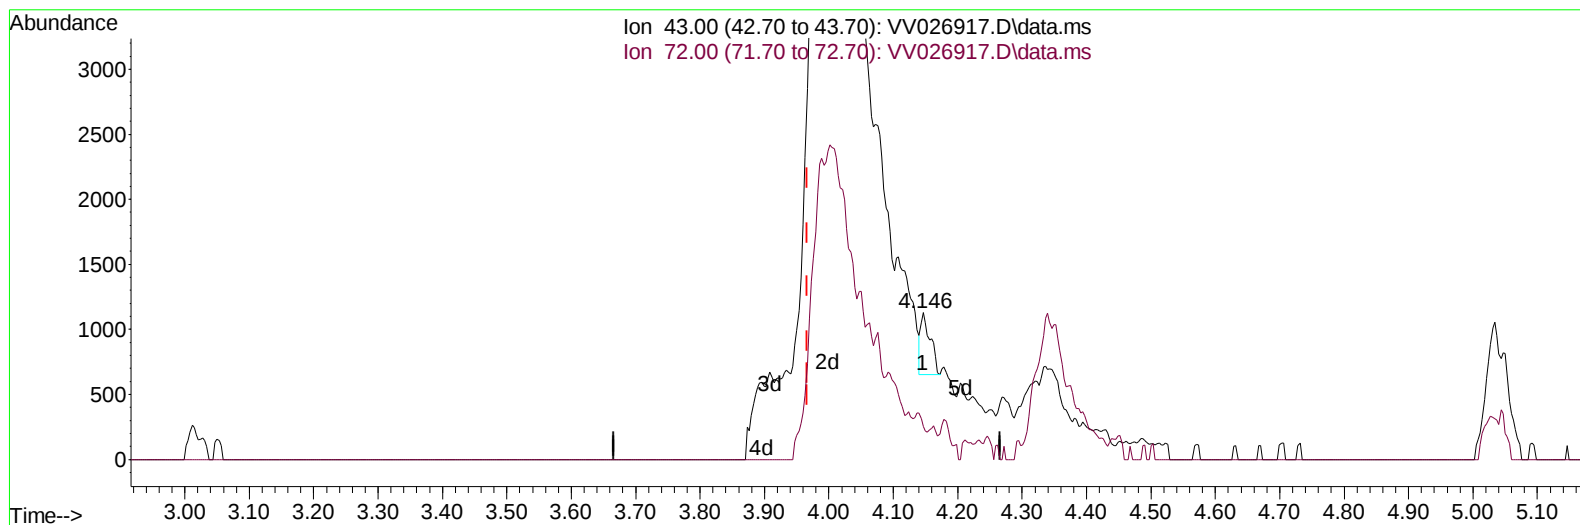

TIC: VV026917.D\data.ms

(22) 2-Butanone (T)

4.146min (+ 0.180) 0.11 ug/L

response 490

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	31.84
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026917.D
 Acq On : 23 Jul 2022 13:09
 Operator : SY/MD
 Sample : N3743-16ME
 Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

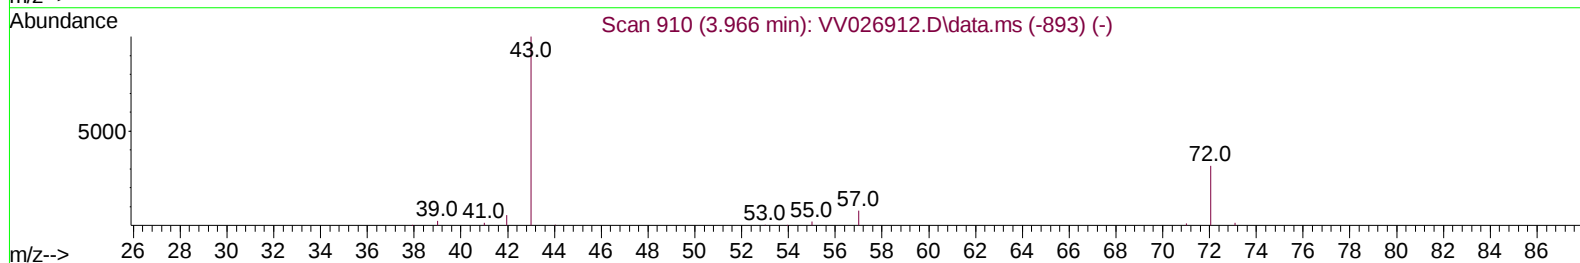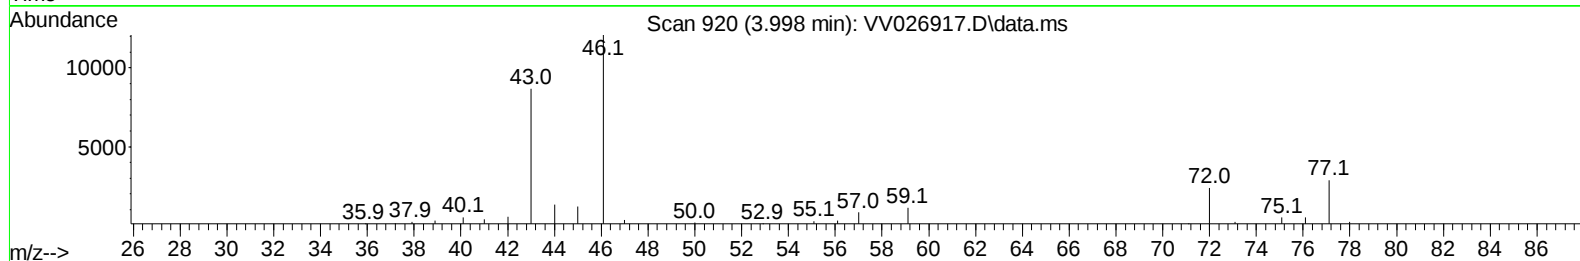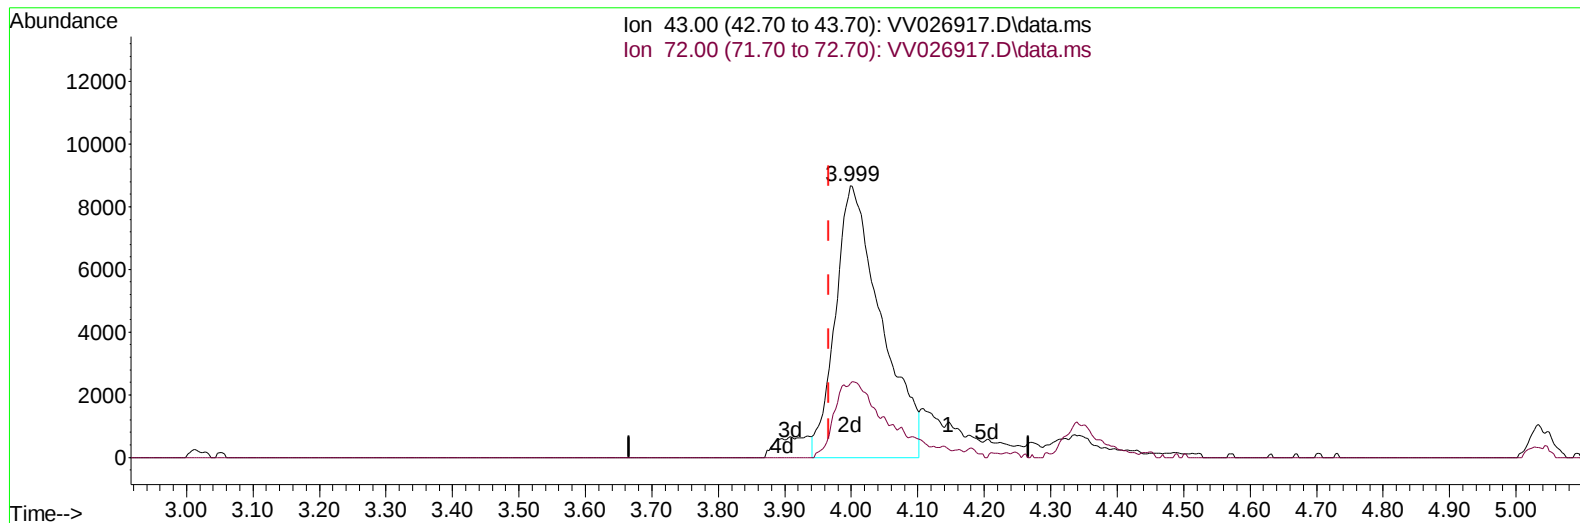

TIC: VV026917.D\data.ms

(22) 2-Butanone (T)

3.998min (+ 0.032) 8.94 ug/L m

response 41387

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	0.38#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026917.D
 Acq On : 23 Jul 2022 13:09
 Operator : SY/MD
 Sample : N3743-16ME
 Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	855184	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	841224	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	368104	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	206180m	28.746	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	57.500%#	
7) Chloroethane-d5	1.558	69	109279m	18.833	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	37.660%#	
11) 1,1-Dichloroethene-d2	2.073	63	295658	22.912	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	45.820%#	
21) 2-Butanone-d5	3.899	46	383335	79.290	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	79.290%	
24) Chloroform-d	4.339	84	483547	34.255	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	68.520%#	
26) 1,2-Dichloroethane-d4	5.024	65	298966	37.026	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	74.060%	
32) Benzene-d6	5.037	84	975034	38.344	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	76.680%	
36) 1,2-Dichloropropane-d6	6.063	67	321671	39.254	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	78.500%	
41) Toluene-d8	7.310	98	802021	36.048	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	72.100%#	
43) trans-1,3-Dichloroprop...	7.619	79	126292	36.781	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	73.560%	
47) 2-Hexanone-d5	8.095	63	281201	78.810	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	78.810%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	452397	36.341	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	72.680%	
66) 1,2-Dichlorobenzene-d4	11.625	152	302016	43.733	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	87.460%	
Target Compounds						
20) cis-1,2-Dichloroethene	3.899	96	6318	0.858	ug/L	94
22) 2-Butanone	3.998	43	41387m	8.939	ug/L	
46) Tetrachloroethene	7.973	164	13076	2.411	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026917.D
Acq On : 23 Jul 2022 13:09
Operator : SY/MD
Sample : N3743-16ME
Misc : 6.43g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D14ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:08:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

