




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026924.D
 Acq On : 23 Jul 2022 16:01
 Operator : SY/MD
 Sample : N3745-02ME
 Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

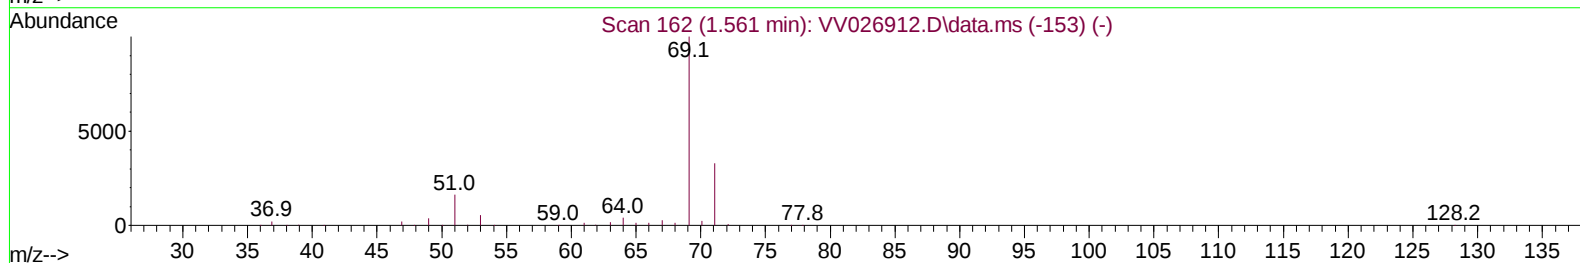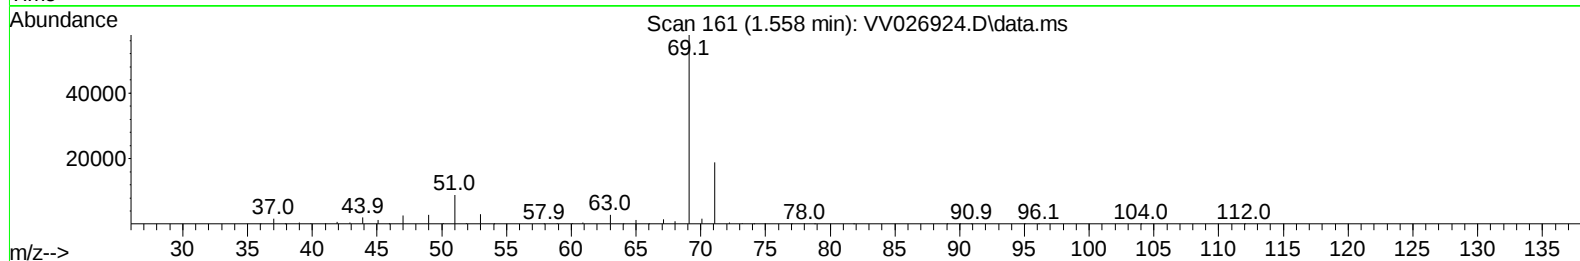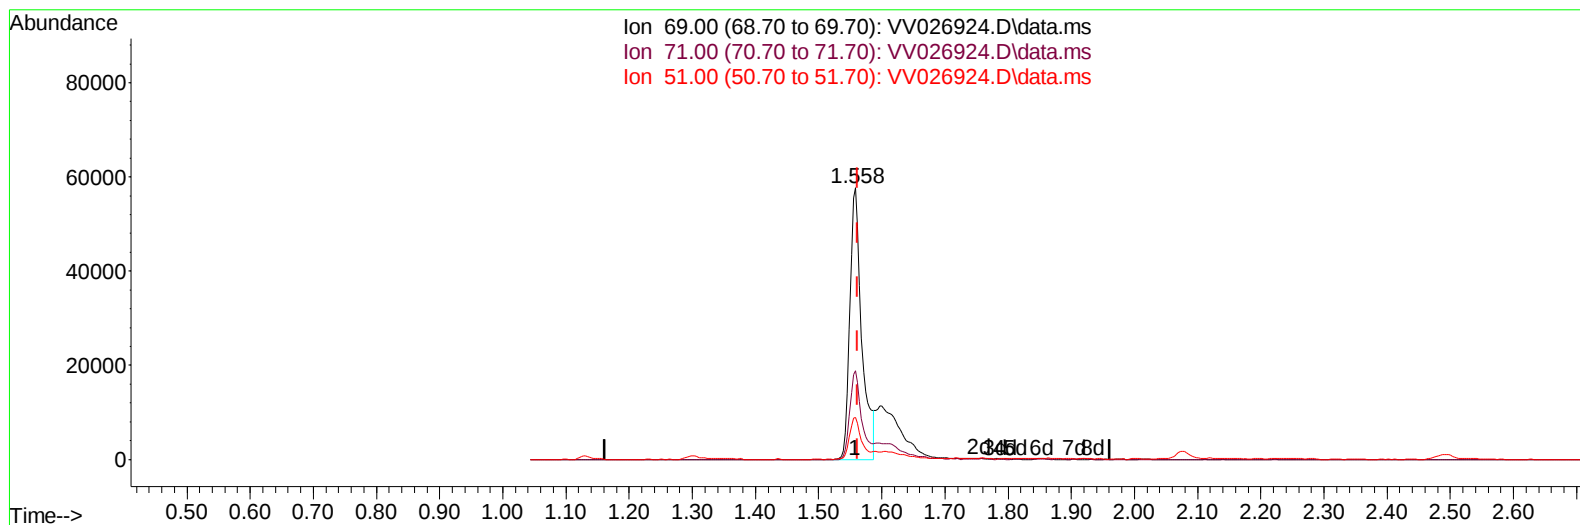

TIC: VV026924.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 15.59 ug/L

response 76365

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	33.07
51.00	23.00	15.12#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026924.D
 Acq On : 23 Jul 2022 16:01
 Operator : SY/MD
 Sample : N3745-02ME
 Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

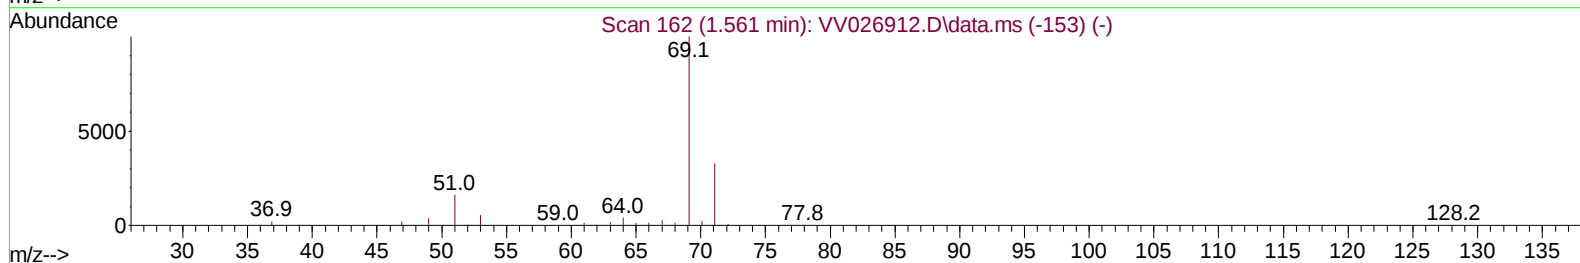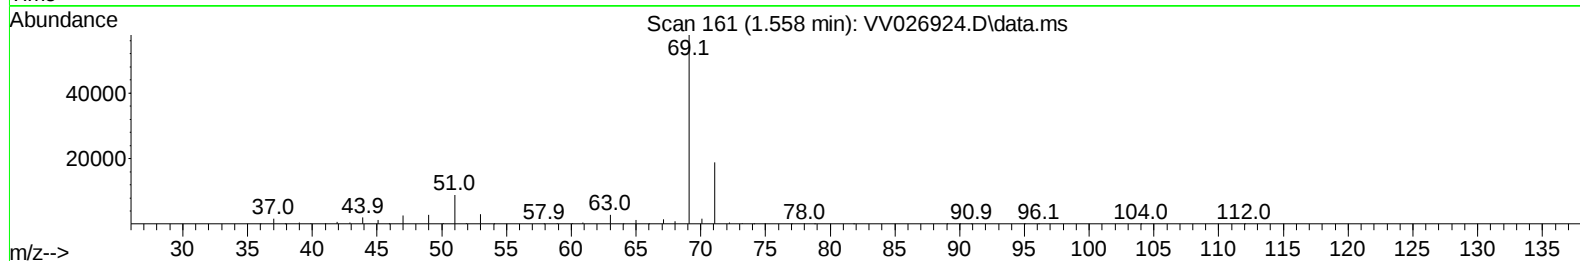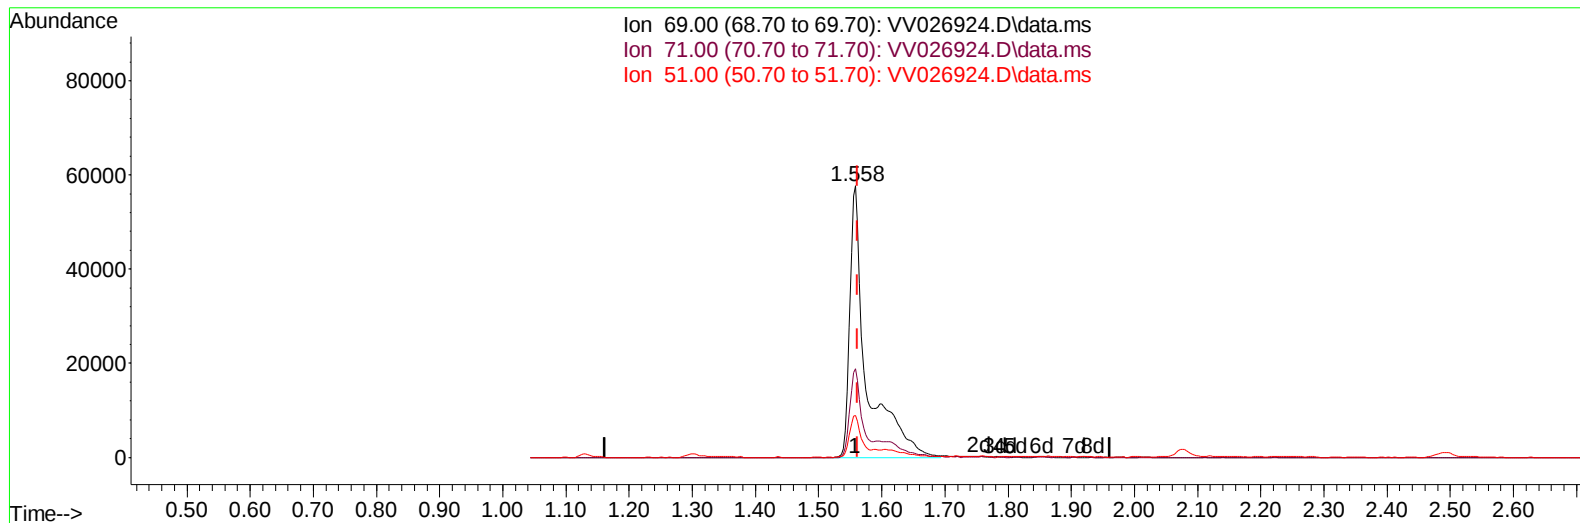

TIC: VV026924.D\data.ms

(7) Chloroethane-d5 (S)

1.558min (-0.003) 22.07 ug/L m

response 108131

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	23.36
51.00	23.00	10.68#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026924.D
 Acq On : 23 Jul 2022 16:01
 Operator : SY/MD
 Sample : N3745-02ME
 Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

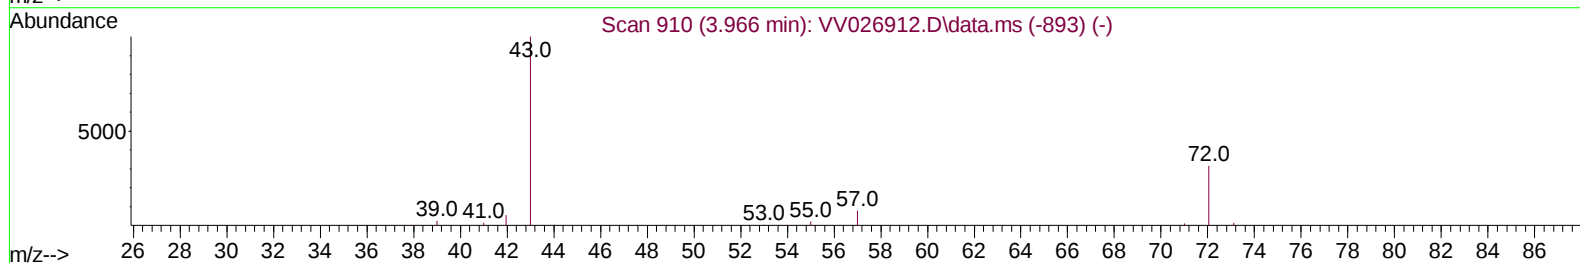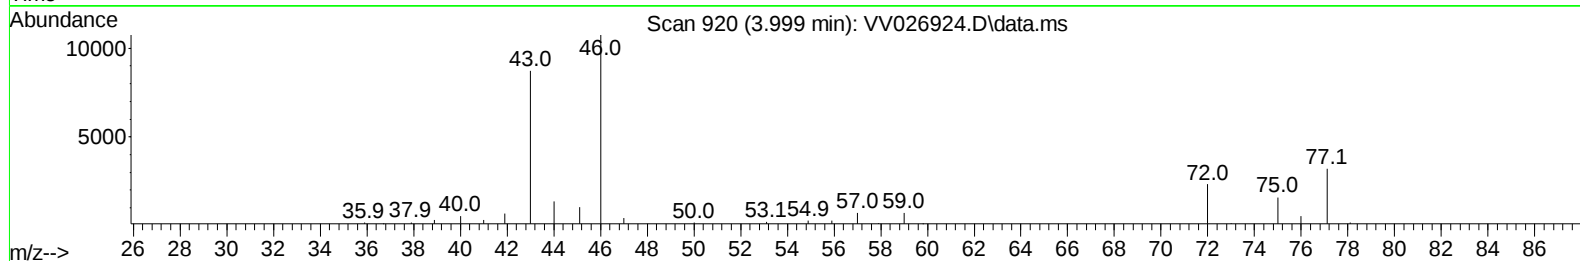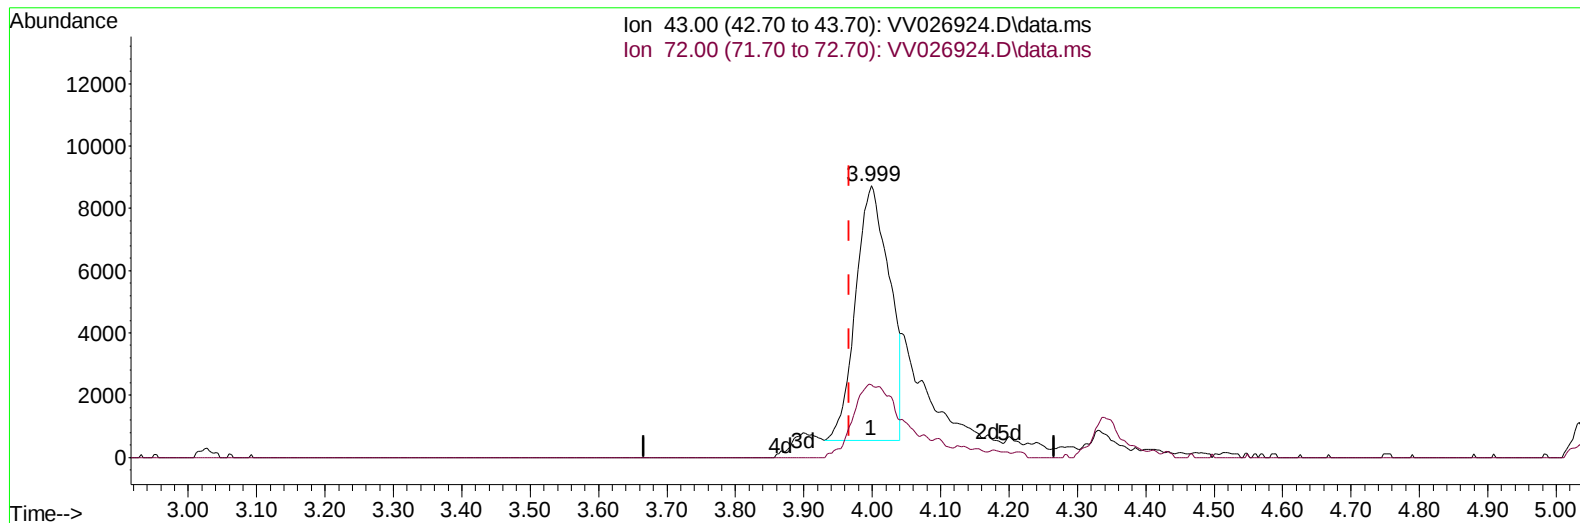

TIC: VV026924.D\data.ms

(22) 2-Butanone (T)

3.999min (+ 0.032) 7.15 ug/L

response 27941

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	15.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026924.D
 Acq On : 23 Jul 2022 16:01
 Operator : SY/MD
 Sample : N3745-02ME
 Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

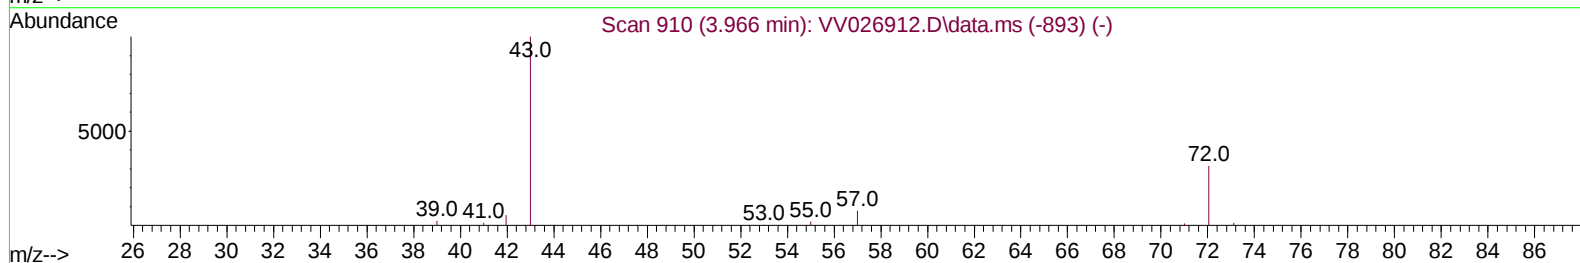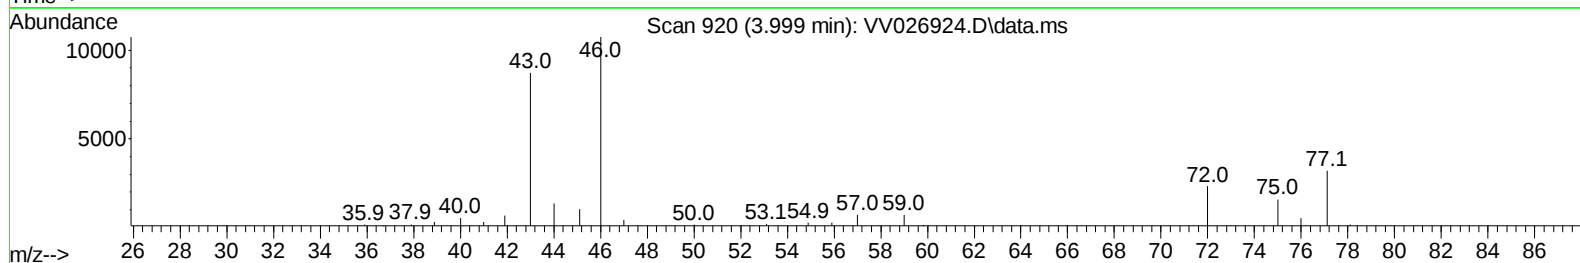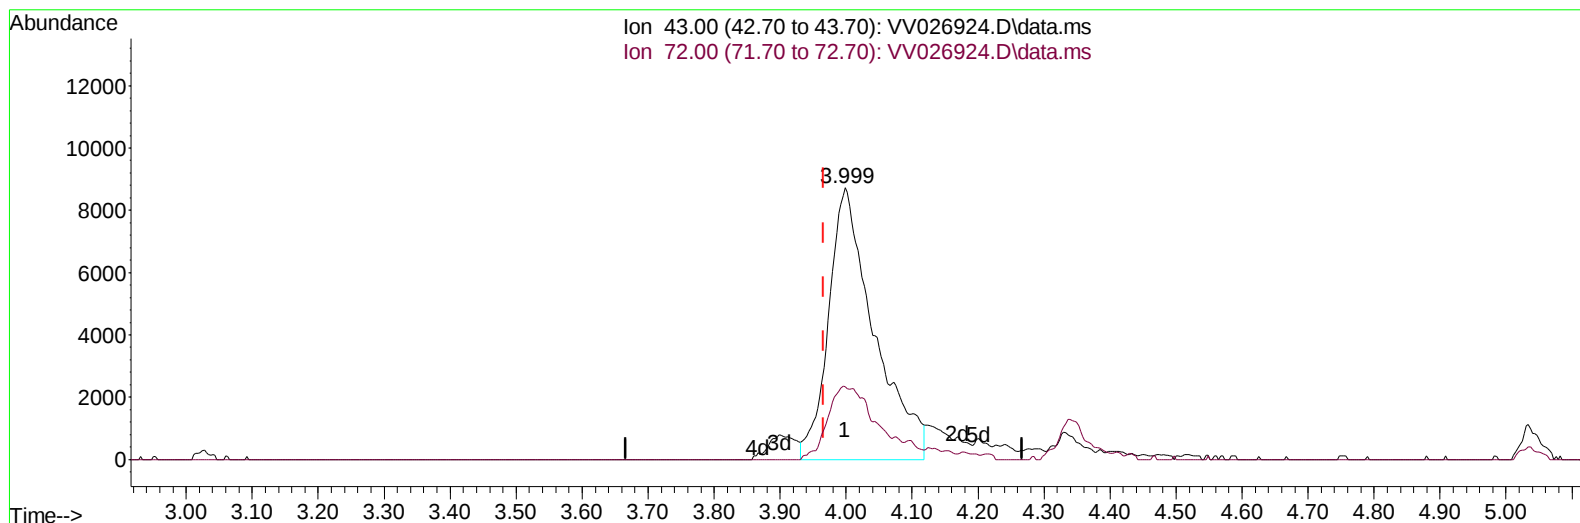

TIC: VV026924.D\data.ms

(22) 2-Butanone (T)

3.999min (+ 0.032) 10.66 ug/L m

response 41680

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.70	10.25#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
 Data File : VV026924.D
 Acq On : 23 Jul 2022 16:01
 Operator : SY/MD
 Sample : N3745-02ME
 Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5D06ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM07222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 25 02:02:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.609	114		722061	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		705088	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152		310402	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		201095	33.206	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	66.420%	
7) Chloroethane-d5	1.558	69		108131m	22.071	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	44.140%#	
11) 1,1-Dichloroethene-d2	2.076	63		296184	27.185	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125		Recovery	=	54.360%#	
21) 2-Butanone-d5	3.896	46		391994	96.030	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130		Recovery	=	96.030%	
24) Chloroform-d	4.339	84		494132	41.459	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	82.920%	
26) 1,2-Dichloroethane-d4	5.021	65		301515	44.226	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	88.460%	
32) Benzene-d6	5.037	84		988095	46.360	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	92.720%	
36) 1,2-Dichloropropane-d6	6.063	67		326972	47.605	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	95.200%	
41) Toluene-d8	7.310	98		819011	43.919	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	87.840%	
43) trans-1,3-Dichloroprop...	7.619	79		123331	42.853	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	85.700%	
47) 2-Hexanone-d5	8.095	63		292305	97.739	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	97.740%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84		462880	44.362	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	88.720%	
66) 1,2-Dichlorobenzene-d4	11.625	152		307547	52.813	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	105.620%	
Target Compounds							
22) 2-Butanone	3.999	43		41680m	10.662	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072322\
Data File : VV026924.D
Acq On : 23 Jul 2022 16:01
Operator : SY/MD
Sample : N3745-02ME
Misc : 6.79g/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5D06ME

Manual IntegrationsAPPROVED

Quant Time: Jul 25 02:09:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072222WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 25 02:02:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

